


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062017\
 Data File : BF096042.D
 Acq On : 20 Jun 2017 13:29
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 16:05:47 2017

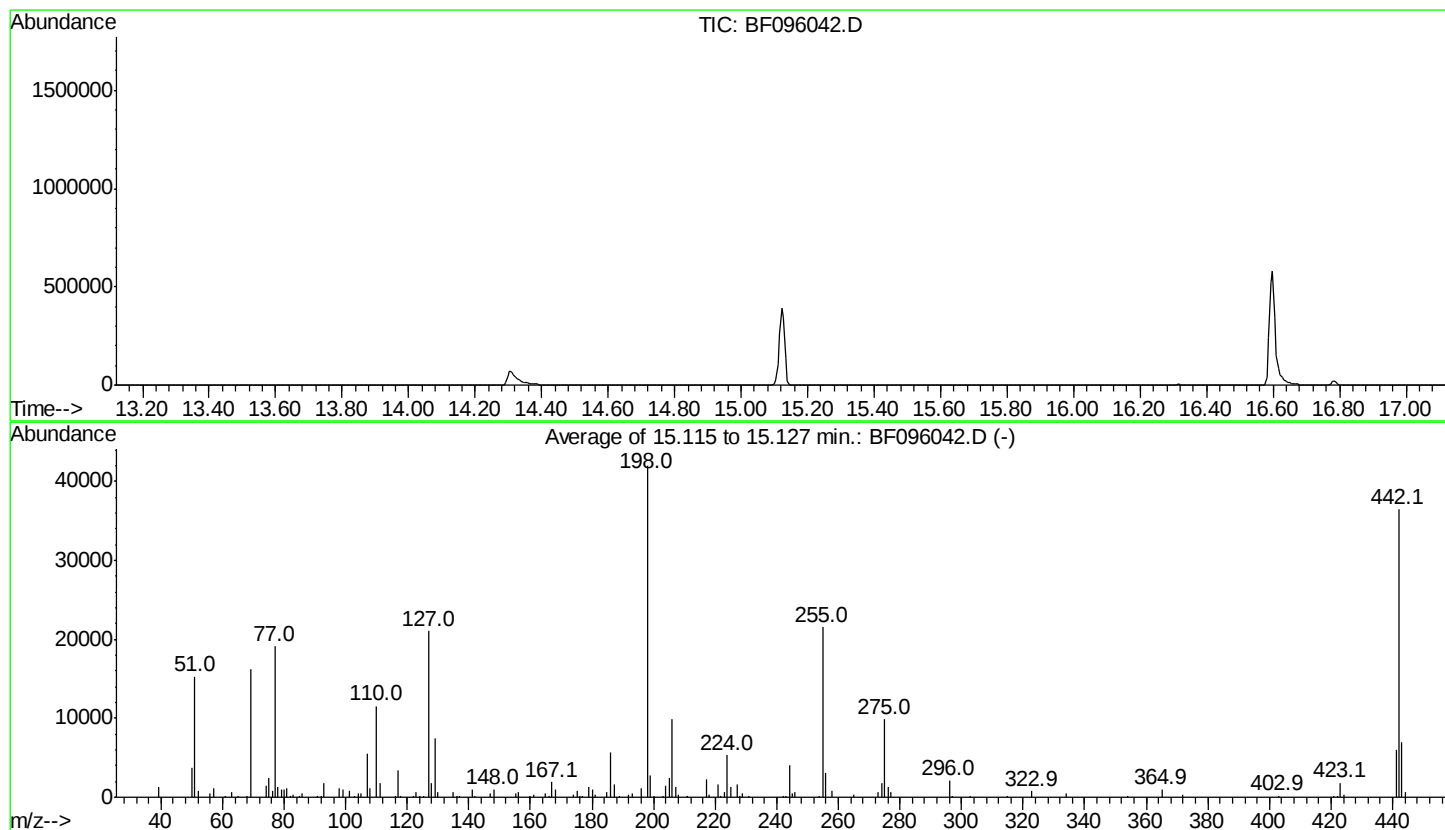

AutoFind: Scans 2317, 2318, 2319; Background Corrected with Scan 2311

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	15261	PASS
68	69	0.00	2	0.8	124	PASS
69	198	0.00	100	38.5	16179	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.1	21026	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41997	PASS
199	198	5	9	6.7	2823	PASS
275	198	10	60	23.4	9834	PASS
365	198	1	100	2.3	972	PASS
441	442	0.01	24	16.5	6013	PASS
442	198	50	100	86.8	36437	PASS
443	442	15	24	19.2	6995	PASS