


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062017\
 Data File : BF096064.D
 Acq On : 21 Jun 2017 2:41
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 16:05:47 2017

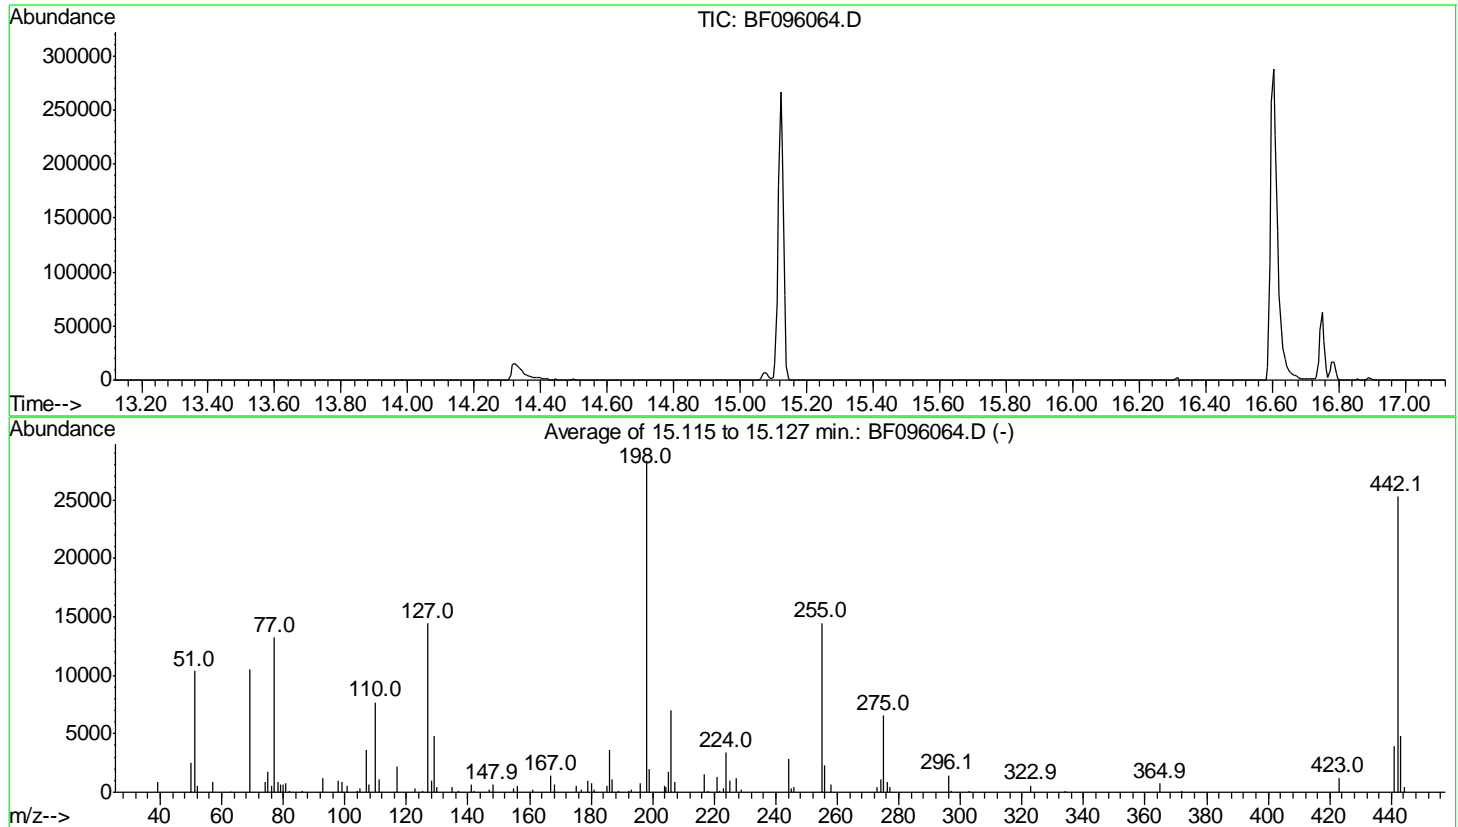

AutoFind: Scans 2317, 2318, 2319; Background Corrected with Scan 2311

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	10346	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.0	10498	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	14441	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28344	PASS
199	198	5	9	7.0	1988	PASS
275	198	10	60	23.1	6535	PASS
365	198	1	100	2.6	724	PASS
441	442	0.01	24	15.6	3935	PASS
442	198	50	100	89.1	25252	PASS
443	442	15	24	18.9	4780	PASS