

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062018\
 Data File : BF106645.D
 Acq On : 21 Jun 2018 2:49
 Operator : JU/SJ
 Sample : J3554-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 A-3(5.0)

Quant Time: Jun 21 04:56:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 19 14:32:09 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	83780	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	302069	20.00	ng	0.00
38) Acenaphthene-d10	10.00	164	139139	20.00	ng	0.00
63) Phenanthrene-d10	11.49	188	239282	20.00	ng	0.00
75) Chrysene-d12	14.14	240	257062	20.00	ng	-0.01
86) Perylene-d12	15.68	264	202450	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	577132	116.65	ng	0.00
7) Phenol-d6	6.61	99	727546	117.75	ng	0.00
23) Nitrobenzene-d5	7.52	82	481305	88.55	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	197396	122.40	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	782483	97.33	ng	0.00
78) Terphenyl-d14	13.08	244	826825	77.91	ng	0.00
Target Compounds						
10) Phenol	6.62	94	14255	2.022	ng	92
49) Dimethylphthalate	9.71	163	180294	17.277	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062018\
Data File : BF106645.D
Acq On : 21 Jun 2018 2:49
Operator : JU/SJ
Sample : J3554-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A-3(5.0)

Quant Time: Jun 21 04:56:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 19 14:32:09 2018
Response via : Initial Calibration

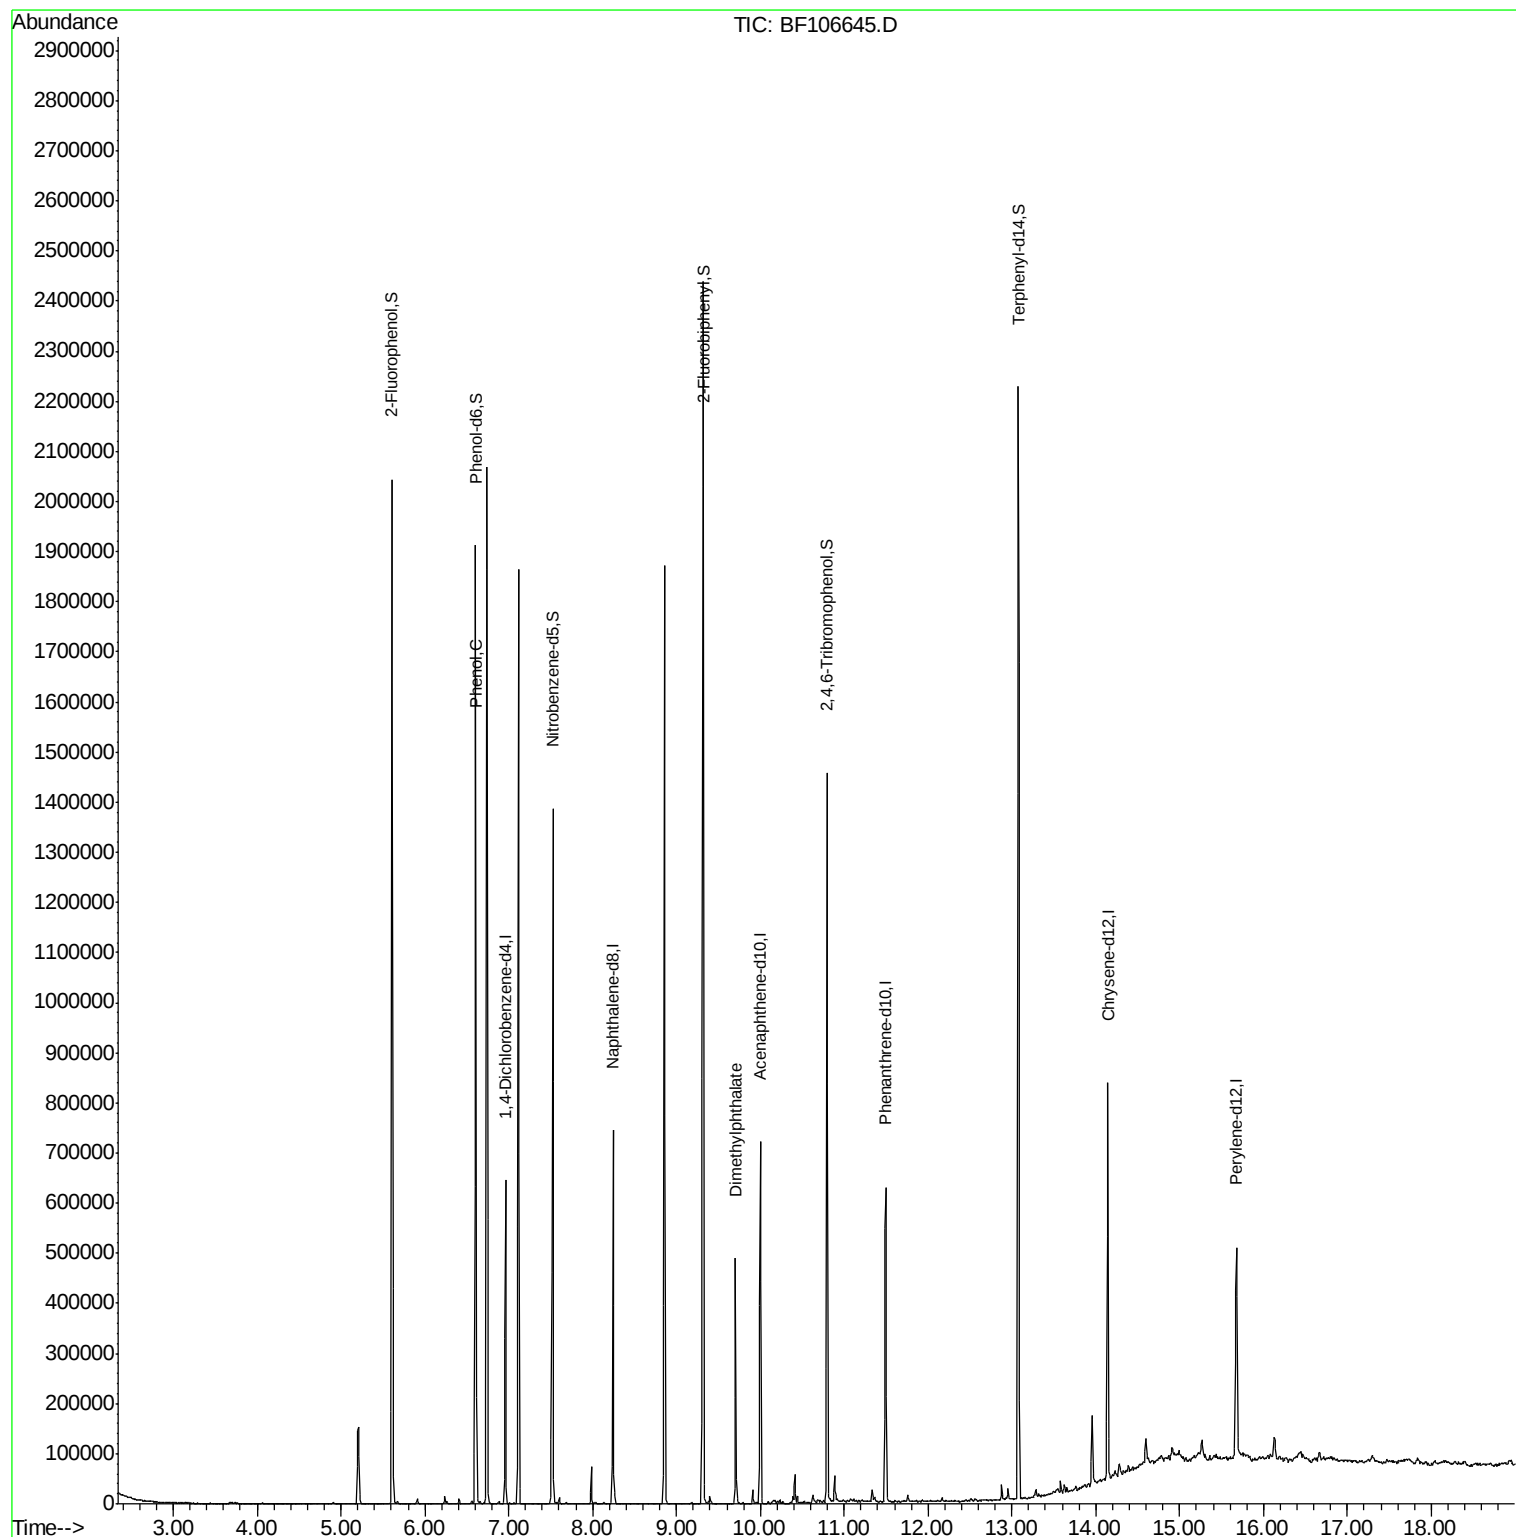




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.96 min Scan# 786
 Delta R.T. 0.00 min
 Lab File: BF106645.D
 Acq: 21 Jun 2018 2:49

Instrument :
 BNA_F
 ClientSampled :
 A-3(5.0)

Tot Ion:152 Resp: 83780
 Ion Ratio Lower Upper
 152 100
 150 157.6 124.6 186.8
 115 61.1 50.1 75.1

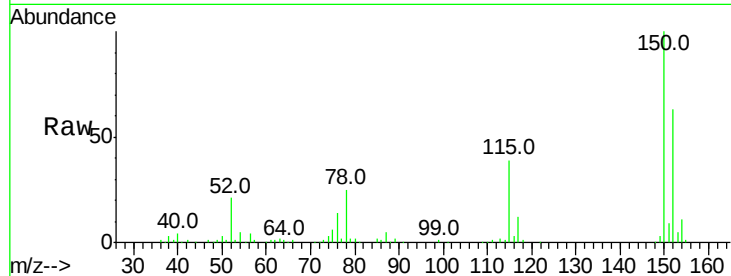


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

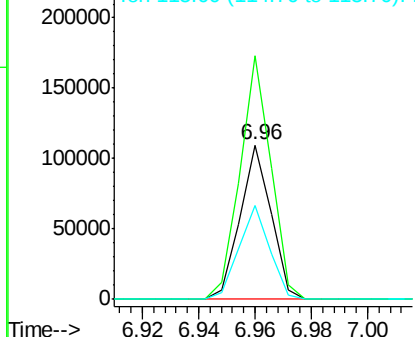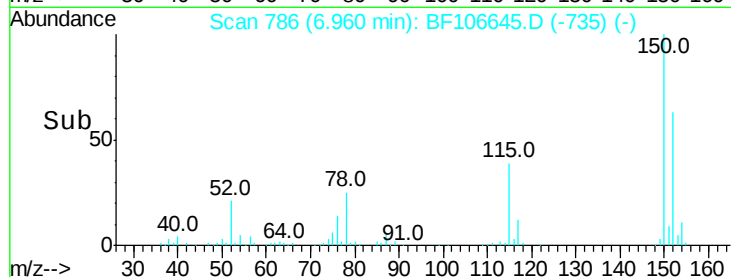



#5

2-Fluorophenol
 Concen: 116.647 ng
 RT: 5.61 min Scan# 556
 Delta R.T. 0.01 min
 Lab File: BF106645.D
 Acq: 21 Jun 2018 2:49

Tgt Ion:112 Resp: 577132
 Ion Ratio Lower Upper
 112 100
 64 59.8 47.9 71.9
 63 30.0 23.7 35.5

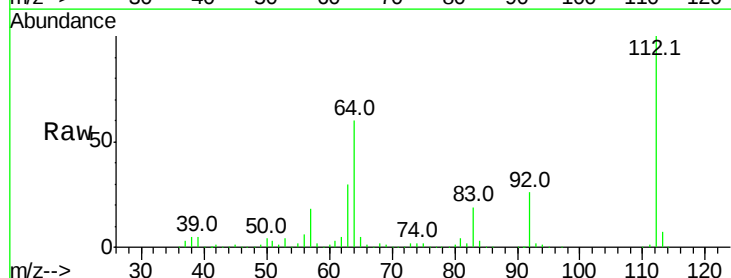

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

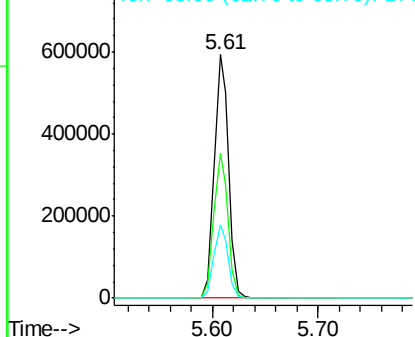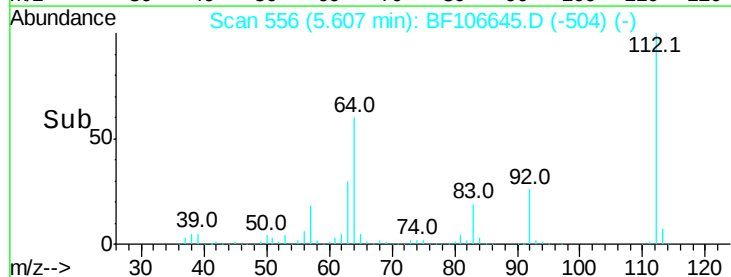



#7

Phenol-d6

Concen: 117.751 ng

RT: 6.61 min Scan# 726

Delta R.T. 0.00 min

Lab File: BF106645.D

Acq: 21 Jun 2018 2:49

Instrument :

BNA_F

ClientSampleId :

A-3(5.0)


Tot Ion: 99 Resp: 727546

Ion Ratio Lower Upper




99 100

42 17.3 14.5 21.7

71 35.1 25.4 38.0

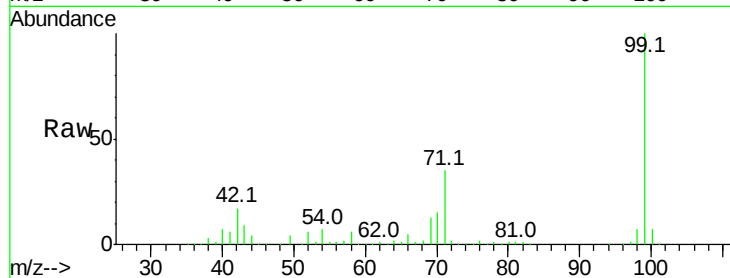

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

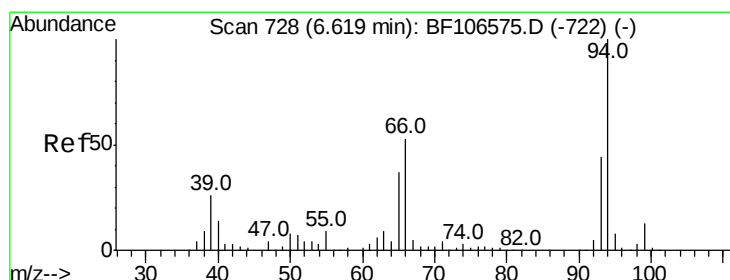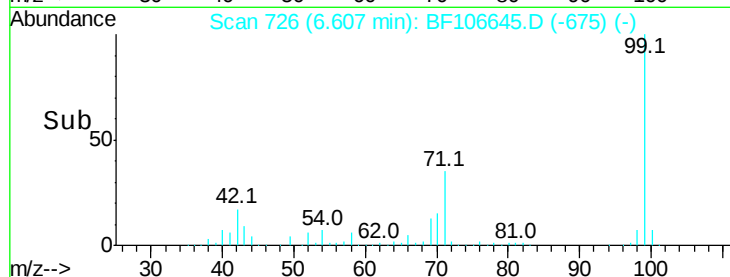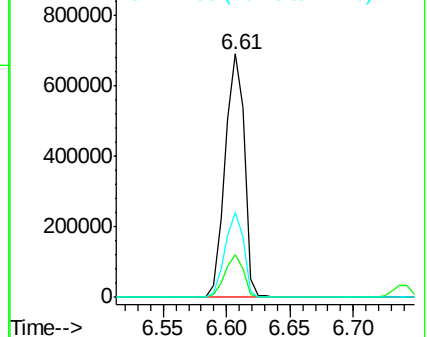

#10

Phenol

Concen: 2.022 ng

RT: 6.62 min Scan# 728

Delta R.T. 0.00 min

Lab File: BF106645.D

Acq: 21 Jun 2018 2:49


Tgt Ion: 94 Resp: 14255

Ion Ratio Lower Upper



94 100

65 29.0 7.9 47.9

66 43.8 16.2 56.2

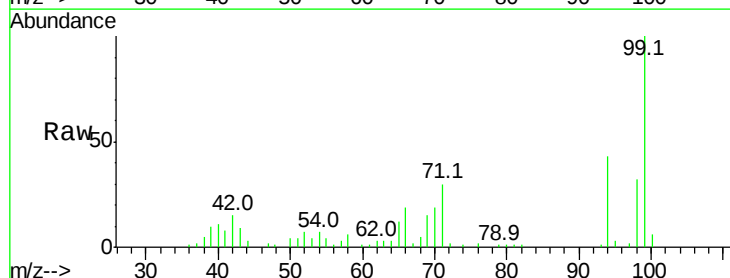

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

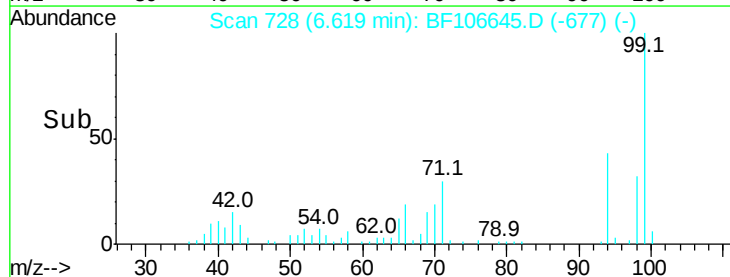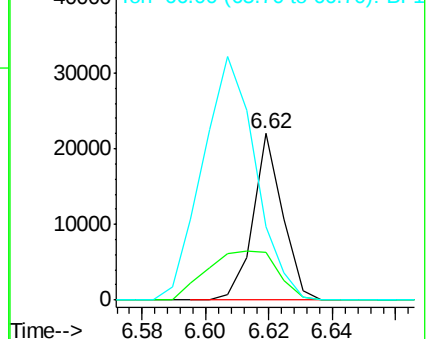



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.24 min Scan# 1004

Delta R.T. -0.01 min

Lab File: BF106645.D

Acq: 21 Jun 2018 2:49

Instrument :

BNA_F

ClientSampleId :

A-3(5.0)

Tot Ion:136 Resp: 302069



Ion Ratio Lower Upper

136 100

137 11.1 8.9 13.3

54 8.3 6.6 9.8

68 6.5 5.0 7.4

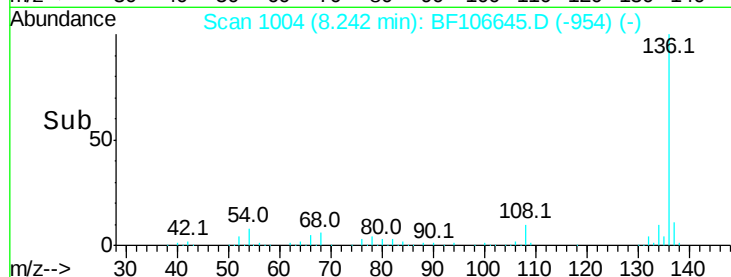
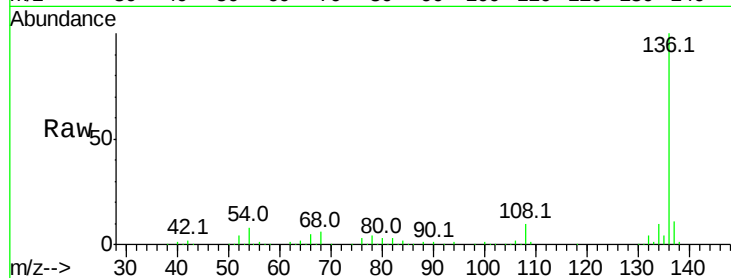


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

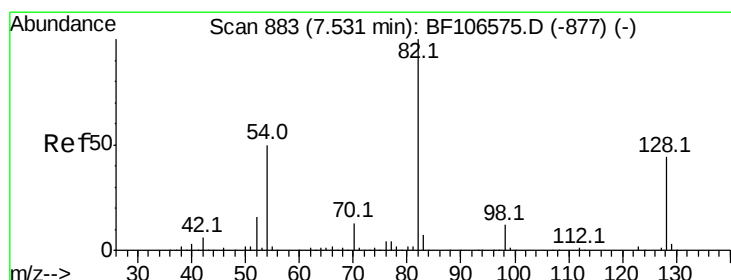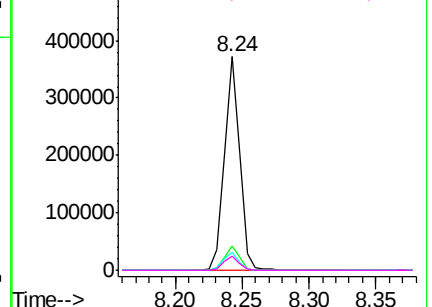

#23

Nitrobenzene-d5

Concen: 88.549 ng

RT: 7.52 min Scan# 882

Delta R.T. -0.01 min

Lab File: BF106645.D

Acq: 21 Jun 2018 2:49



Tgt Ion: 82 Resp: 481305

Ion Ratio Lower Upper

82 100

128 43.4 36.1 54.1


54 49.8 41.4 62.2

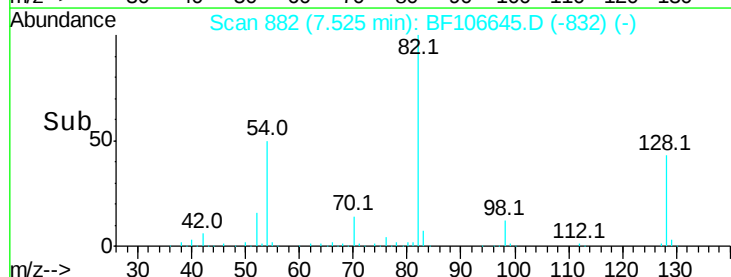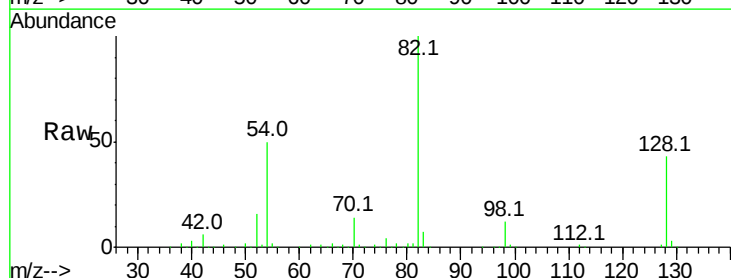

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1




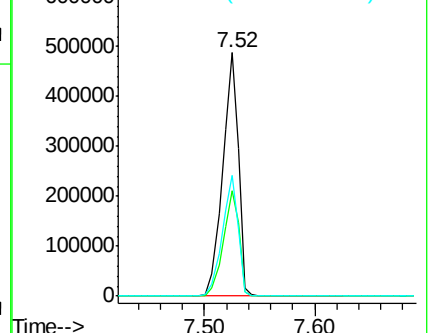




#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.00 min Scan# 1303
Delta R.T. -0.01 min
Lab File: BF106645.D
Acq: 21 Jun 2018 2:49




Instrument :
BNA_F
ClientSampleId :
A-3(5.0)

Tot Ion:164 Resp: 139139
Ion Ratio Lower Upper
164 100
162 96.7 86.1 129.1
160 44.4 38.3 57.5

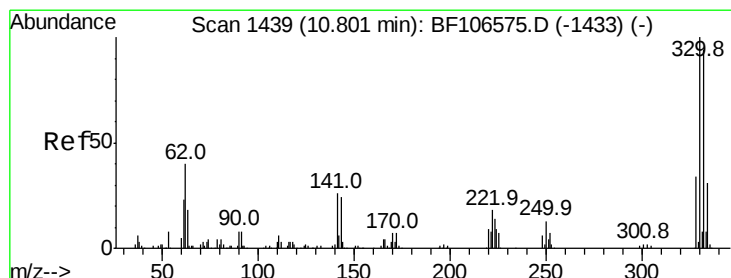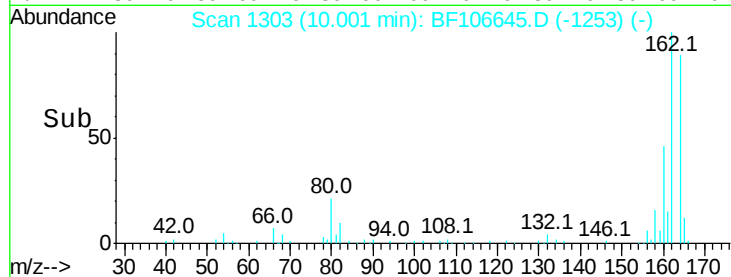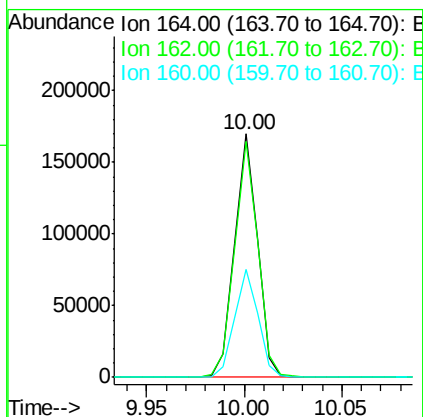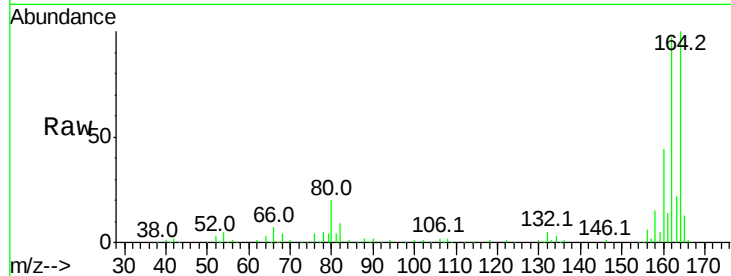

#41
2,4,6-Tribromophenol
Concen: 122.404 ng
RT: 10.80 min Scan# 1438
Delta R.T. -0.01 min
Lab File: BF106645.D
Acq: 21 Jun 2018 2:49

Tgt Ion:330 Resp: 197396
Ion Ratio Lower Upper
330 100
332 95.2 77.0 115.6
141 24.4 29.9 44.9#

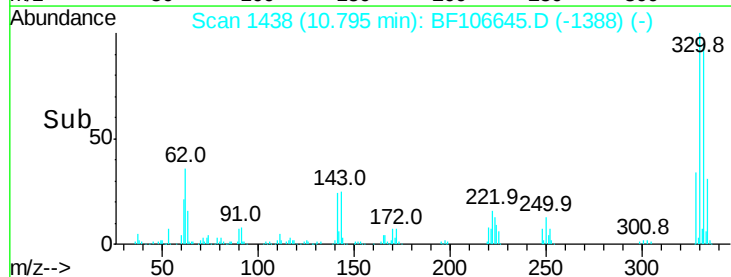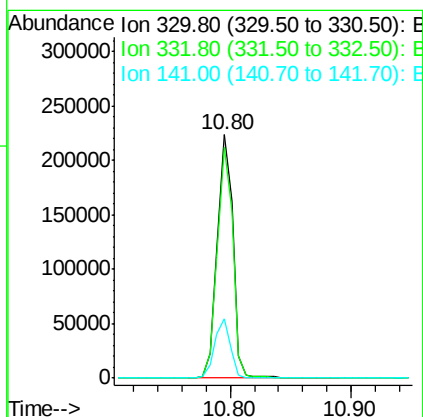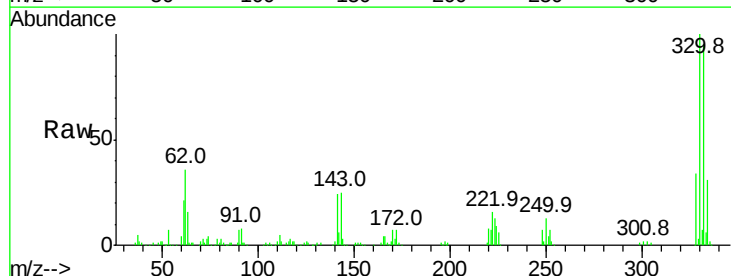







#44
2-Fluorobiphenyl
Concen: 97.329 ng
RT: 9.32 min Scan# 1187
Delta R.T. -0.01 min
Lab File: BF106645.D
Acq: 21 Jun 2018 2:49

Instrument :
BNA_F
ClientSampleId :
A-3(5.0)

Tot Ion:172 Resp: 782483
Ion Ratio Lower Upper
172 100
171 37.2 29.7 44.5
170 24.6 19.6 29.4

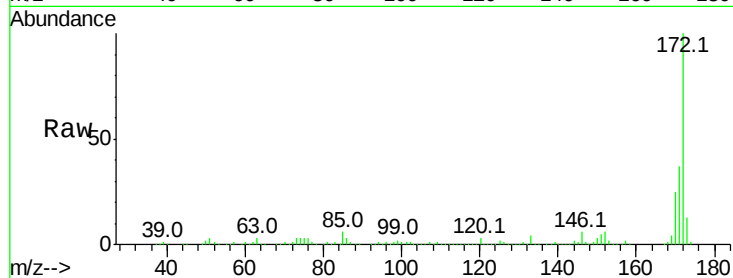


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

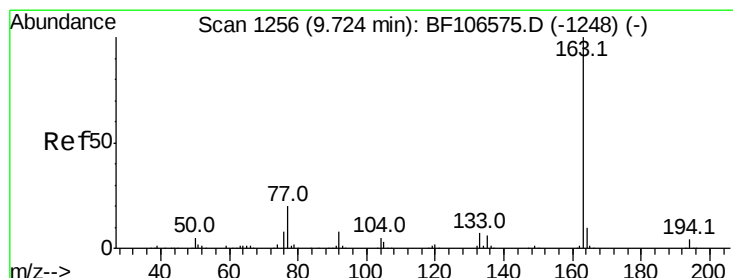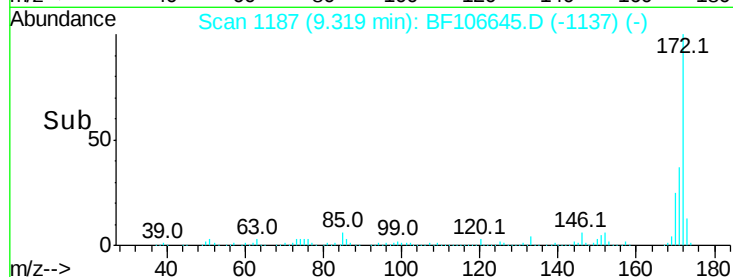
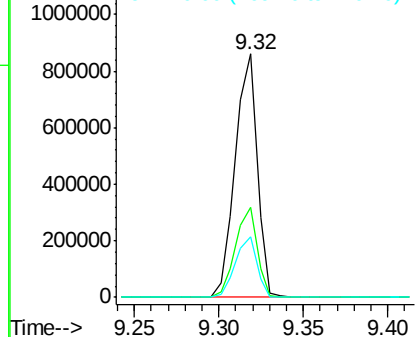


#49
Dimethylphthalate
Concen: 17.277 ng
RT: 9.71 min Scan# 1253
Delta R.T. -0.02 min
Lab File: BF106645.D
Acq: 21 Jun 2018 2:49

Tgt Ion:163 Resp: 180294
Ion Ratio Lower Upper
163 100
194 3.9 2.7 4.1
164 11.3 8.2 12.2

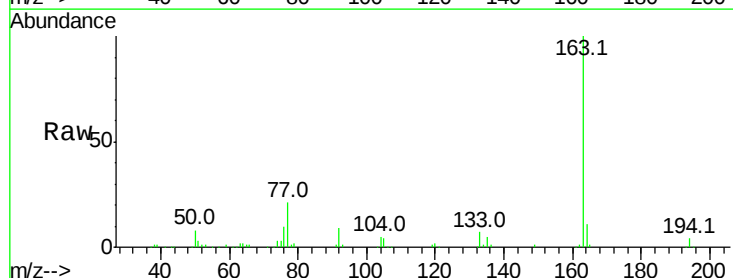

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

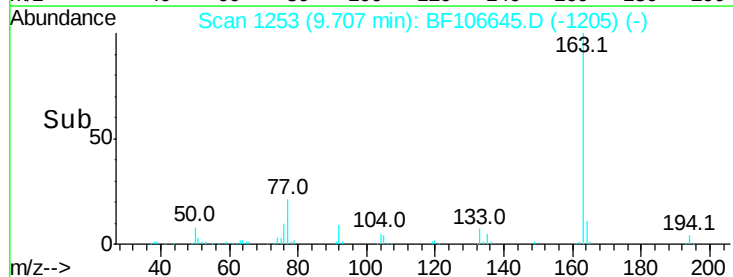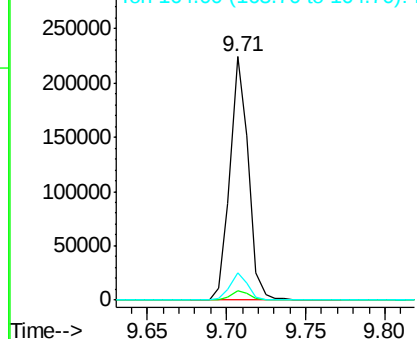



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.49 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BF106645.D

Acq: 21 Jun 2018 2:49

Instrument :

BNA_F

ClientSampleId :

A-3(5.0)


Tot Ion:188 Resp: 239282

Ion Ratio Lower Upper

188 100

94 8.4 8.5 12.7#




80 9.6 9.2 13.8

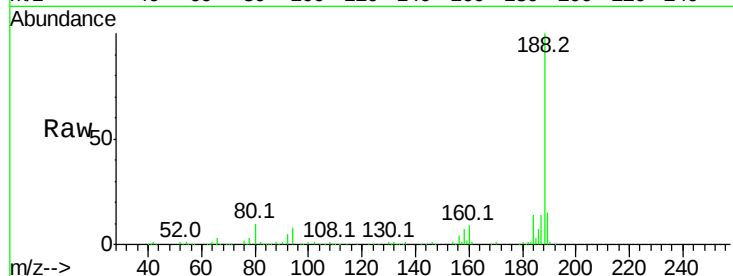

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

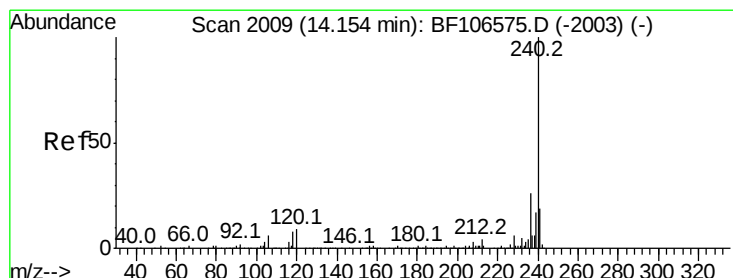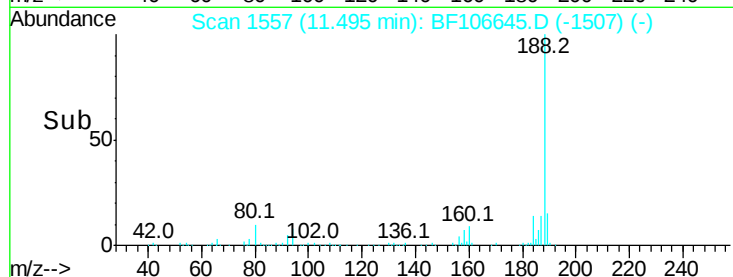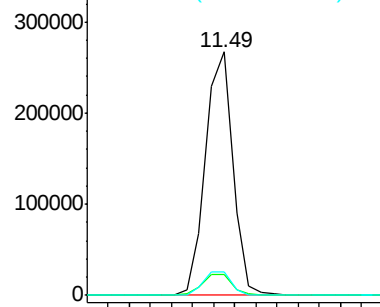

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.14 min Scan# 2007

Delta R.T. -0.01 min

Lab File: BF106645.D

Acq: 21 Jun 2018 2:49


Tgt Ion:240 Resp: 257062

Ion Ratio Lower Upper

240 100

120 9.8 9.5 14.3



236 26.2 20.7 31.1

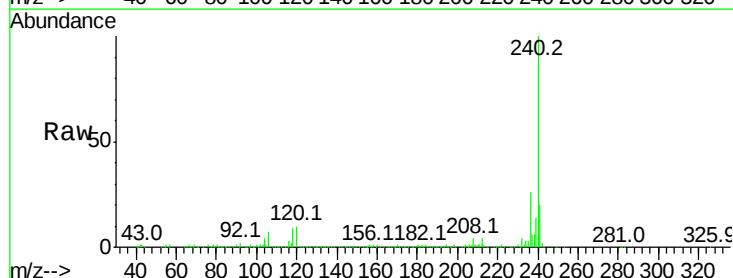


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



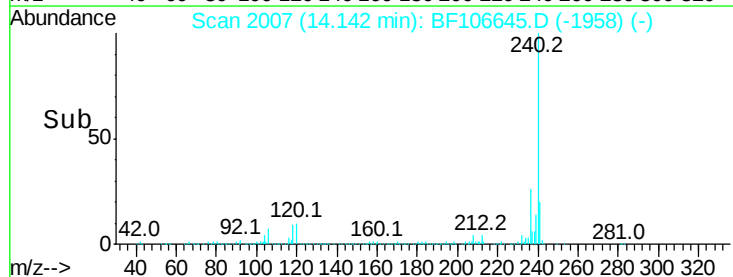
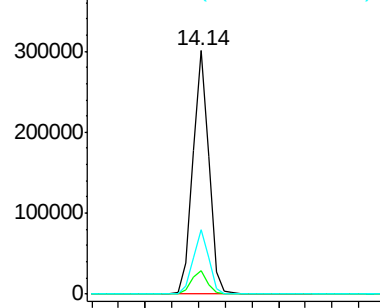


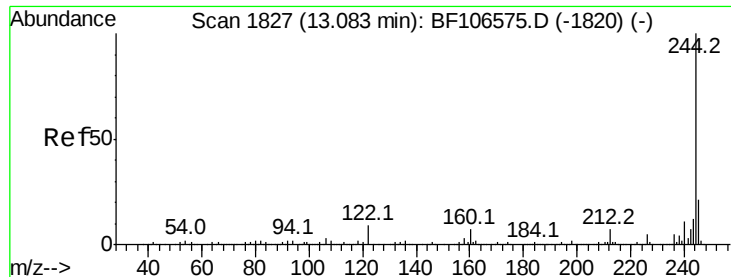

#78
 Terphenyl-d14
 Concen: 77.912 ng
 RT: 13.08 min Scan# 1826
 Delta R.T. -0.01 min
 Lab File: BF106645.D
 Acq: 21 Jun 2018 2:49

Instrument :
 BNA_F
 ClientSampleId :
 A-3(5.0)

Tot Ion:244 Resp: 826825
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.4 8.0
 122 9.5 11.0 16.4#

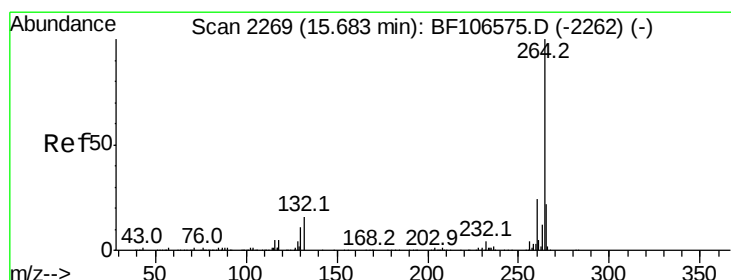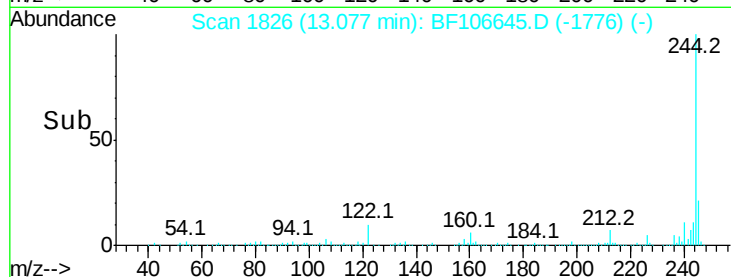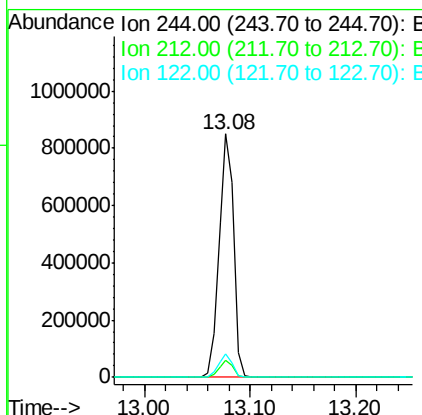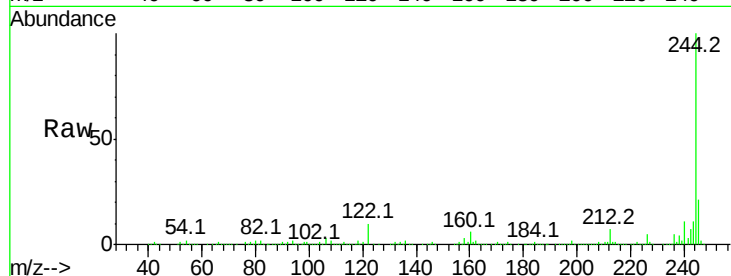

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.68 min Scan# 2268
 Delta R.T. -0.01 min
 Lab File: BF106645.D
 Acq: 21 Jun 2018 2:49

Tgt Ion:264 Resp: 202450
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.2 28.8
 265 21.7 17.5 26.3

