


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062018\
 Data File : BF106619.D
 Acq On : 20 Jun 2018 15:04
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 19 14:32:09 2018

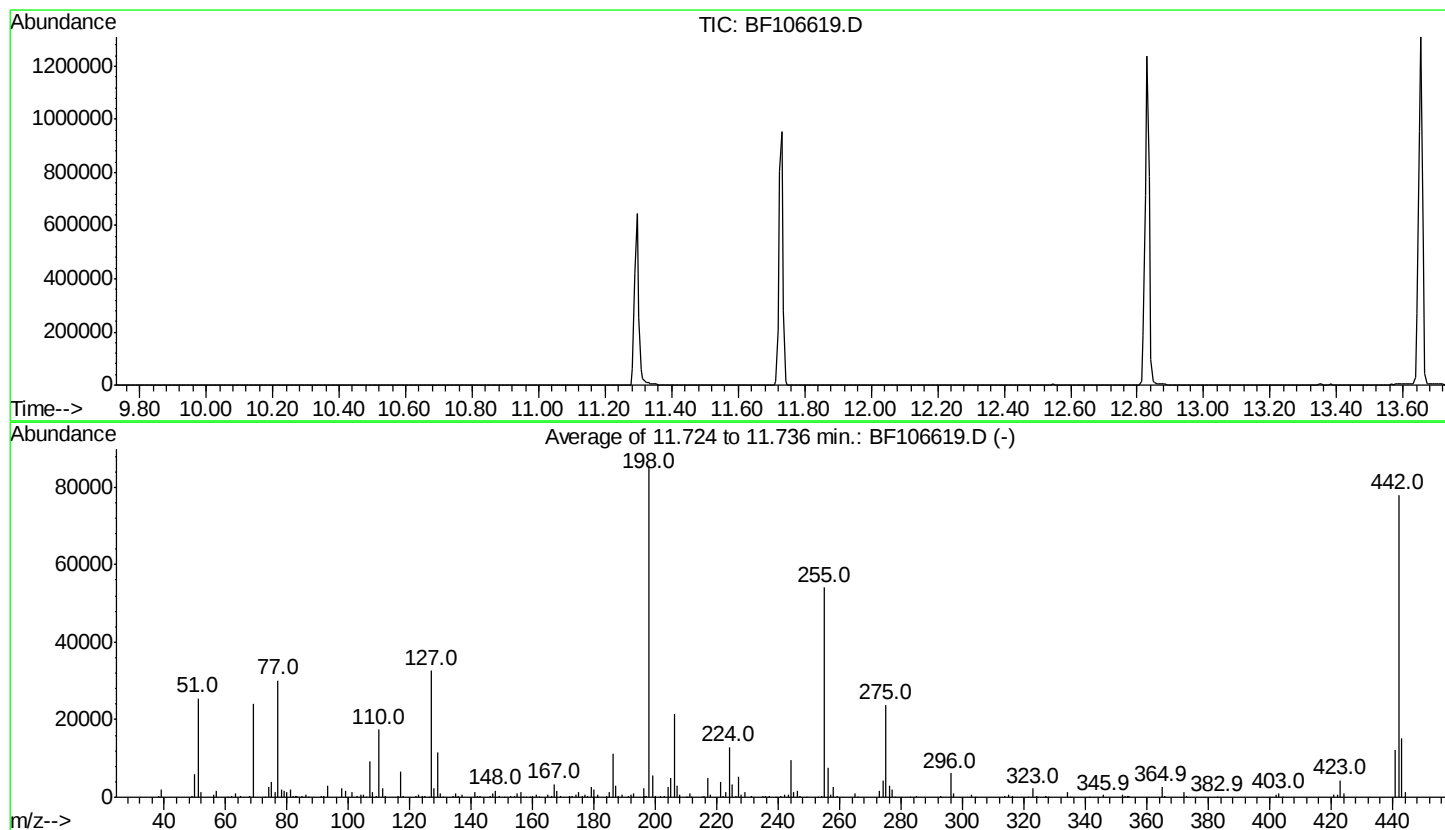

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	25531	PASS
68	69	0.00	2	1.4	333	PASS
69	198	0.00	100	28.1	24075	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.1	32615	PASS
197	198	0.00	2	0.3	214	PASS
198	198	100	100	100.0	85557	PASS
199	198	5	9	6.6	5645	PASS
275	198	10	60	27.9	23833	PASS
365	198	1	100	3.2	2765	PASS
441	443	0.01	100	82.0	12331	PASS
442	198	50	100	91.3	78090	PASS
443	442	15	24	19.3	15042	PASS