


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062018\
 Data File : BF106646.D
 Acq On : 21 Jun 2018 3:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 19 14:32:09 2018

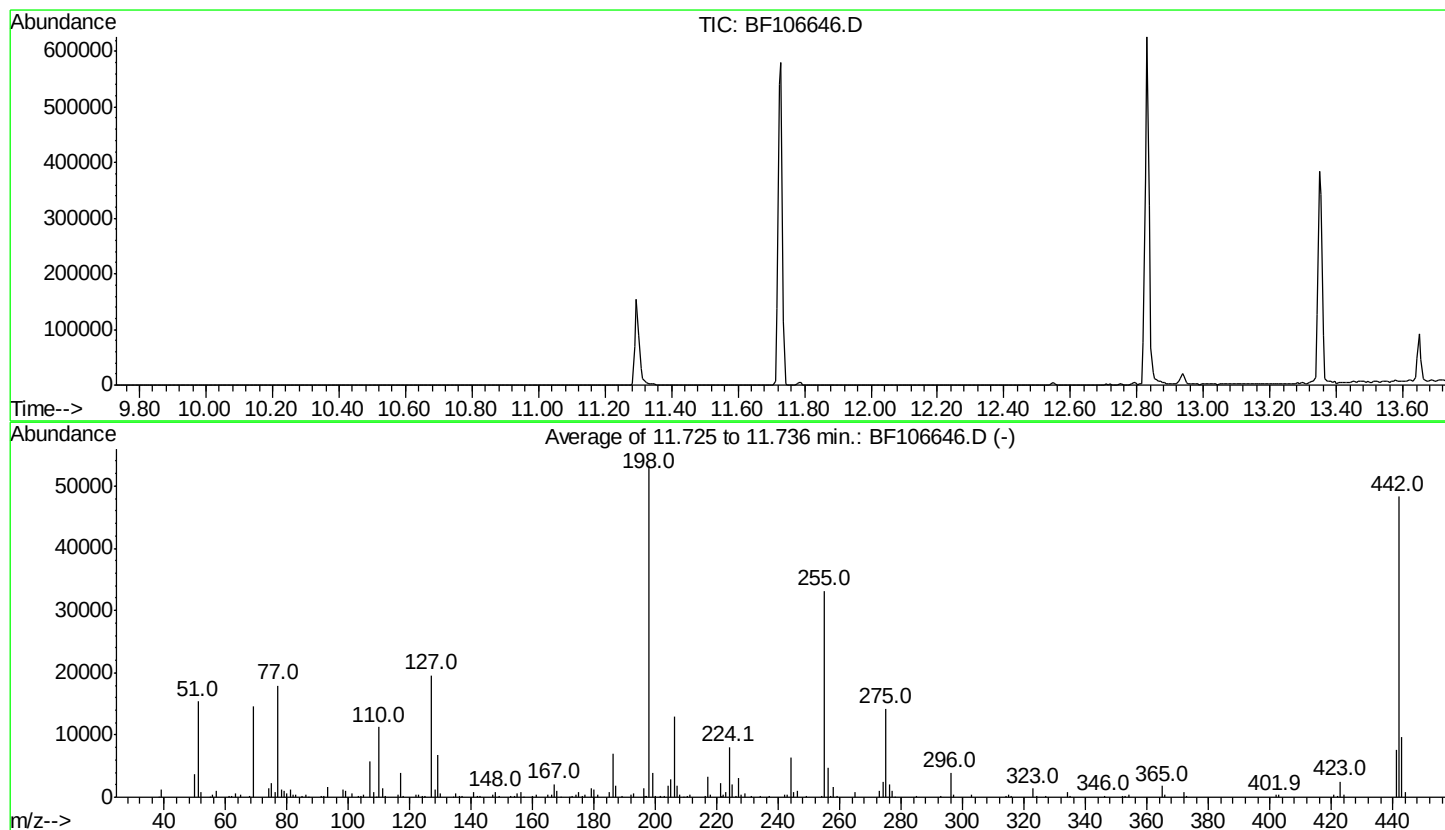

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	15401	PASS
68	69	0.00	2	1.6	230	PASS
69	198	0.00	100	27.4	14611	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.8	19624	PASS
197	198	0.00	2	0.4	234	PASS
198	198	100	100	100.0	53273	PASS
199	198	5	9	7.2	3847	PASS
275	198	10	60	26.7	14209	PASS
365	198	1	100	3.3	1763	PASS
441	443	0.01	100	77.4	7517	PASS
442	198	50	100	90.6	48242	PASS
443	442	15	24	20.1	9708	PASS