
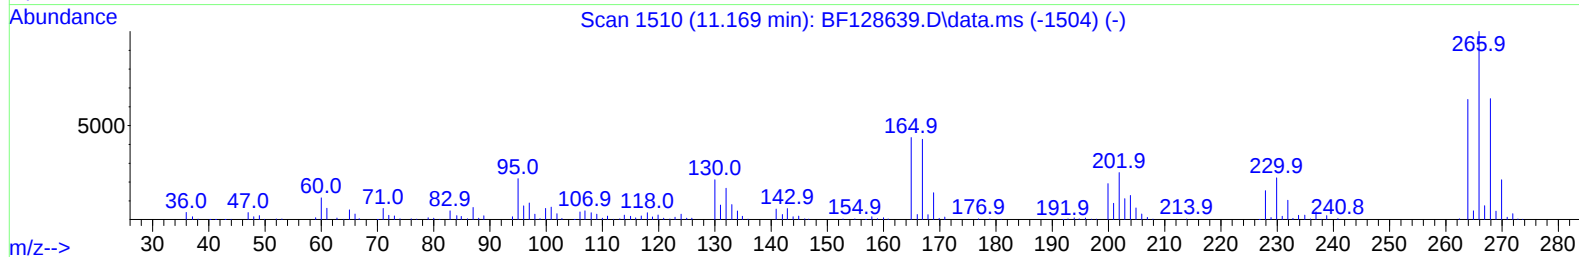
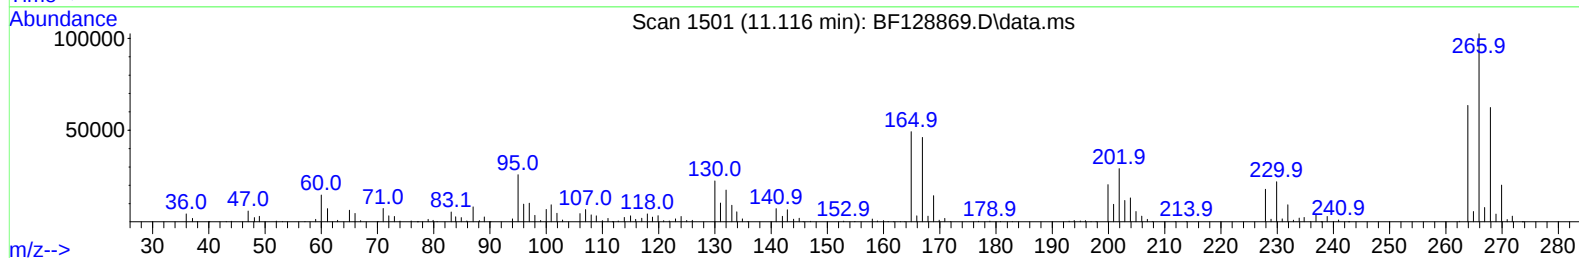


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128869.D
Acq On : 20 Jun 2022 10:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 05:37:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 21 00:40:09 2022
Response via : Initial Calibration

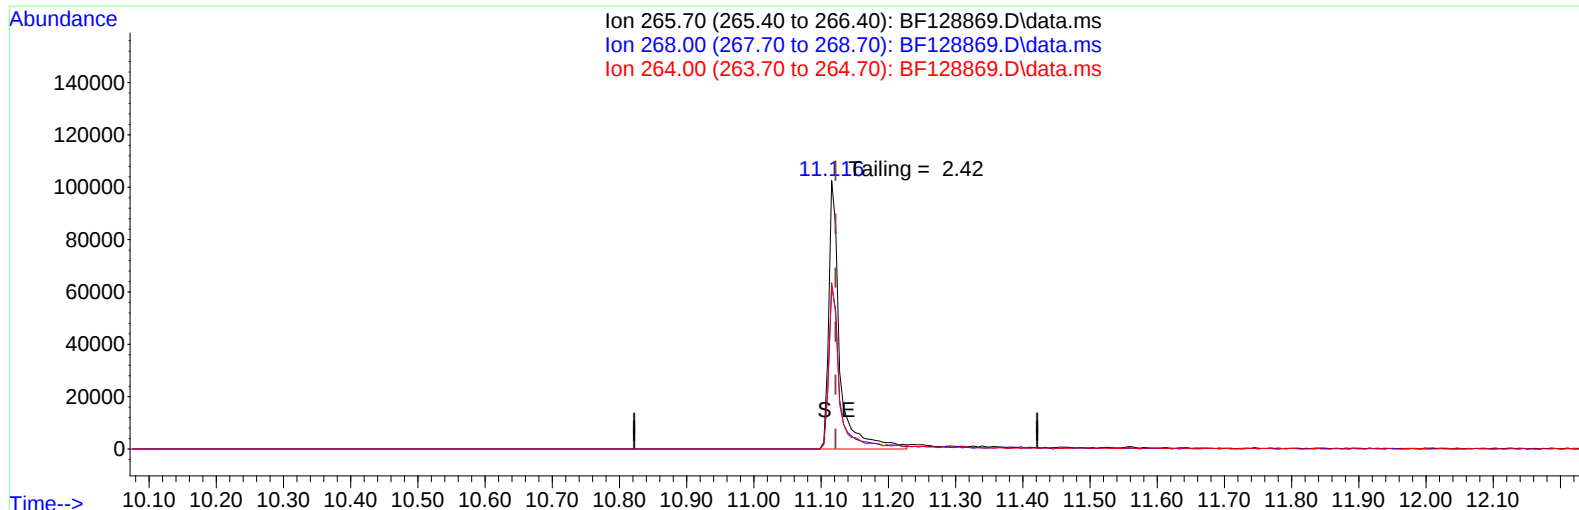

TIC: BF128869.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.006) 33431.32 ng

response 117601

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	60.84
264.00	61.80	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128869.D
Acq On : 20 Jun 2022 10:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 05:37:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 21 00:40:09 2022
Response via : Initial Calibration

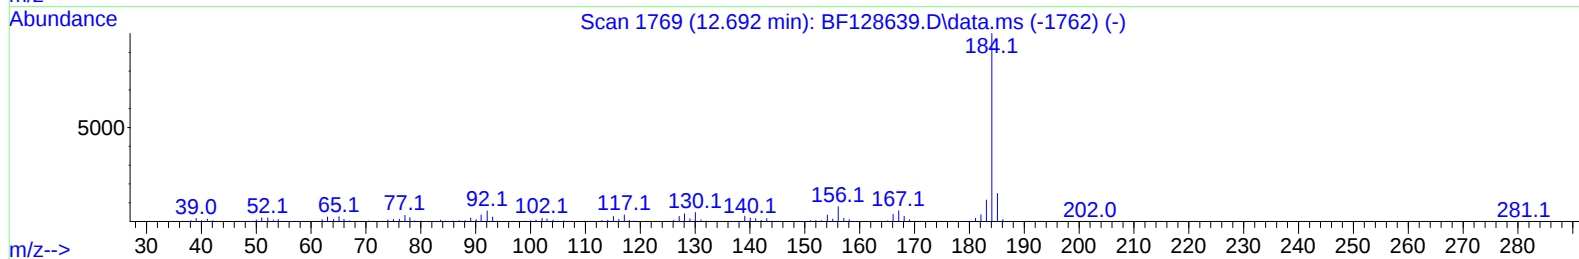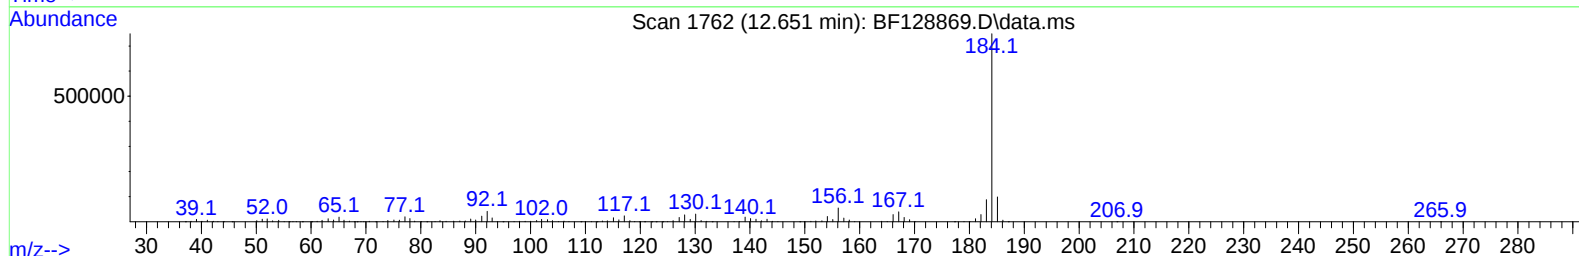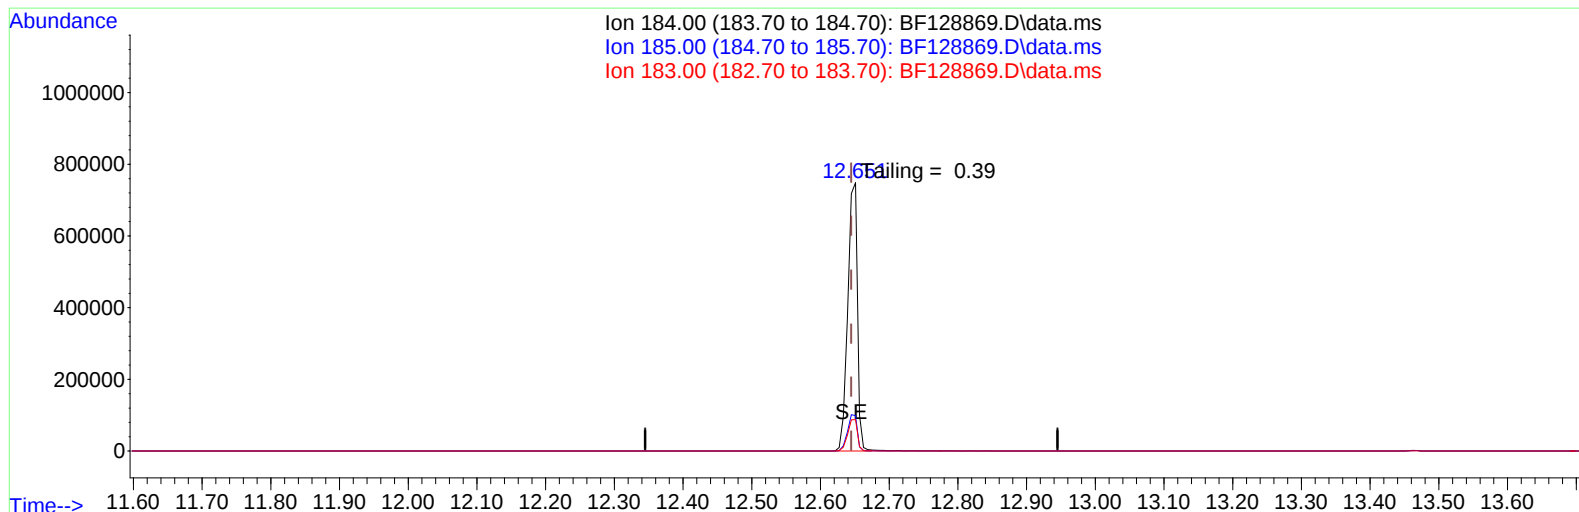

TIC: BF128869.D\data.ms

(77) Benzidine

12.651min (+ 0.006) 488575.18 ng

response 720722

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.17
183.00	11.60	11.73
0.00	0.00	0.00