

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060222\
 Data File : BF128876.D
 Acq On : 20 Jun 2022 14:57
 Operator : CG\JU
 Sample : N3383-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RB-01-(10-11.5)

Quant Time: Jun 21 01:14:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 21 00:40:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.775	152	85487	20.000	ng	0.00
21) Naphthalene-d8	8.057	136	341761	20.000	ng	# 0.00
39) Acenaphthene-d10	9.810	164	193782	20.000	ng	0.00
64) Phenanthrene-d10	11.298	188	361017	20.000	ng	0.00
76) Chrysene-d12	13.945	240	206823	20.000	ng	# 0.00
86) Perylene-d12	15.392	264	159892	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.410	112	667845	124.436	ng	0.00
7) Phenol-d6	6.434	99	861967	131.571	ng	0.00
23) Nitrobenzene-d5	7.340	82	525923	71.647	ng	-0.01
42) 2,4,6-Tribromophenol	10.610	330	237622	103.782	ng	0.00
45) 2-Fluorobiphenyl	9.134	172	1026115	74.175	ng	0.00
79) Terphenyl-d14	12.892	244	1079364	90.683	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128876.D
Acq On : 20 Jun 2022 14:57
Operator : CG\JU
Sample : N3383-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RB-01-(10-11.5)

Quant Time: Jun 21 01:14:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 21 00:40:09 2022
Response via : Initial Calibration




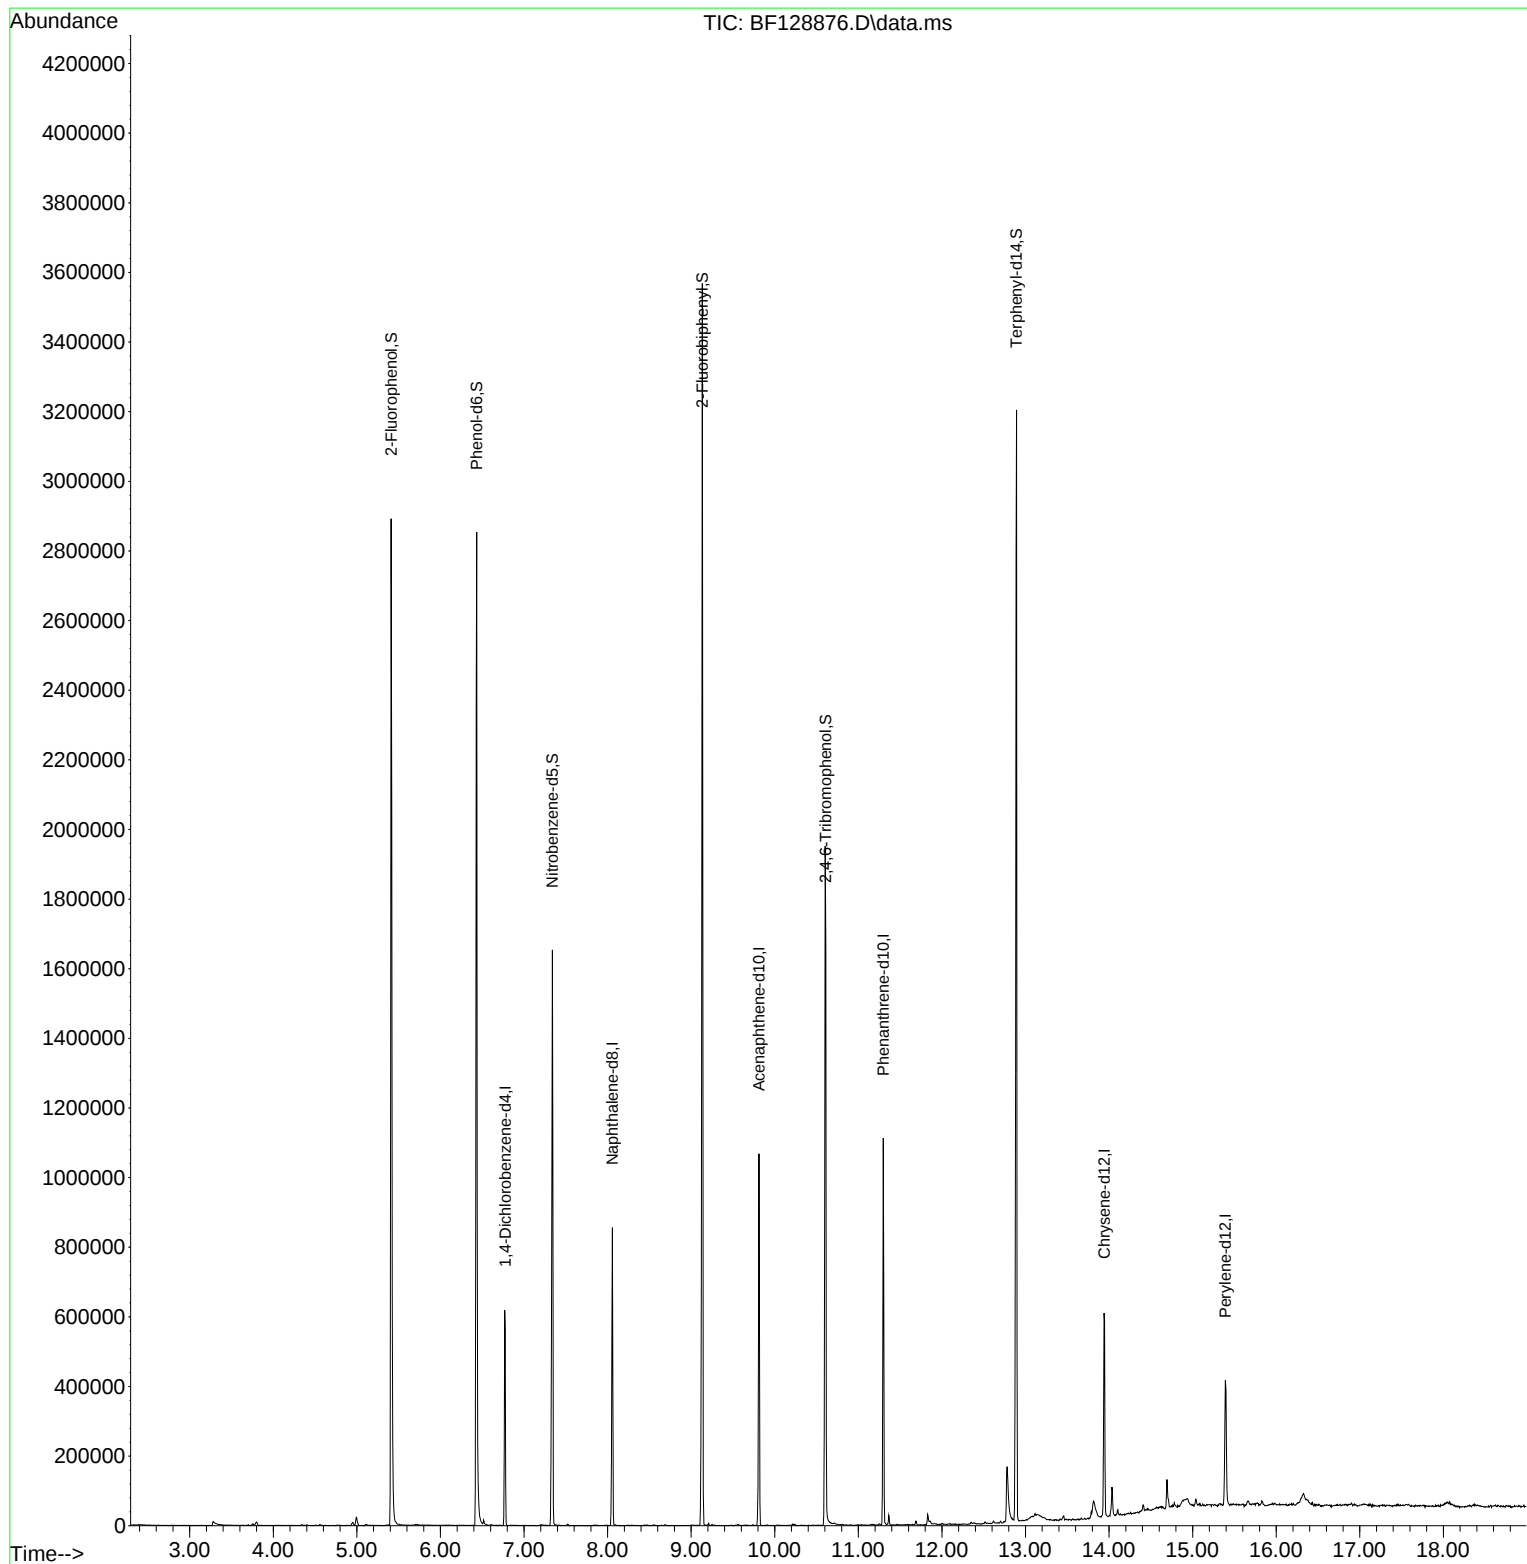


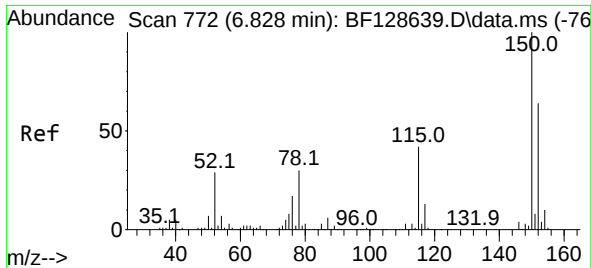

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.775 min Scan# 70
Delta R.T. -0.000 min
Lab File: BF128876.D
Acq: 20 Jun 2022 14:57




Instrument :
BNA_F
ClientSampleId :
RB-01-(10-11.5)


Tgt Ion:152 Resp: 85487
Ion Ratio Lower Upper
152 100
150 153.1 123.7 185.5
115 62.9 49.9 74.9

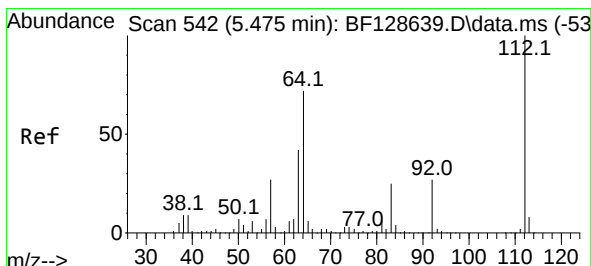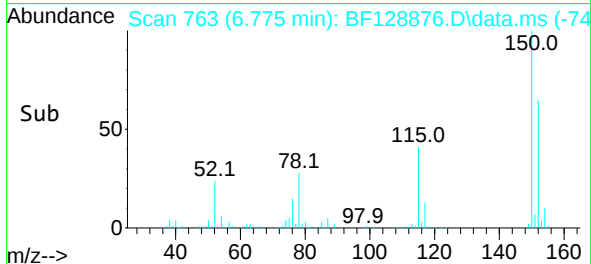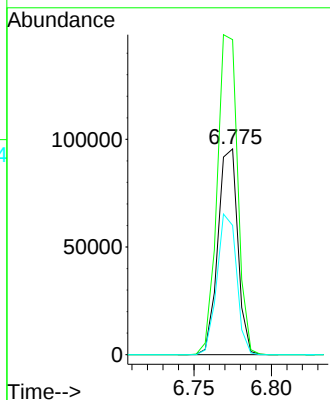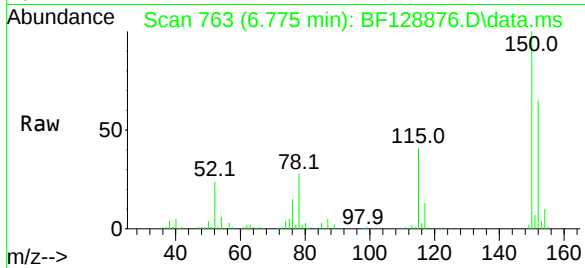

#5
2-Fluorophenol
Concen: 124.436 ng
RT: 5.410 min Scan# 531
Delta R.T. 0.000 min
Lab File: BF128876.D
Acq: 20 Jun 2022 14:57

Tgt Ion:112 Resp: 667845
Ion Ratio Lower Upper
112 100
64 70.9 53.3 79.9
63 39.4 28.0 42.0


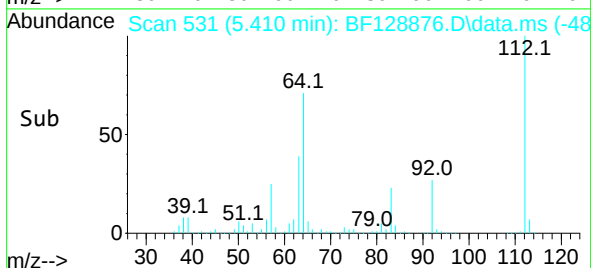
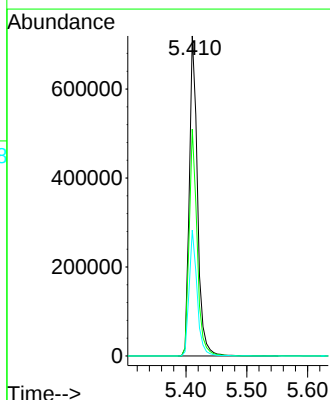
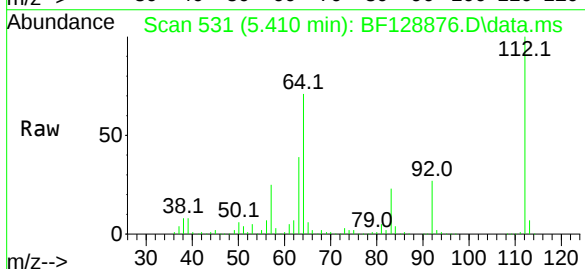


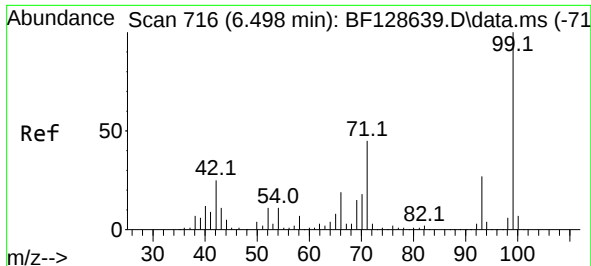

#7
Phenol-d6
Concen: 131.571 ng
RT: 6.434 min Scan# 716
Delta R.T. -0.006 min
Lab File: BF128876.D
Acq: 20 Jun 2022 14:57




Instrument :
BNA_F
ClientSampleId :
RB-01-(10-11.5)


Tgt Ion: 99 Resp: 861967
Ion Ratio Lower Upper
99 100
42 23.1 17.3 25.9
71 41.5 28.9 43.3

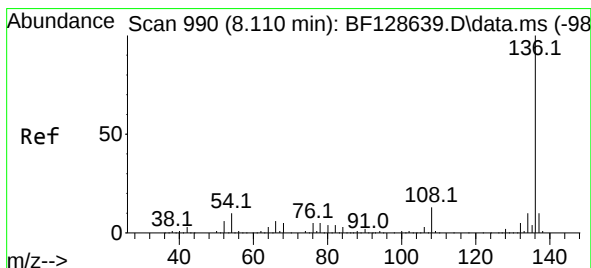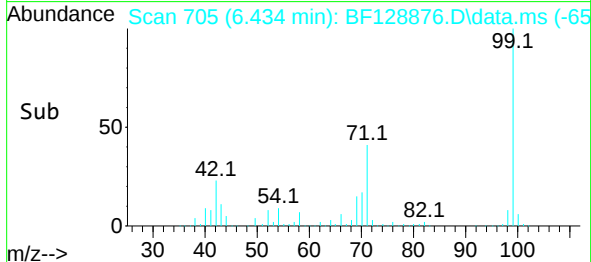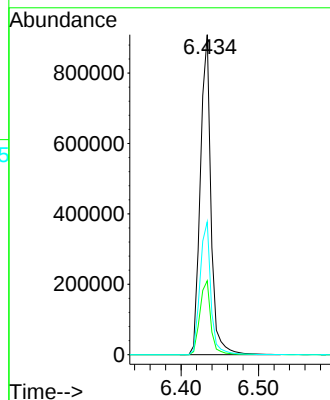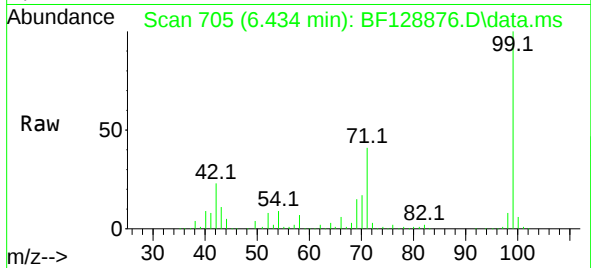

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.057 min Scan# 981
Delta R.T. -0.006 min
Lab File: BF128876.D
Acq: 20 Jun 2022 14:57

Tgt Ion: 136 Resp: 341761
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 9.5 7.5 11.3
68 4.6 4.7 7.1#

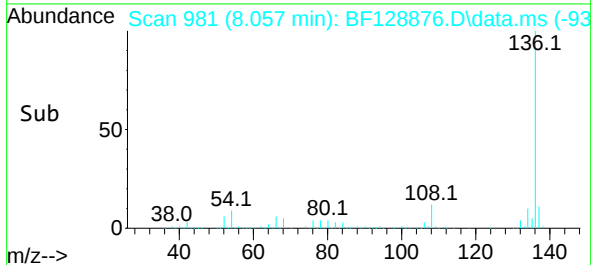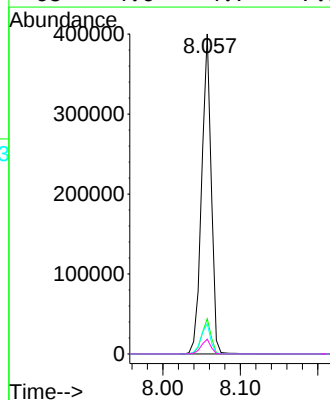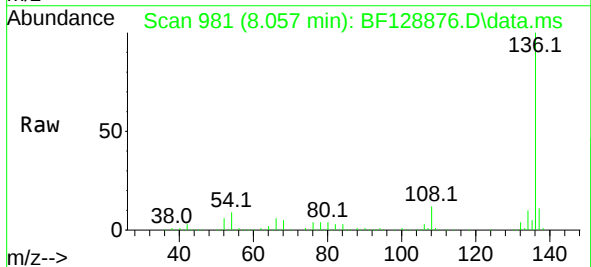

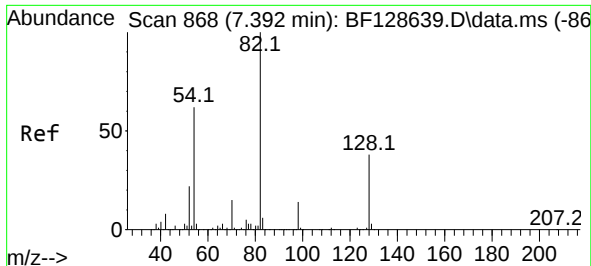

#23

Nitrobenzene-d5

Concen: 71.647 ng

RT: 7.340 min Scan# 81

Delta R.T. -0.012 min

Lab File: BF128876.D

Acq: 20 Jun 2022 14:57

Instrument :

BNA_F

ClientSampleId :

RB-01-(10-11.5)





Tgt Ion: 82 Resp: 525923

Ion Ratio Lower Upper

82 100

128 40.0 34.0 51.0

54 60.9 46.9 70.3

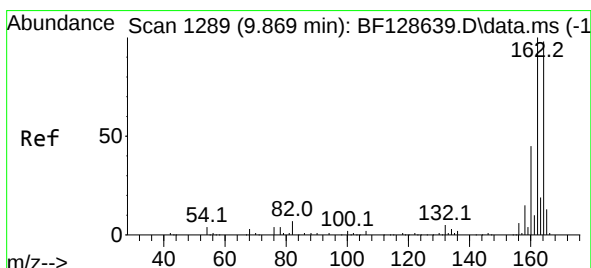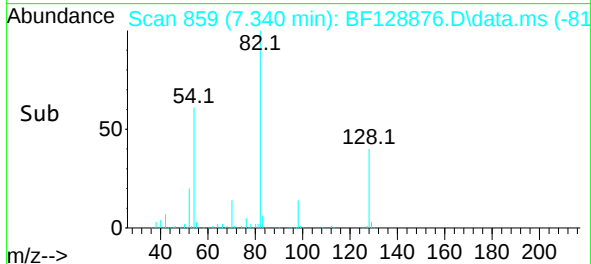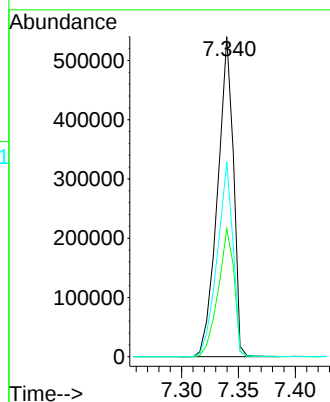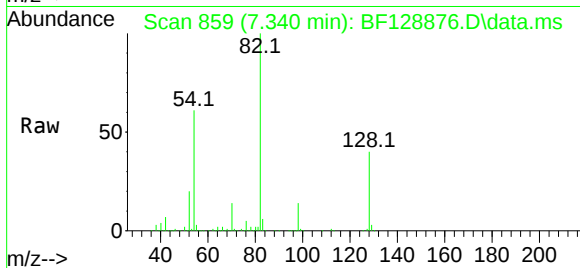

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.810 min Scan# 1279

Delta R.T. -0.006 min

Lab File: BF128876.D

Acq: 20 Jun 2022 14:57




Tgt Ion: 164 Resp: 193782


Ion Ratio Lower Upper

164 100

162 102.2 79.5 119.3

160 46.7 34.2 51.4

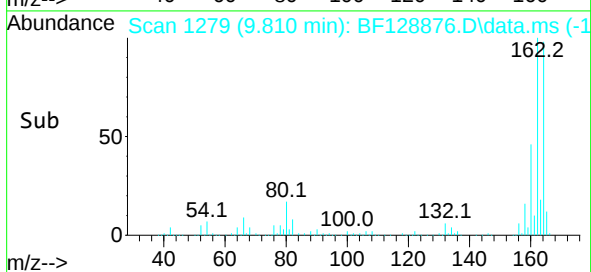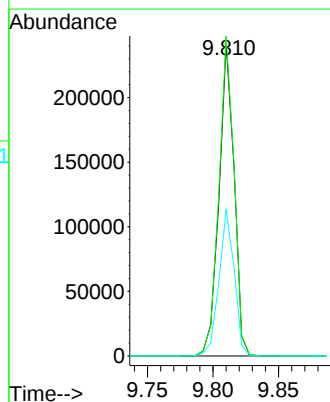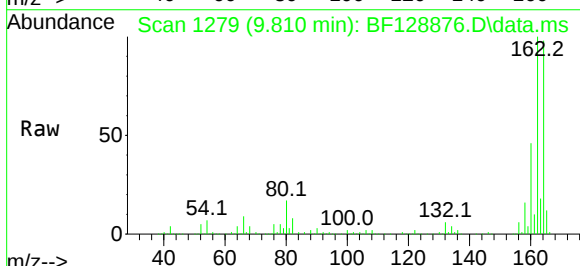

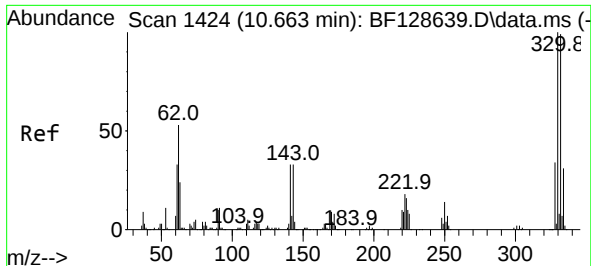

#42

2,4,6-Tribromophenol

Concen: 103.782 ng

RT: 10.610 min Scan# 1424

Delta R.T. 0.000 min

Lab File: BF128876.D

Acq: 20 Jun 2022 14:57

Instrument :

BNA_F

ClientSampleId :

RB-01-(10-11.5)





Tgt Ion:330 Resp: 237622

Ion Ratio Lower Upper

330 100

332 97.1 76.8 115.2

141 34.4 28.0 42.0

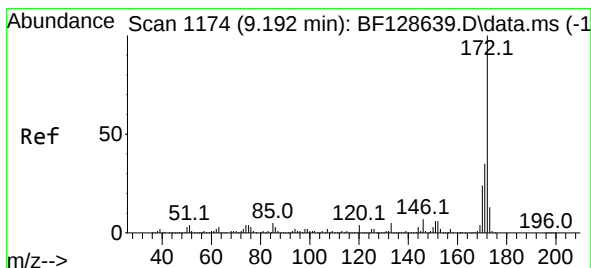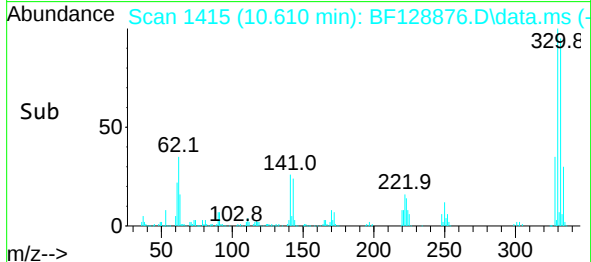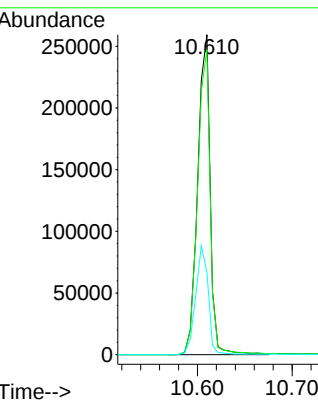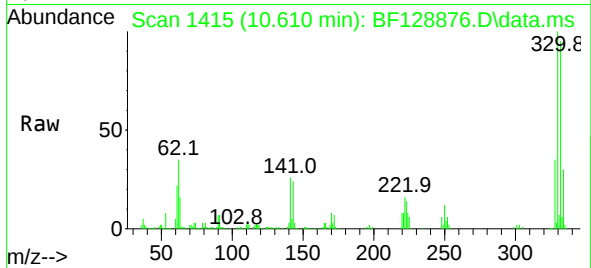

#45

2-Fluorobiphenyl

Concen: 74.175 ng

RT: 9.134 min Scan# 1164

Delta R.T. -0.006 min

Lab File: BF128876.D

Acq: 20 Jun 2022 14:57




Tgt Ion:172 Resp: 1026115


Ion Ratio Lower Upper

172 100

171 34.6 28.8 43.2

170 23.6 19.8 29.8


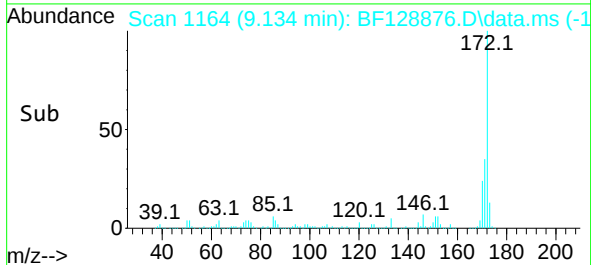
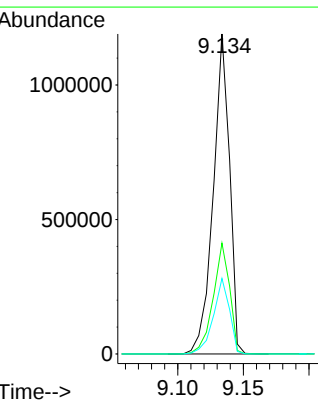
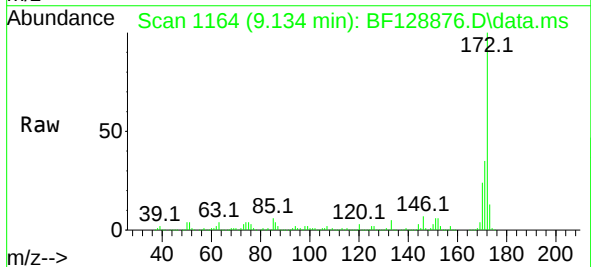


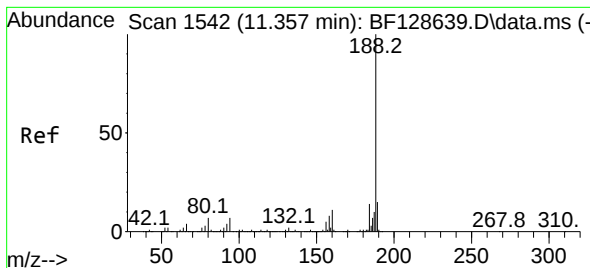

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.298 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF128876.D
Acq: 20 Jun 2022 14:57




Instrument :
BNA_F
ClientSampleId :
RB-01-(10-11.5)


Tgt Ion:188 Resp: 361017
Ion Ratio Lower Upper
188 100
94 7.7 7.0 10.6
80 8.5 7.6 11.4

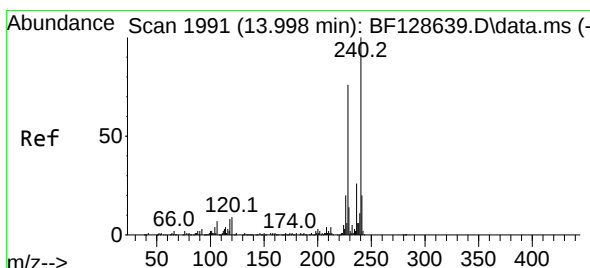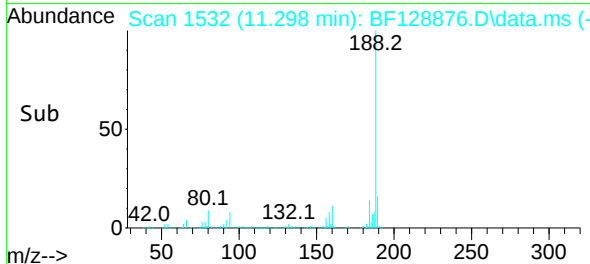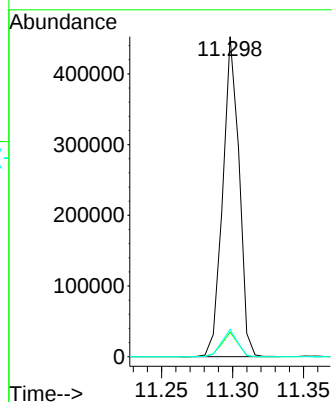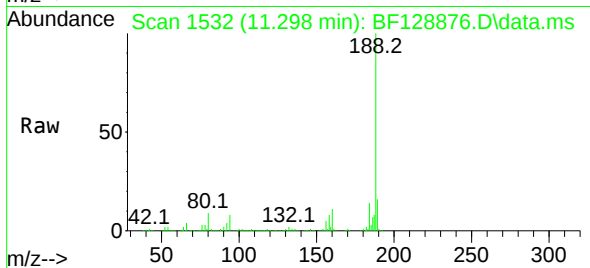

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.945 min Scan# 1982
Delta R.T. -0.006 min
Lab File: BF128876.D
Acq: 20 Jun 2022 14:57


Tgt Ion:240 Resp: 206823
Ion Ratio Lower Upper
240 100
120 6.5 8.9 13.3#
236 24.8 20.8 31.2

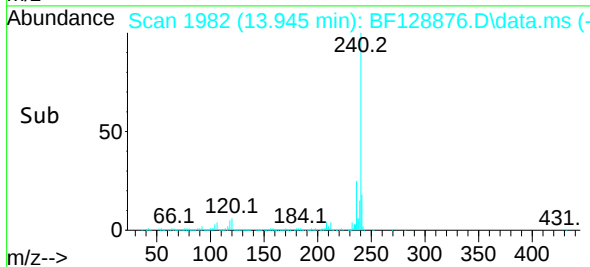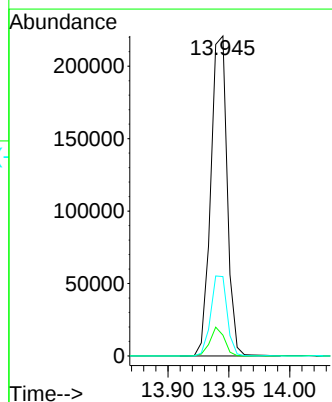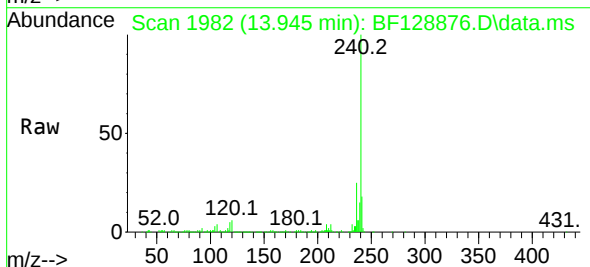



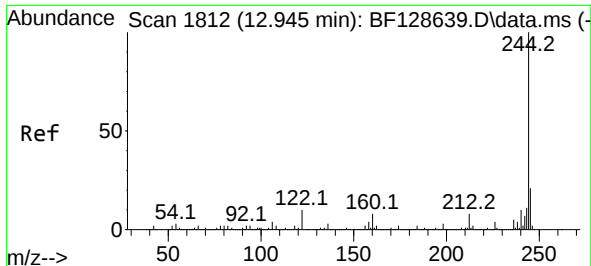


#79
 Terphenyl-d14
 Concen: 90.683 ng
 RT: 12.892 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BF128876.D
 Acq: 20 Jun 2022 14:57

Instrument :
 BNA_F
 ClientSampleId :
 RB-01-(10-11.5)

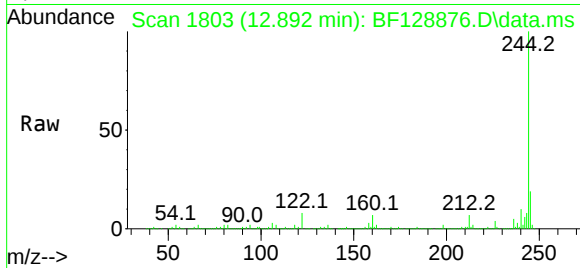

Tgt Ion:244 Resp: 1079364
 Ion Ratio Lower Upper
 244 100
 212 7.0 6.1 9.1
 122 8.2 8.8 13.2#

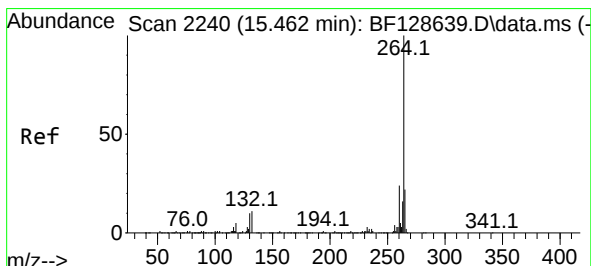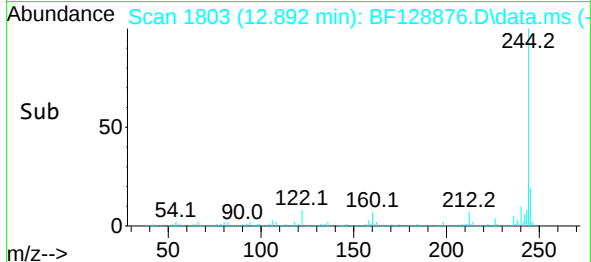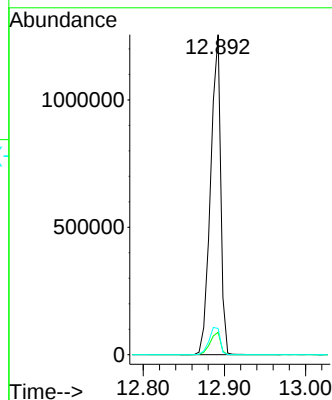

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.392 min Scan# 2228
 Delta R.T. -0.006 min
 Lab File: BF128876.D
 Acq: 20 Jun 2022 14:57

Tgt Ion:264 Resp: 159892
 Ion Ratio Lower Upper
 264 100
 260 25.2 18.4 27.6
 265 22.5 17.2 25.8

