

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
 Data File : BF128872.D
 Acq On : 20 Jun 2022 13:03
 Operator : CG\JU
 Sample : N3367-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MJS-MW-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128872.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.822	82	91	99	rBV	39705	63670	1.17%	0.275%
2	4.987	455	459	464	rVB	49297	61466	1.13%	0.265%
3	5.410	528	531	540	rBV	1831107	1818960	33.30%	7.855%
4	6.428	701	704	716	rVB	1216089	1027825	18.81%	4.439%
5	6.775	759	763	766	rBV	648162	575411	10.53%	2.485%
6	7.345	853	860	863	rBV	2087606	2235183	40.92%	9.653%
7	8.057	976	981	984	rBV	883639	768911	14.07%	3.321%
8	9.139	1158	1165	1168	rBV	4481577	4458194	81.61%	19.253%
9	9.810	1274	1279	1283	rBV	1057370	940622	17.22%	4.062%
10	10.610	1408	1415	1418	rBV	3092486	2895660	53.01%	12.505%
11	11.298	1528	1532	1536	rBV	1151050	1031362	18.88%	4.454%
12	11.833	1617	1623	1631	rBV2	95950	146855	2.69%	0.634%
13	12.615	1752	1756	1764	rBV2	47139	63473	1.16%	0.274%
14	12.898	1798	1804	1807	rBV	5339087	5462969	100.00%	23.592%
15	13.821	1957	1961	1972	rVB3	57577	140906	2.58%	0.608%
16	13.945	1978	1982	1985	rVB	1033525	876800	16.05%	3.786%
17	14.039	1993	1998	2001	rVB	89521	96896	1.77%	0.418%
18	15.398	2224	2229	2237	rVB	391744	491187	8.99%	2.121%




Sum of corrected areas: 23156350

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128872.D
Acq On : 20 Jun 2022 13:03
Operator : CG\JU
Sample : N3367-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MJS-MW-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

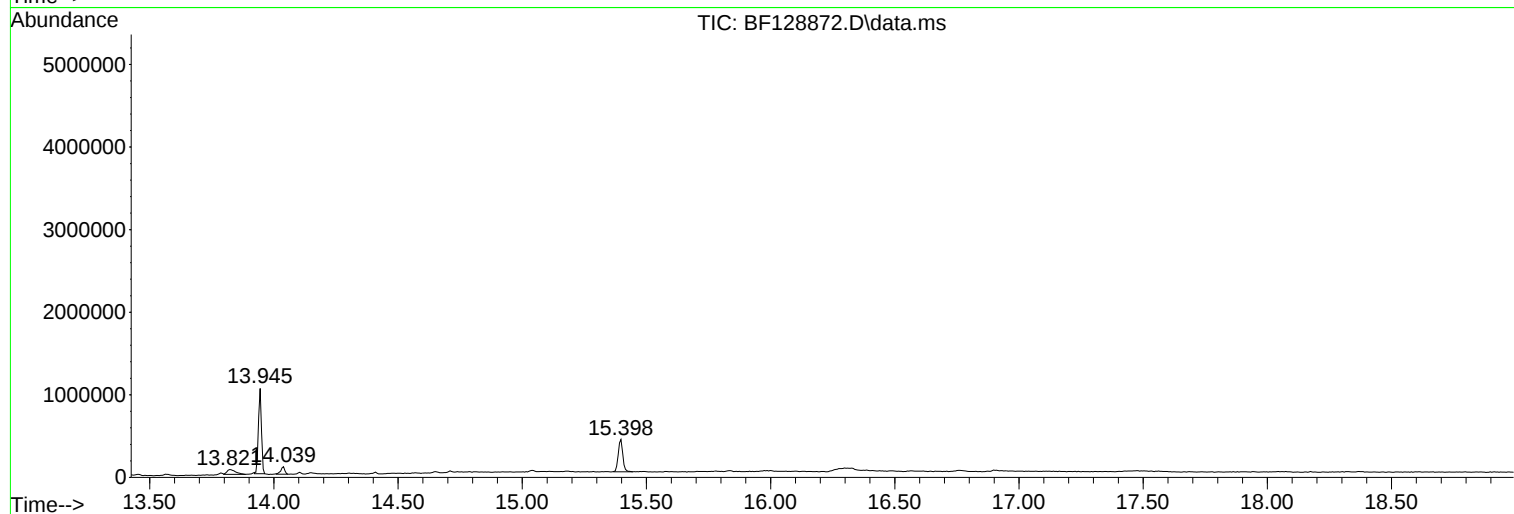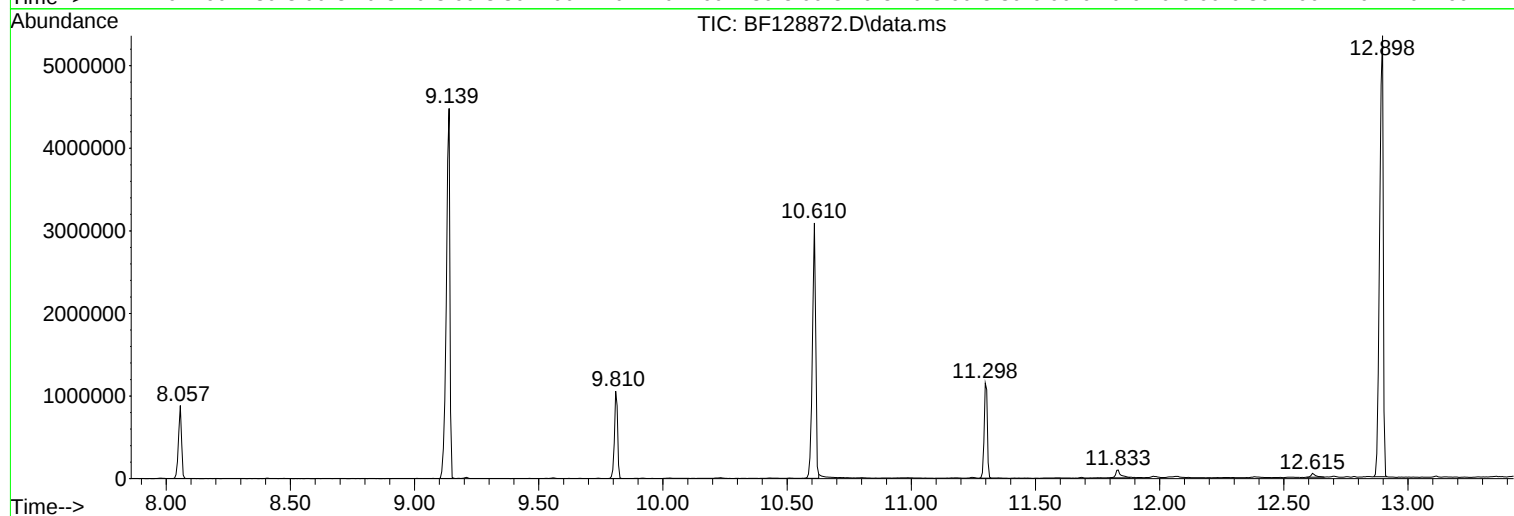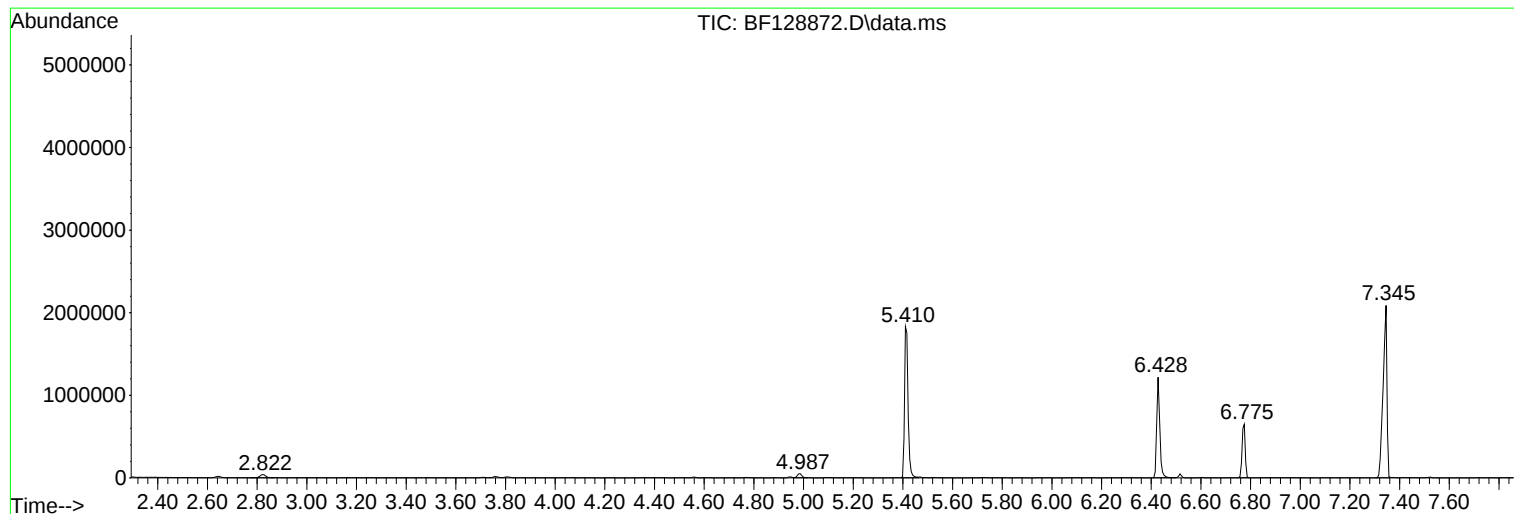

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128872.D
Acq On : 20 Jun 2022 13:03
Operator : CG\JU
Sample : N3367-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MJS-MW-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128872.D
Acq On : 20 Jun 2022 13:03
Operator : CG\JU
Sample : N3367-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MJS-MW-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------