

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
 Data File : BF128873.D
 Acq On : 20 Jun 2022 13:31
 Operator : CG\JU
 Sample : N3383-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RB-04-(10-15)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128873.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	455	459	466	rVB	70399	90265	2.42%	0.398%
2	5.410	528	531	546	rBV	2409532	2248612	60.29%	9.911%
3	6.428	700	704	717	rBV	2666589	2571418	68.94%	11.334%
4	6.775	759	763	766	rBV	725483	663825	17.80%	2.926%
5	7.340	853	859	862	rBV	1840324	1772016	47.51%	7.810%
6	8.057	976	981	984	rBV	996279	870617	23.34%	3.837%
7	9.134	1158	1164	1167	rBV	3854751	3440641	92.25%	15.165%
8	9.398	1205	1209	1212	rBV	151857	112986	3.03%	0.498%
9	9.810	1274	1279	1283	rVB	1227949	1040672	27.90%	4.587%
10	10.604	1409	1414	1418	rBV	2258013	2062808	55.31%	9.092%
11	11.298	1528	1532	1536	rBV	1262122	1114691	29.89%	4.913%
12	11.563	1569	1577	1590	rBV8	33250	118022	3.16%	0.520%
13	11.692	1595	1599	1602	rBV	222762	172292	4.62%	0.759%
14	11.827	1619	1622	1626	rBV2	33899	42493	1.14%	0.187%
15	12.380	1709	1716	1717	rBV3	110878	214361	5.75%	0.945%
16	12.398	1717	1719	1731	rVV2	210796	247157	6.63%	1.089%
17	12.486	1731	1734	1737	rVB	190098	156110	4.19%	0.688%
18	12.545	1740	1744	1747	rBV	238794	193942	5.20%	0.855%
19	12.892	1798	1803	1806	rBV	4141591	3729823	100.00%	16.440%
20	13.333	1875	1878	1880	rVB	52267	43234	1.16%	0.191%
21	13.816	1956	1960	1974	rVB2	88289	236422	6.34%	1.042%
22	13.945	1978	1982	1986	rVB	986951	841500	22.56%	3.709%
23	14.033	1993	1997	2002	rBV	79938	101678	2.73%	0.448%
24	14.692	2106	2109	2116	rBV2	117473	140793	3.77%	0.621%
25	15.398	2224	2229	2235	rBV	373331	461401	12.37%	2.034%




Sum of corrected areas: 22687779

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128873.D
Acq On : 20 Jun 2022 13:31
Operator : CG\JU
Sample : N3383-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RB-04-(10-15)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

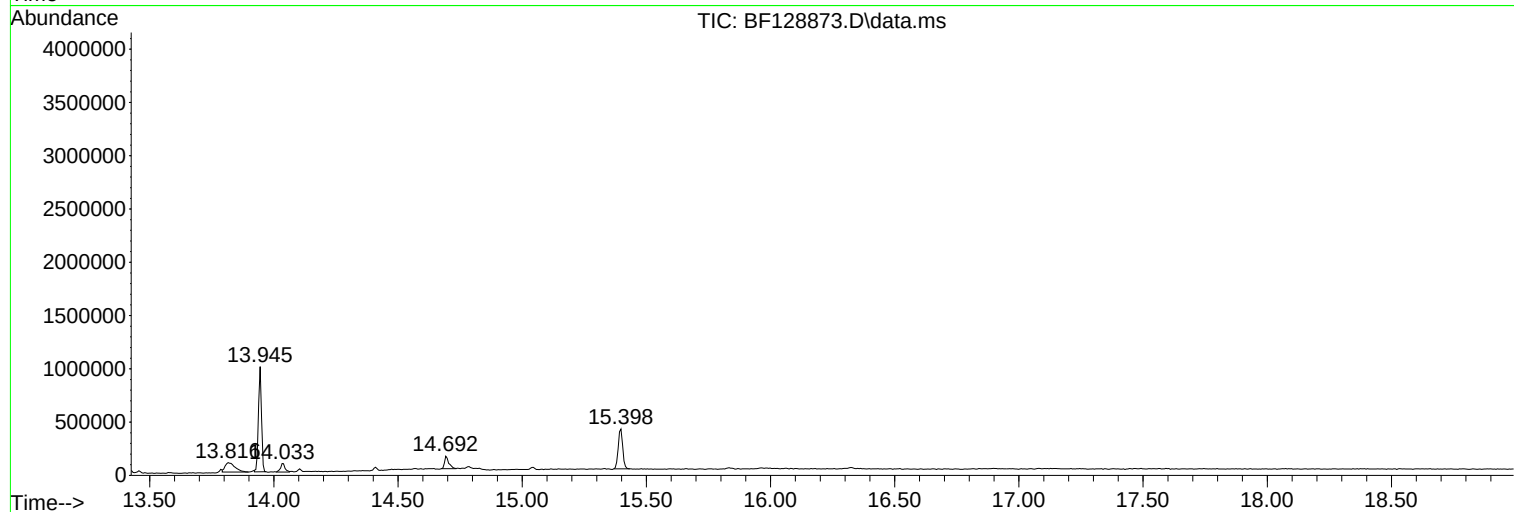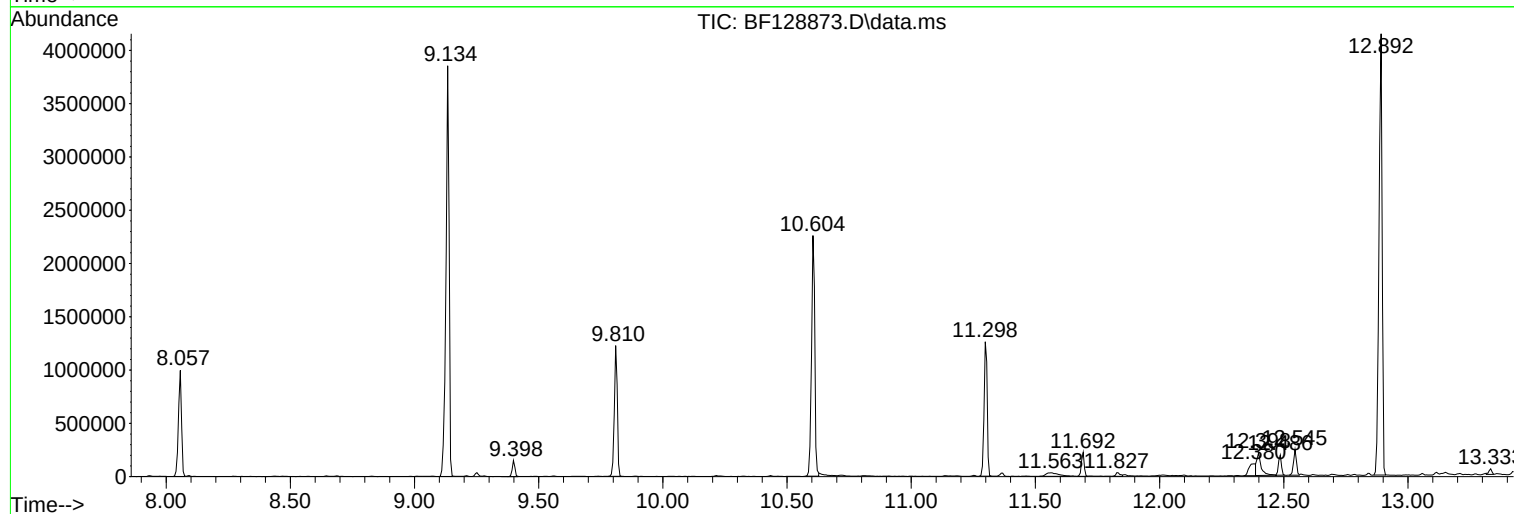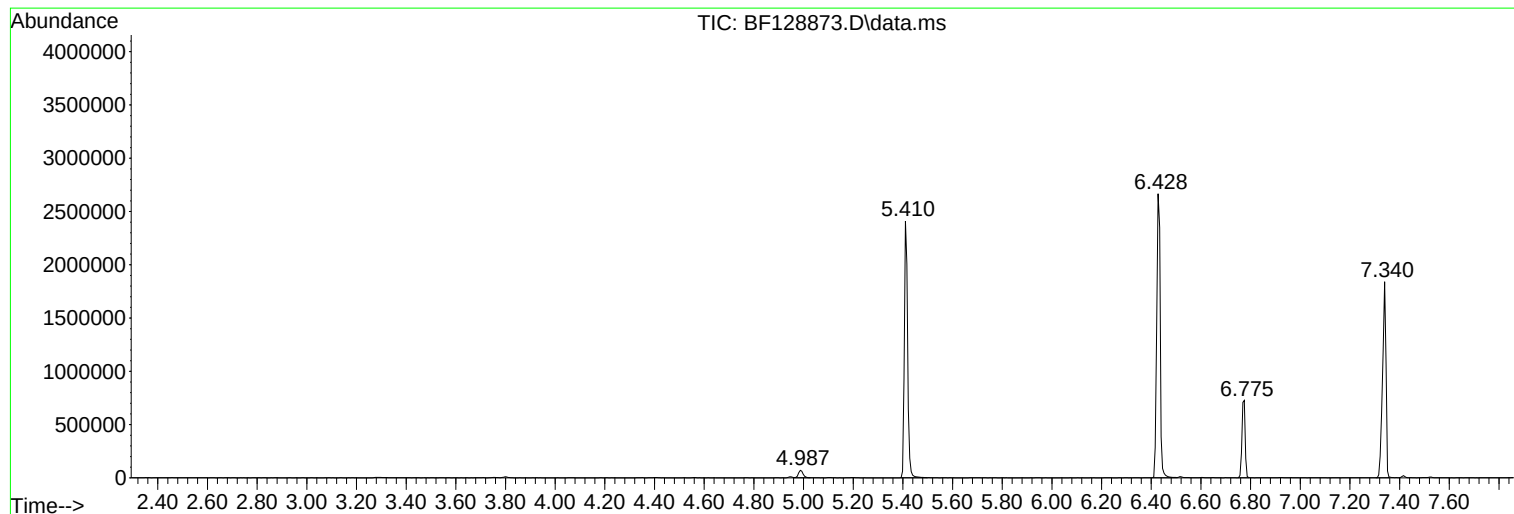

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128873.D
Acq On : 20 Jun 2022 13:31
Operator : CG\JU
Sample : N3383-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RB-04-(10-15)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128873.D
Acq On : 20 Jun 2022 13:31
Operator : CG\JU
Sample : N3383-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RB-04-(10-15)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------