


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
 Data File : BF128869.D
 Acq On : 20 Jun 2022 10:39
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 21 00:40:09 2022

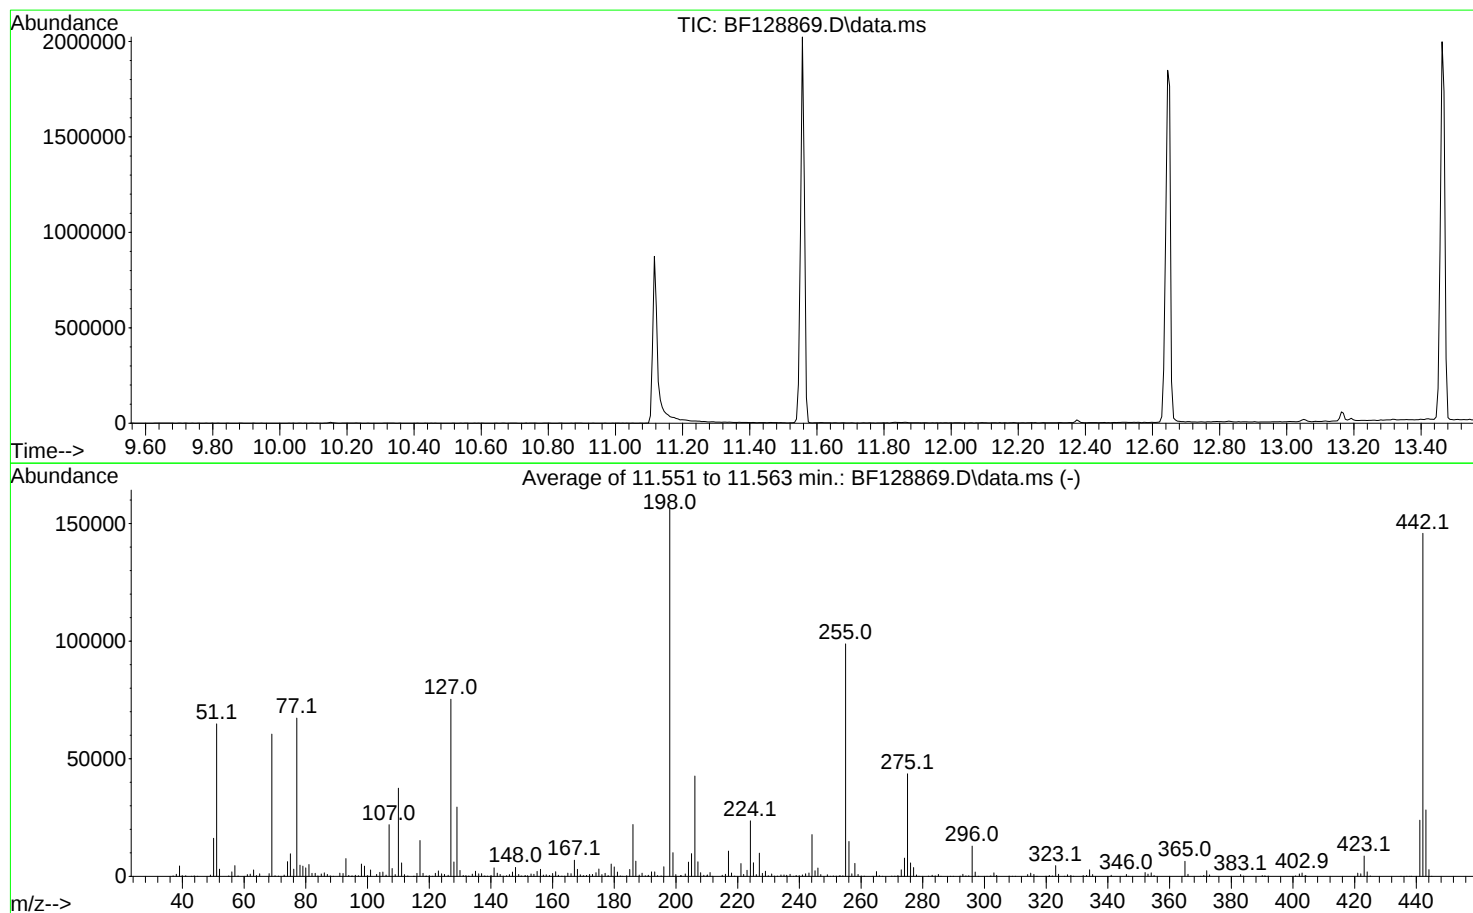




AutoFind: Scans 1575, 1576, 1577; Background Corrected with Scan 1569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	64832	PASS
68	69	0.00	2	1.9	1158	PASS
69	198	0.00	100	38.7	60499	PASS
70	69	0.00	2	0.5	281	PASS
127	198	10	80	48.2	75323	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	156387	PASS
199	198	5	9	6.4	10047	PASS
275	198	10	60	27.9	43627	PASS
365	198	1	100	4.1	6430	PASS
441	198	0.01	100	15.3	23864	PASS
442	442	50	100	100.0	145813	PASS
443	442	15	24	19.3	28200	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128869.D
Acq On : 20 Jun 2022 10:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 21 05:37:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 21 00:40:09 2022
Response via : Initial Calibration

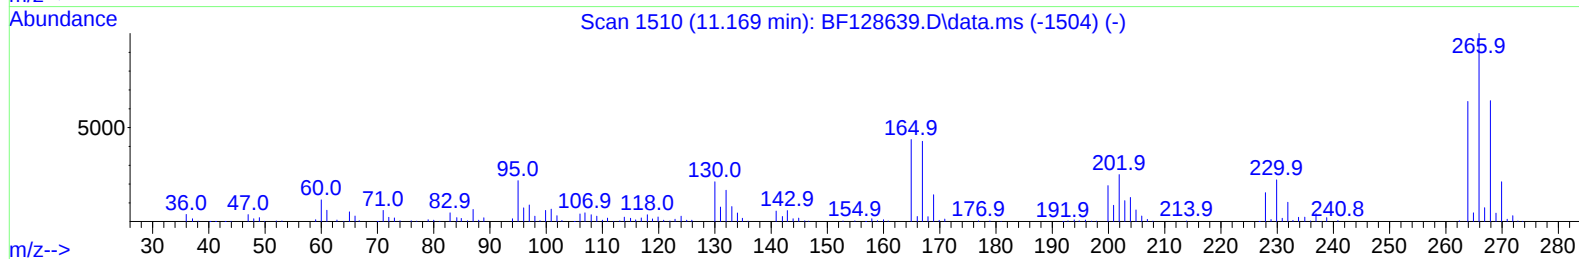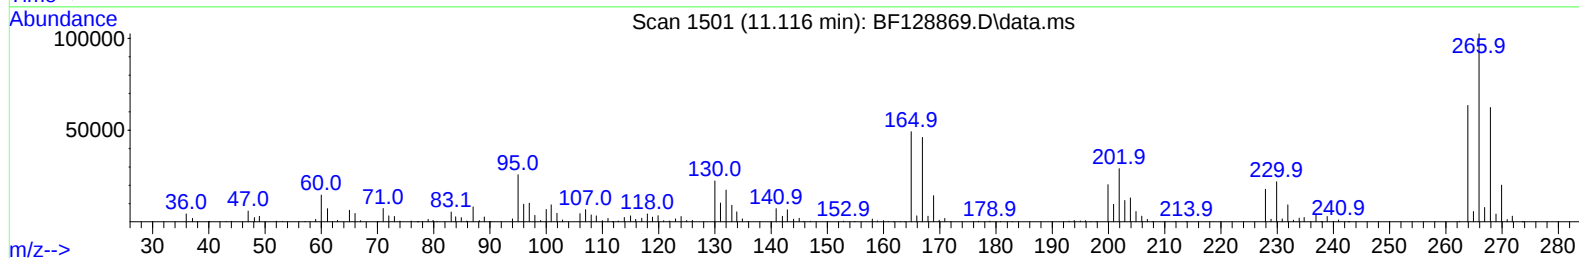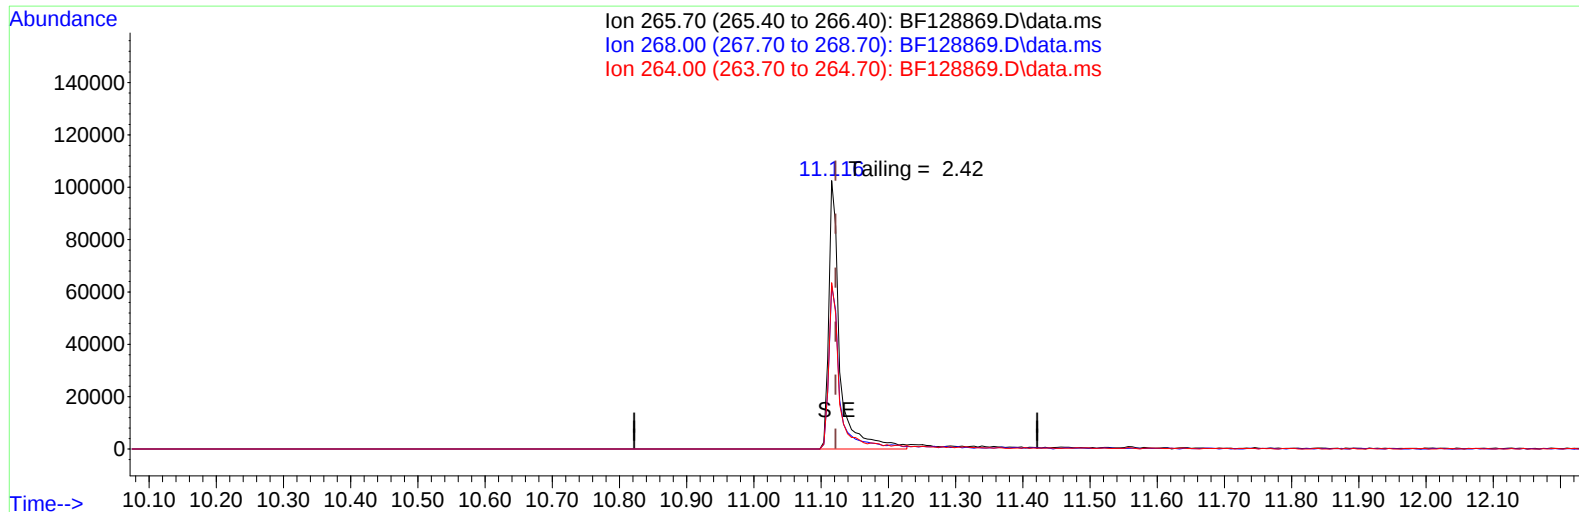

TIC: BF128869.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.006) 33431.32 ng




response 117601

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	60.84
264.00	61.80	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062022\
Data File : BF128869.D
Acq On : 20 Jun 2022 10:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 21 05:37:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 21 00:40:09 2022
Response via : Initial Calibration

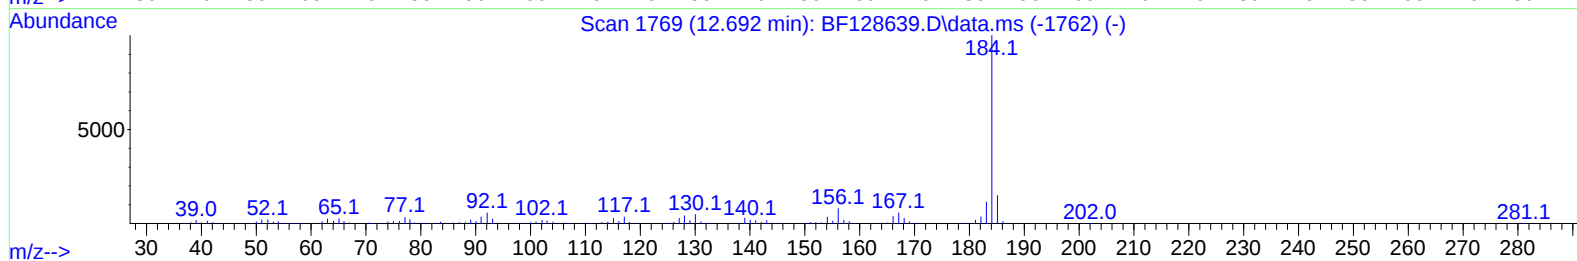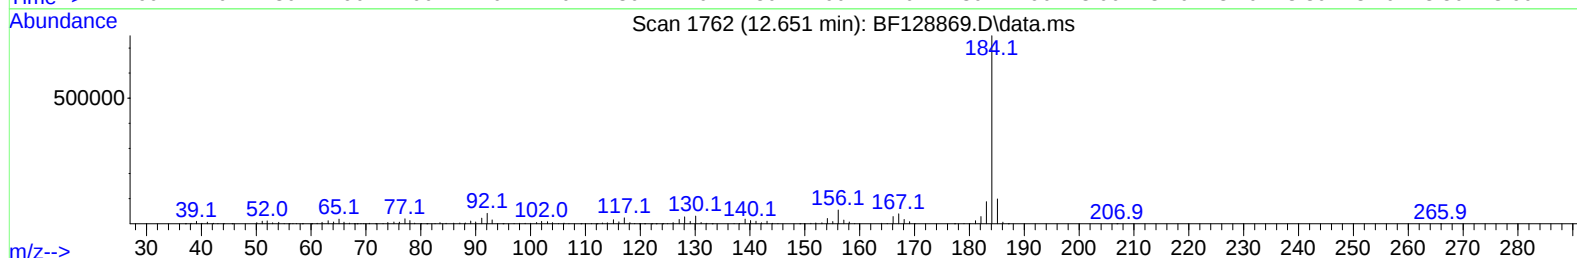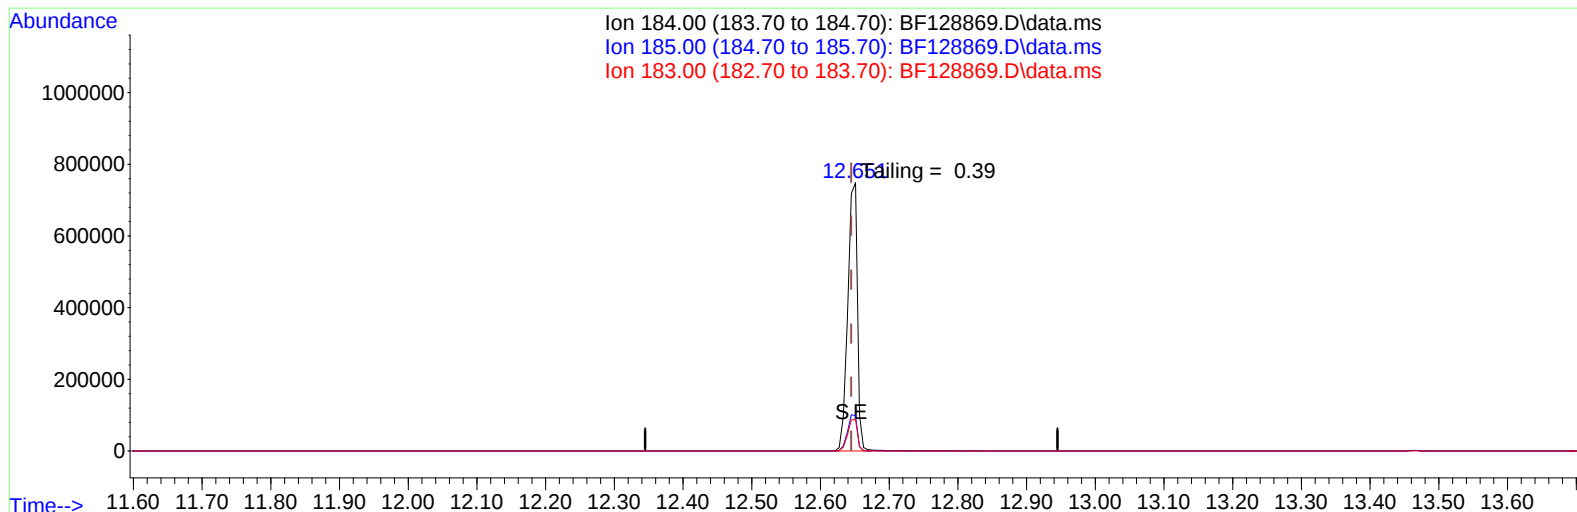

TIC: BF128869.D\data.ms

(77) Benzidine

12.651min (+ 0.006) 488575.18 ng

response 720722

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.17
183.00	11.60	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/20/2022	BNA_F	<u>BF128869.D</u>
Compound Name	Response	Retention Time
DDT	345549	13.46
DDD	10649	13.163
DDE	748	12.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11397	356946	3.19

Instrument :
BNA_F
ClientSampleId :
DFTPP