
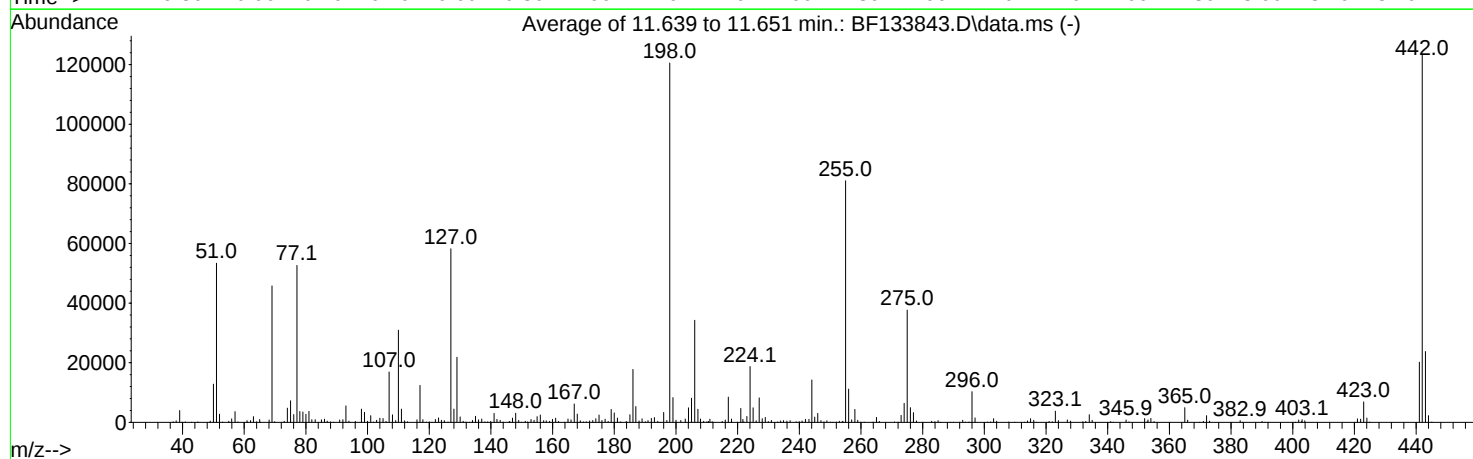


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062023\
 Data File : BF133843.D
 Acq On : 20 Jun 2023 07:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 13:43:46 2023

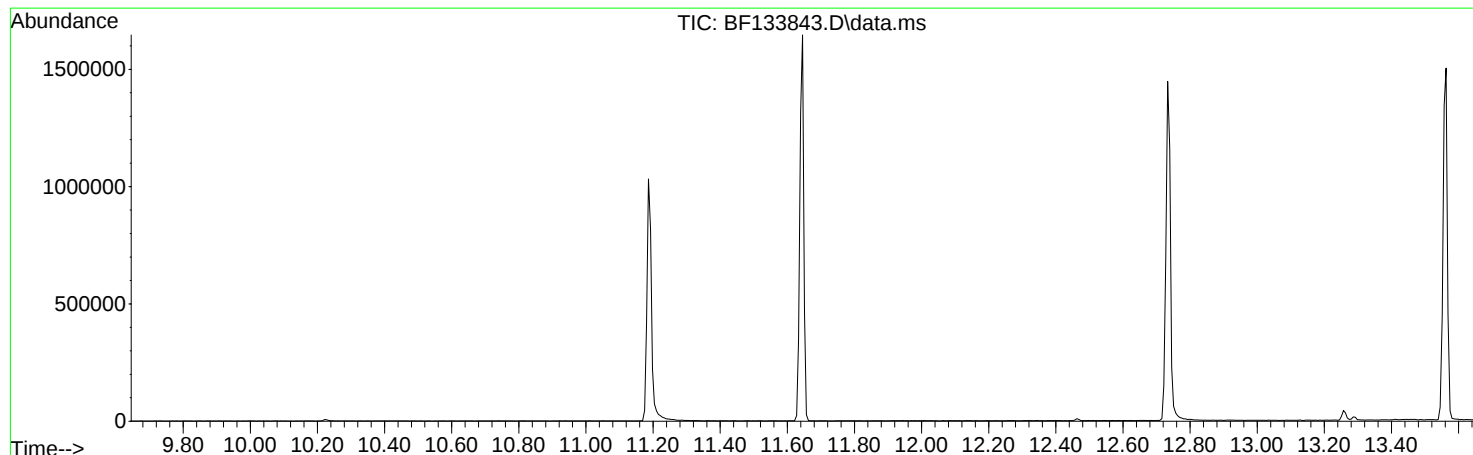




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	53392	PASS
68	69	0.00	2	1.7	782	PASS
69	198	0.00	100	38.0	45765	PASS
70	69	0.00	2	0.4	200	PASS
127	198	10	80	48.3	58224	PASS
197	198	0.00	2	0.5	647	PASS
198	198	100	100	100.0	120563	PASS
199	198	5	9	6.9	8315	PASS
275	198	10	60	31.3	37683	PASS
365	198	1	100	4.1	4921	PASS
441	198	0.01	100	16.8	20202	PASS
442	442	50	100	100.0	123397	PASS
443	442	15	24	19.3	23805	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062023\
Data File : BF133843.D
Acq On : 20 Jun 2023 07:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 20 09:07:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 19 16:00:59 2023
Response via : Initial Calibration

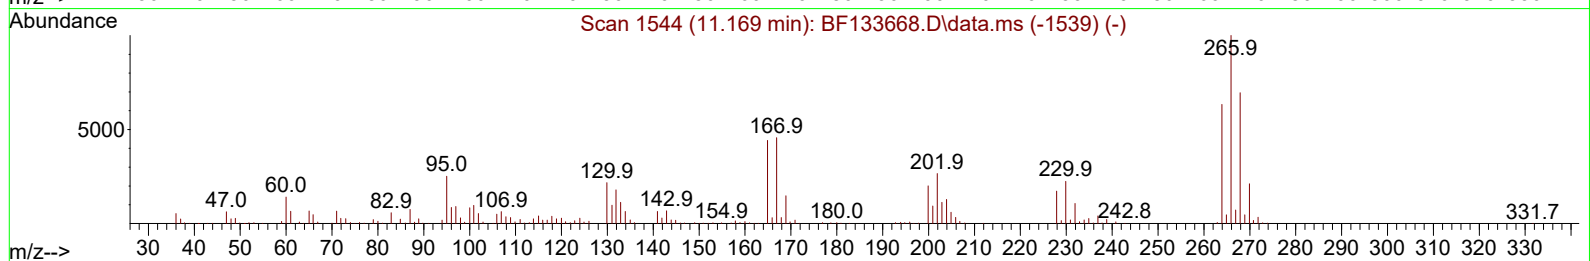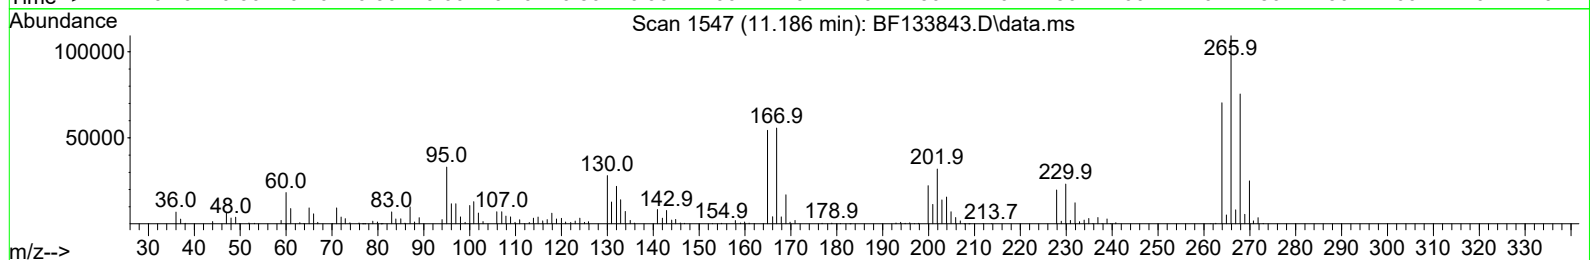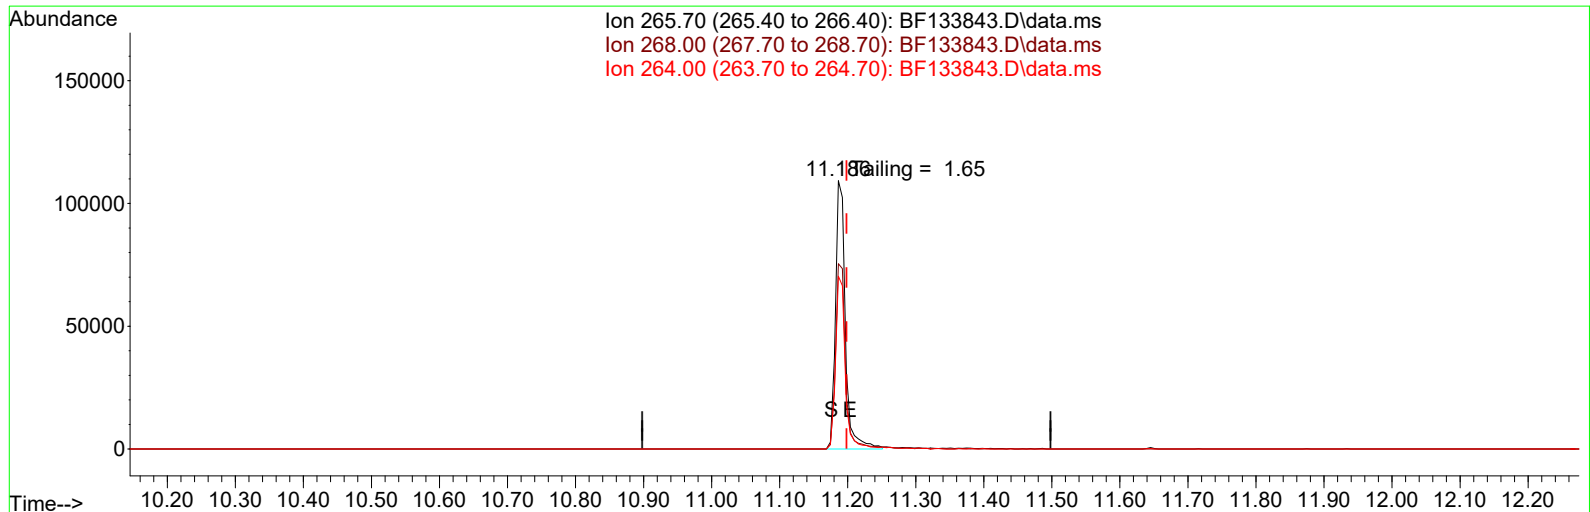

TIC: BF133843.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.012) 26565.04 ng




response 111089

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	69.04
264.00	63.40	64.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062023\
Data File : BF133843.D
Acq On : 20 Jun 2023 07:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 20 09:07:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 19 16:00:59 2023
Response via : Initial Calibration

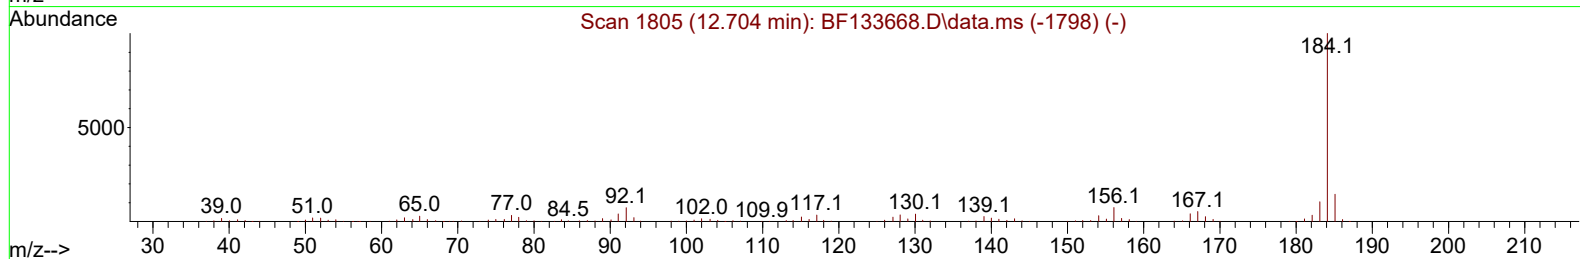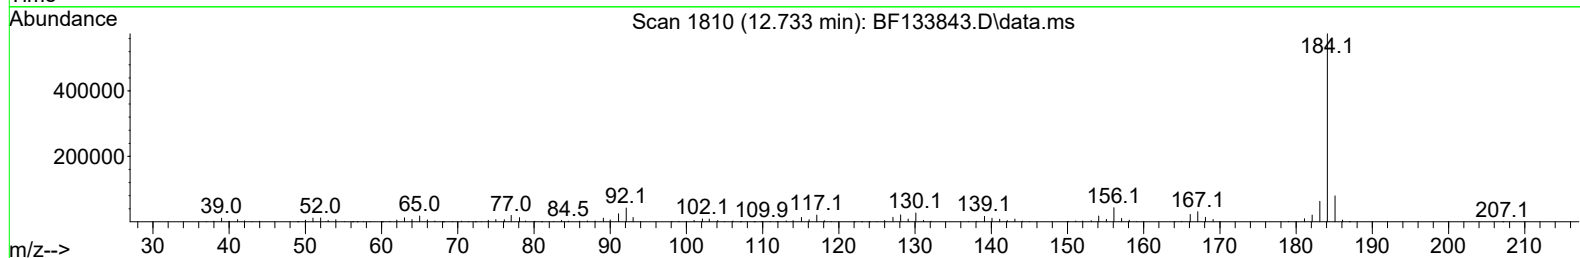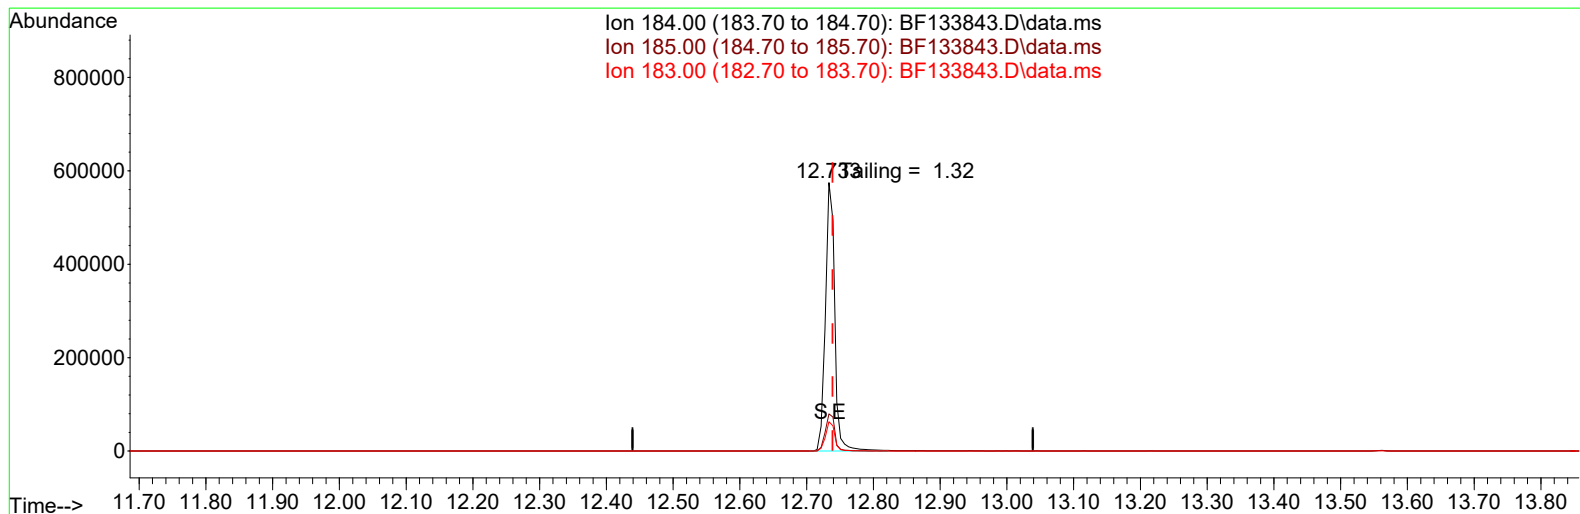

TIC: BF133843.D\data.ms

(77) Benzidine

12.733min (-0.006) 0.00 ng

response 556289

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.84
183.00	10.50	10.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/20/2023	BNA_F	<u>BF133843.D</u>
Compound Name	Response	Retention Time
DDT	261674	13.563
DDD	10123	13.257
DDE	372	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10495	272169	3.86

Instrument :
BNA_F
ClientSampleId :
DFTPP