

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062116\
 Data File : BF088245.D
 Acq On : 22 Jun 2016 7:51
 Operator : UM/SJ
 Sample : H3633-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P0-010

Quant Time: Jun 22 08:32:42 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 17:39:32 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.65	152	84560	20.00	ng	-0.02
21) Naphthalene-d8	7.93	136	333253	20.00	ng	-0.02
38) Acenaphthene-d10	9.68	164	152713	20.00	ng	-0.02
63) Phenanthrene-d10	11.16	188	282900	20.00	ng	-0.01
75) Chrysene-d12	13.79	240	211437	20.00	ng	-0.01
86) Perylene-d12	15.17	264	162682	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.23	112	292928	59.22	ng	-0.02
7) Phenol-d6	6.30	99	234507	39.12	ng	-0.03
23) Nitrobenzene-d5	7.22	82	452310	79.26	ng	-0.02
41) 2,4,6-Tribromophenol	10.48	330	178458	110.67	ng	-0.01
44) 2-Fluorobiphenyl	9.02	172	852543	87.89	ng	-0.02
78) Terphenyl-d14	12.74	244	735379	79.14	ng	-0.02
Target Compounds						Qvalue
9) Benzaldehyde	6.42	77	10419	2.54	ng	# 79
10) Phenol	6.32	94	1075	Below	Cal	# 1
19) n-Nitroso-di-n-propylamine	7.22	70	59009	15.39	ng	# 70
25) Isophorone	7.22	82	357787	33.85	ng	# 65
45) 1,1'-Biphenyl	9.02	154	1707	Below	Cal	# 1
56) 2,4-Dinitrotoluene	9.68	165	19414	5.96	ng	# 37
57) Fluorene	10.47	166	7881	Below	Cal	# 85
64) 4,6-Dinitro-2-methylphenol	10.48	198	442	2.40	ng	# 12
66) 4-Bromophenyl-phenylether	10.48	248	11240	3.70	ng	# 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062116\
Data File : BF088245.D
Acq On : 22 Jun 2016 7:51
Operator : UM/SJ
Sample : H3633-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P0-010

Quant Time: Jun 22 08:32:42 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 17:39:32 2016
Response via : Initial Calibration

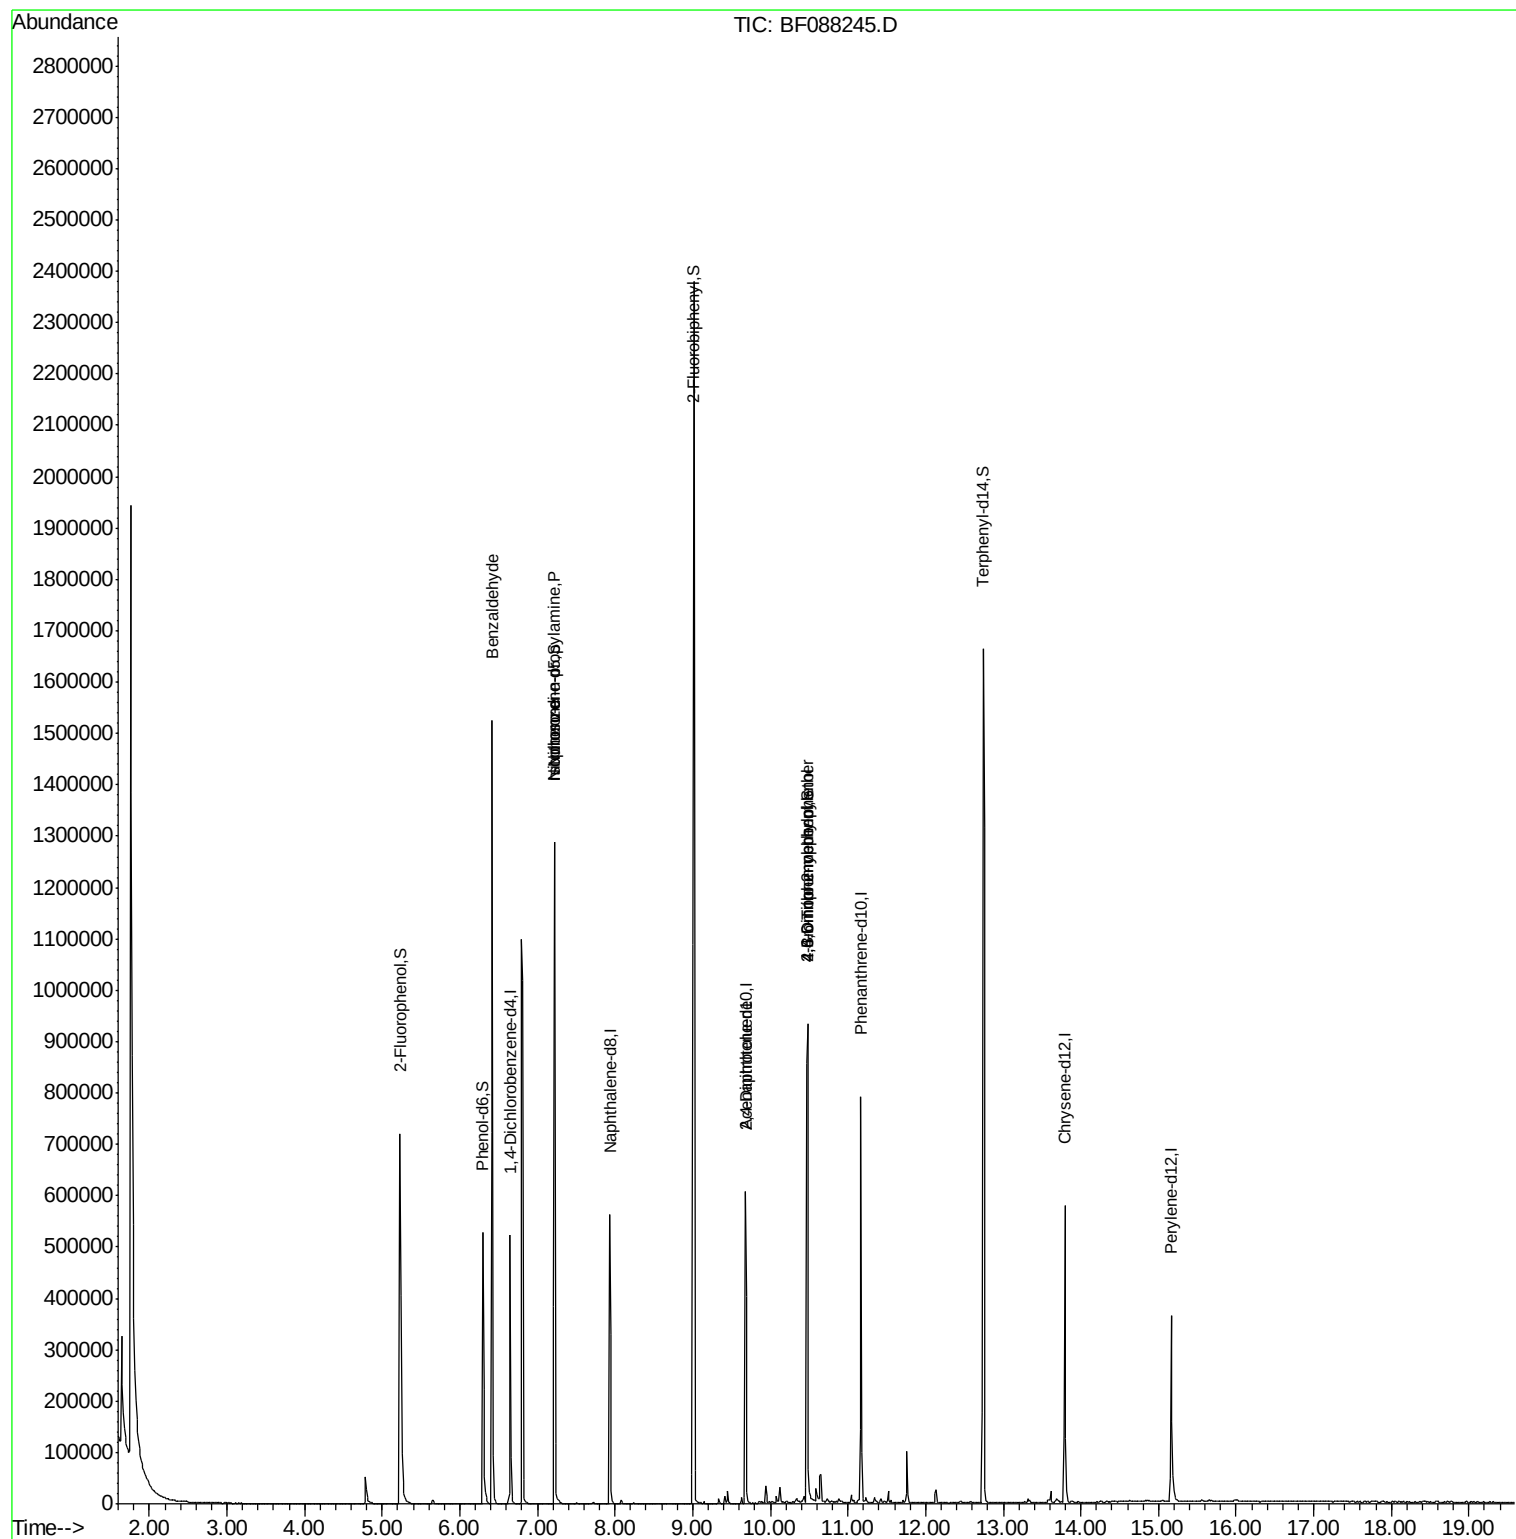

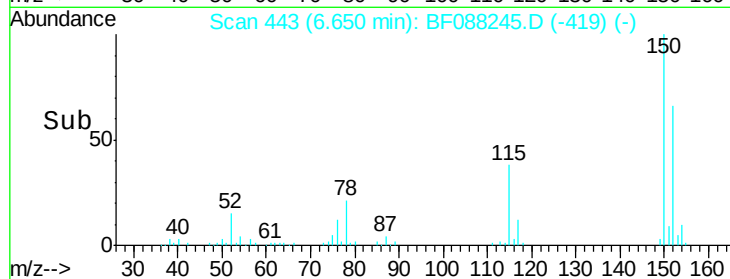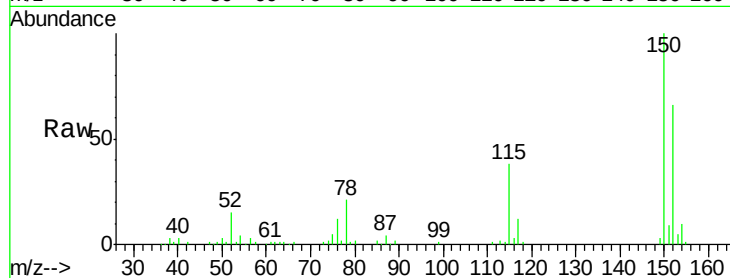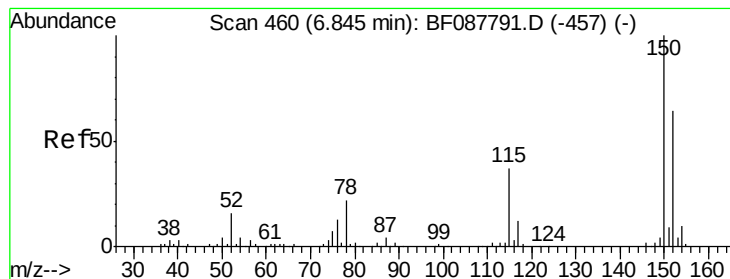

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.65 min Scan# 443

Delta R.T. -0.02 min

Lab File: BF088245.D

Acq: 22 Jun 2016 7:51

Instrument :

BNA_F

ClientSampleId :

P0-010

Tgt Ion:152 Resp: 84560

Ion Ratio Lower Upper

152 100

150 152.2 123.8 185.6

115 57.3 39.6 59.4