
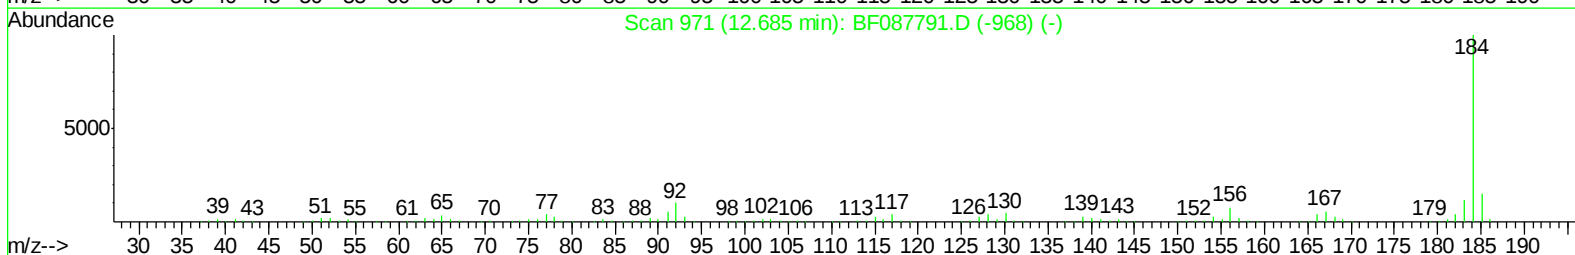
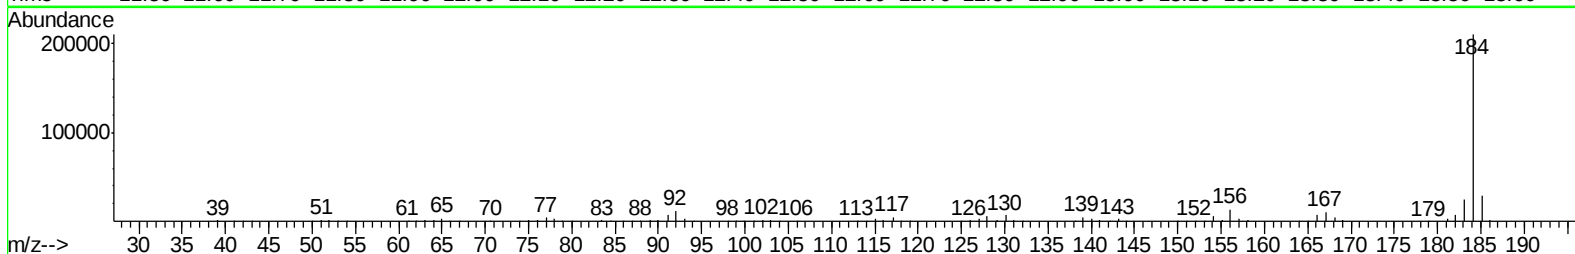


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF062116\  
 Data File : BF088215.D  
 Acq On : 21 Jun 2016 15:53  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 08:14:09 2016  
 Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF060716.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Jun 22 01:34:10 2016  
 Response via : Initial Calibration

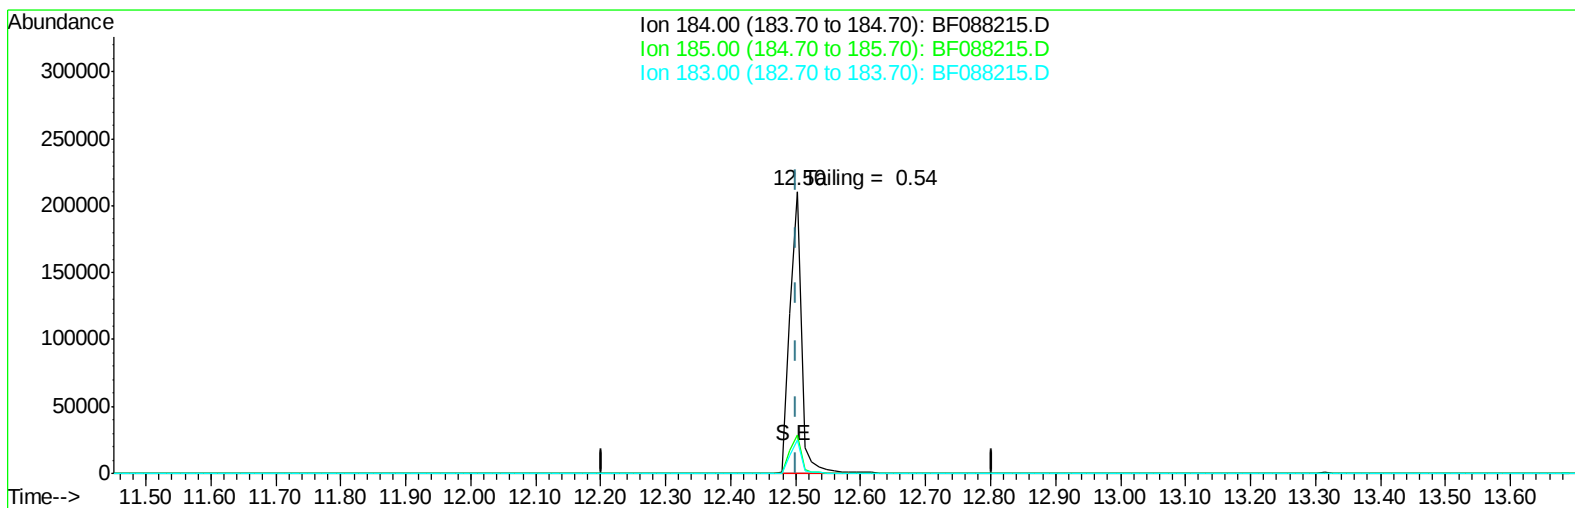

TIC: BF088215.D

(76) Benzidine




12.502min (-0.000) 0.00ng

response 258290

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.60 | 13.57 |
| 183.00 | 11.60 | 11.63 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF062116\  
Data File : BF088215.D  
Acq On : 21 Jun 2016 15:53  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 08:14:09 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF060716.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 22 01:34:10 2016  
Response via : Initial Calibration

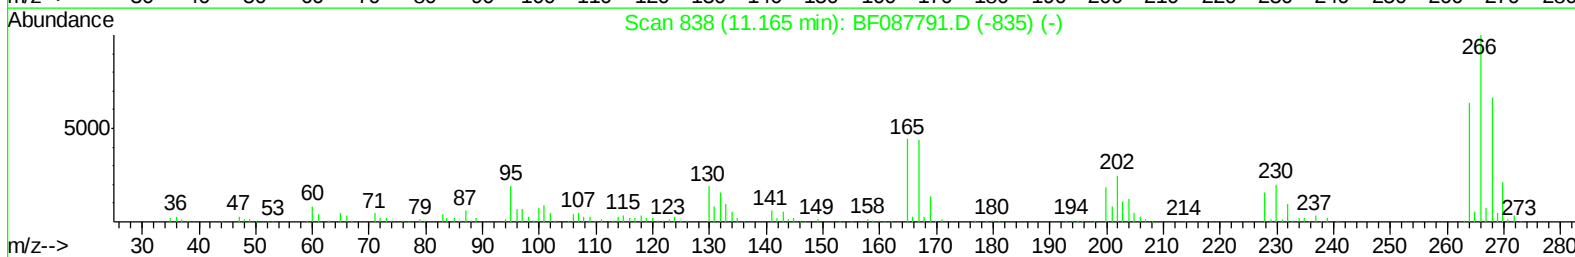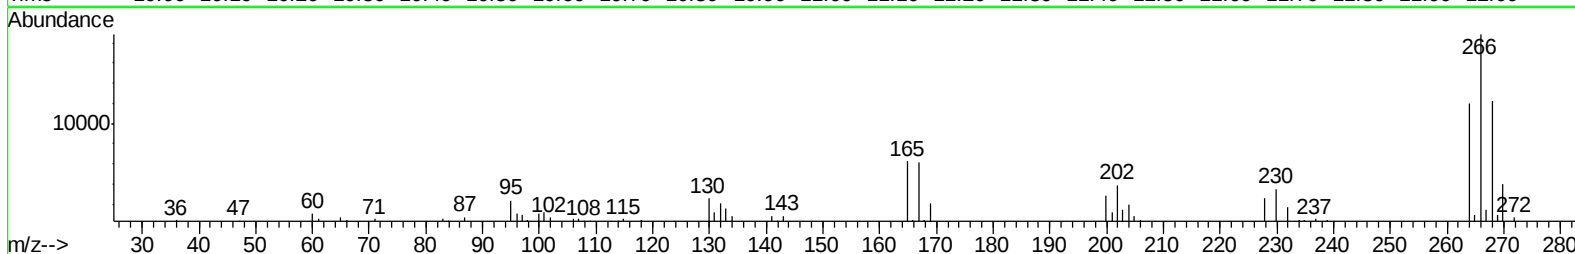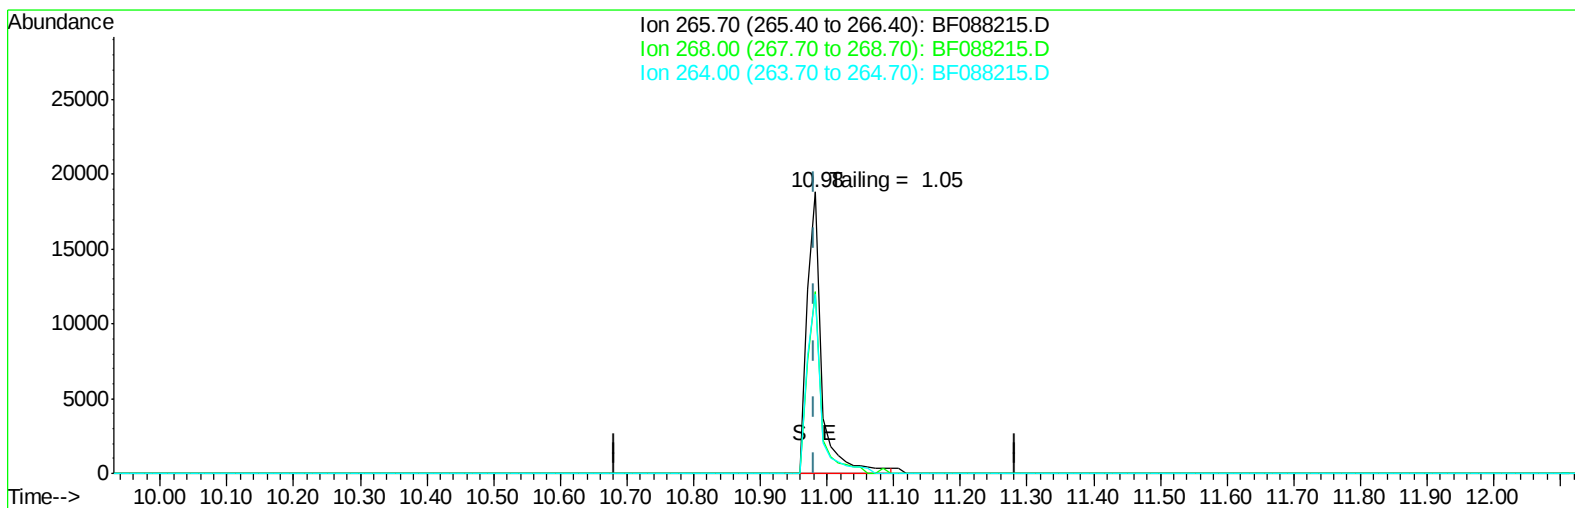

TIC: BF088215.D

(69) Pentachlorophenol (C)

10.982min (-0.000) 0.00ng

response 28532

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.00 | 64.78 |
| 264.00 | 62.00 | 63.87 |
| 0.00   | 0.00  | 0.00  |