


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062116\
 Data File : BF088215.D
 Acq On : 21 Jun 2016 15:53
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 22 14:55:14 2016

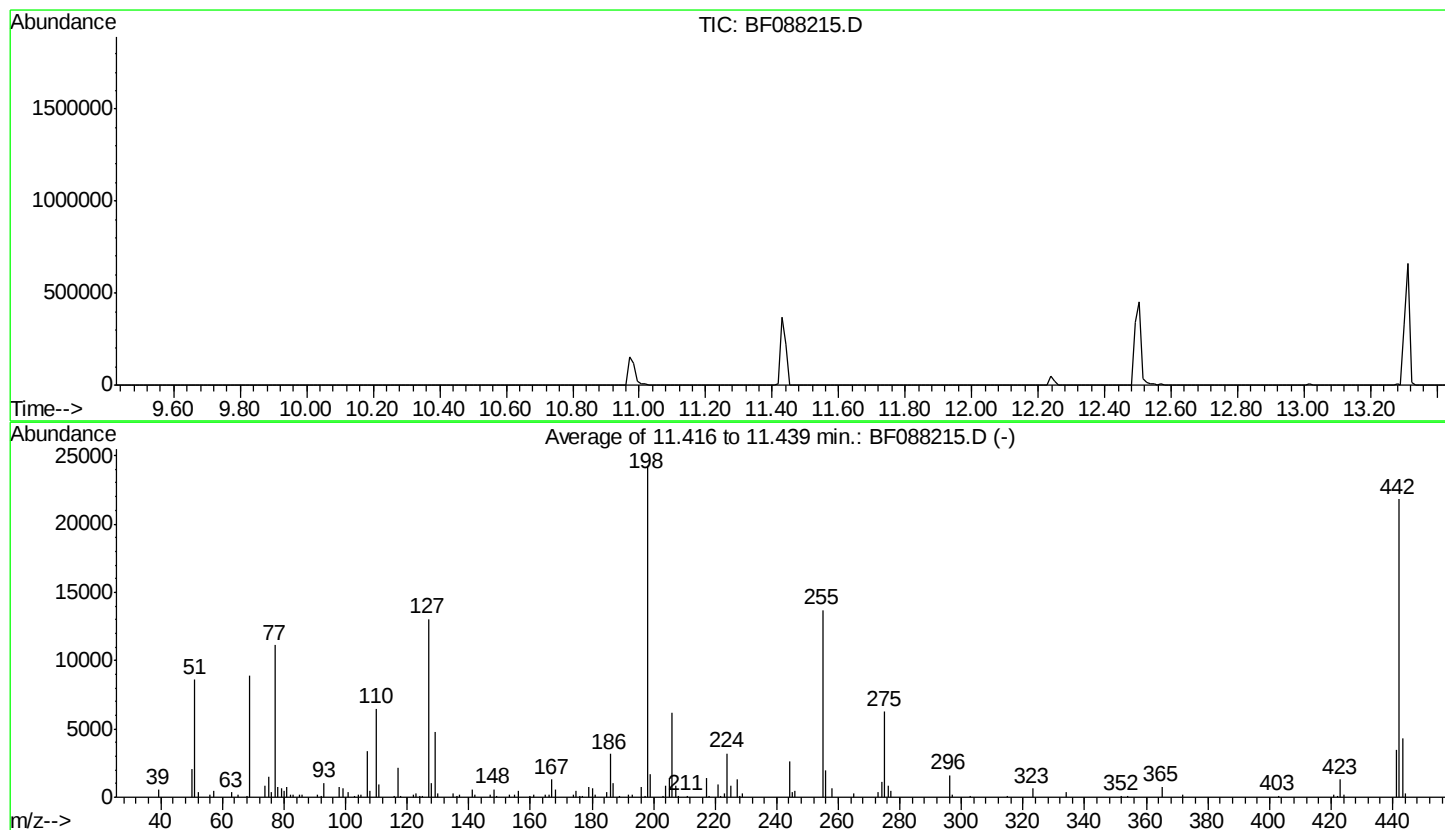

AutoFind: Scans 860, 861, 862; Background Corrected with Scan 857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	8592	PASS
68	69	0.00	2	1.5	133	PASS
69	198	0.00	100	36.8	8937	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.7	13035	PASS
197	198	0.00	2	0.4	109	PASS
198	198	100	100	100.0	24264	PASS
199	198	5	9	6.8	1658	PASS
275	198	10	60	25.7	6245	PASS
365	198	1	100	3.2	768	PASS
441	442	0.01	24	15.8	3442	PASS
442	198	50	100	89.9	21816	PASS
443	442	15	24	19.7	4288	PASS