


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062116\
 Data File : BF088238.D
 Acq On : 22 Jun 2016 4:17
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 22 14:55:14 2016

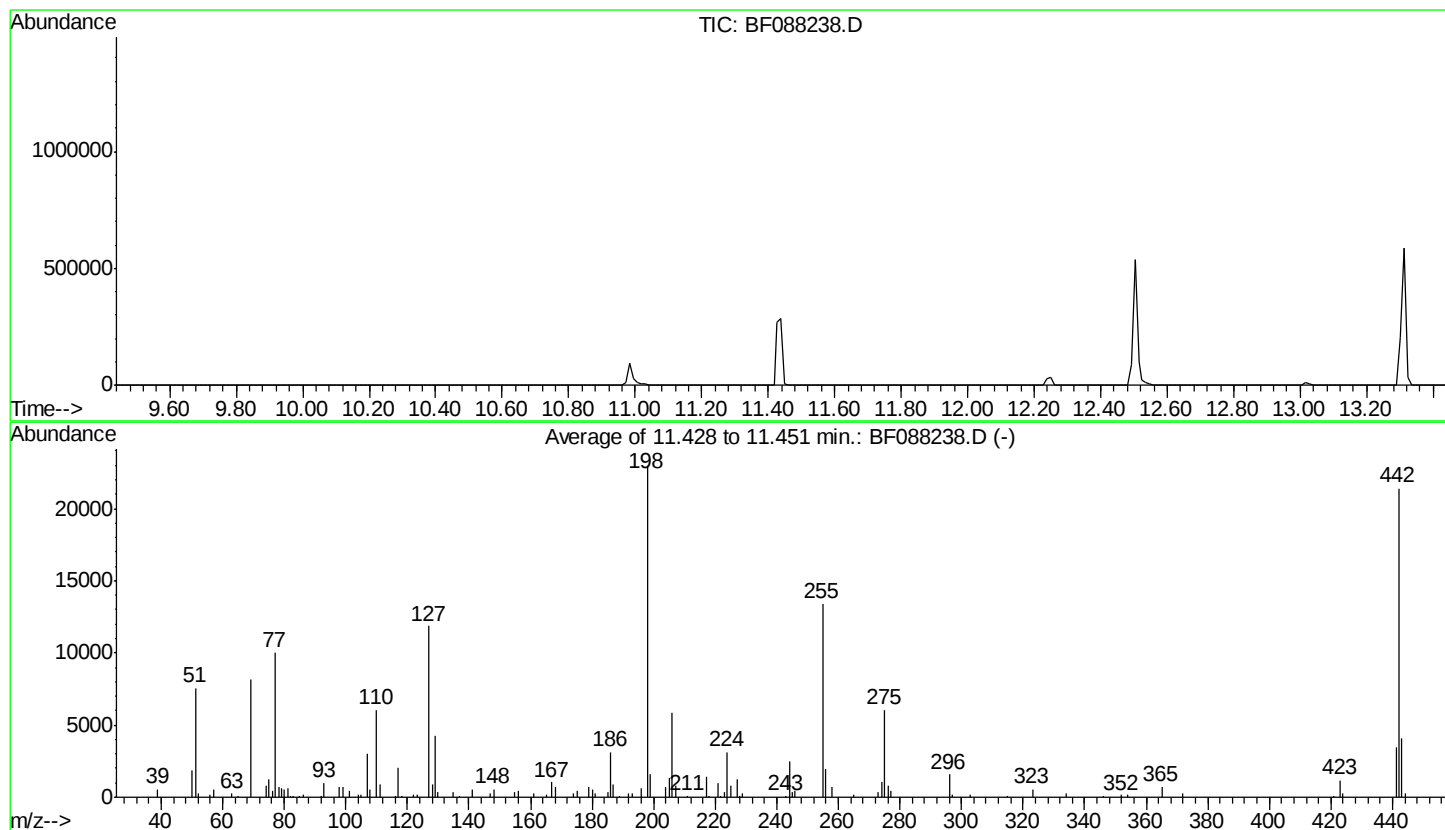

AutoFind: Scans 861, 862, 863; Background Corrected with Scan 857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	7543	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.5	8161	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.6	11851	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22976	PASS
199	198	5	9	6.8	1566	PASS
275	198	10	60	26.4	6075	PASS
365	198	1	100	3.2	737	PASS
441	442	0.01	24	16.0	3438	PASS
442	198	50	100	93.2	21421	PASS
443	442	15	24	19.3	4125	PASS