

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062117\
 Data File : BF096101.D
 Acq On : 22 Jun 2017 00:08
 Operator : SJ/MA
 Sample : I3736-01 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G24-0-1.5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.557	9	12	35	rBV	217756	459114	83.81%	11.189%
2	5.345	650	656	657	rBV3	4883	10744	1.96%	0.262%
3	7.022	935	941	951	rBV4	25210	91571	16.72%	2.232%
4	7.098	952	954	959	rVB4	10415	14592	2.66%	0.356%
5	7.292	983	987	1001	rBV	273333	457215	83.47%	11.142%
6	7.539	1025	1029	1044	rBV	37709	70695	12.91%	1.723%
7	8.292	1153	1157	1158	rBV	6892	8142	1.49%	0.198%
8	9.327	1328	1333	1348	rBV	358735	547773	100.00%	13.349%
9	9.427	1348	1350	1359	rVB2	6073	8179	1.49%	0.199%
10	11.110	1632	1636	1647	rBV	65131	95602	17.45%	2.330%
11	12.145	1807	1812	1827	rBV2	374550	541128	98.79%	13.187%
12	13.004	1953	1958	1963	rVB2	4708	7572	1.38%	0.185%
13	13.486	2035	2040	2047	rBV2	6695	14244	2.60%	0.347%
14	13.792	2083	2092	2096	rBV4	5174	12999	2.37%	0.317%
15	14.539	2215	2219	2233	rVB	320109	469753	85.76%	11.448%
16	15.609	2399	2401	2405	rBV4	3731	5766	1.05%	0.141%
17	15.703	2413	2417	2420	rBV5	5249	7146	1.30%	0.174%
18	15.803	2432	2434	2438	rVB5	5960	6375	1.16%	0.155%
19	16.168	2494	2496	2499	rBV3	7493	7433	1.36%	0.181%
20	16.380	2529	2532	2535	rBV3	19998	28995	5.29%	0.707%
21	16.609	2569	2571	2574	rVB4	9232	7343	1.34%	0.179%
22	16.686	2582	2584	2586	rBV2	11197	10657	1.95%	0.260%
23	16.803	2601	2604	2606	rVB4	14634	16216	2.96%	0.395%
24	16.921	2620	2624	2634	rVB	100810	164852	30.09%	4.017%
25	17.115	2652	2657	2659	rBV6	21840	35584	6.50%	0.867%
26	17.445	2711	2713	2714	rBV2	19618	12849	2.35%	0.313%
27	17.474	2717	2718	2723	rVV4	22849	34370	6.27%	0.838%
28	17.986	2803	2805	2806	rVB2	25652	15332	2.80%	0.374%
29	18.050	2814	2816	2818	rVB3	26127	17679	3.23%	0.431%
30	18.274	2850	2854	2858	rBV	394634	456083	83.26%	11.115%
31	19.944	3135	3138	3146	rVB2	287135	467361	85.32%	11.390%


Sum of corrected areas: 4103364

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062117\
Data File : BF096101.D
Acq On : 22 Jun 2017 00:08
Operator : SJ/MA
Sample : I3736-01 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G24-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

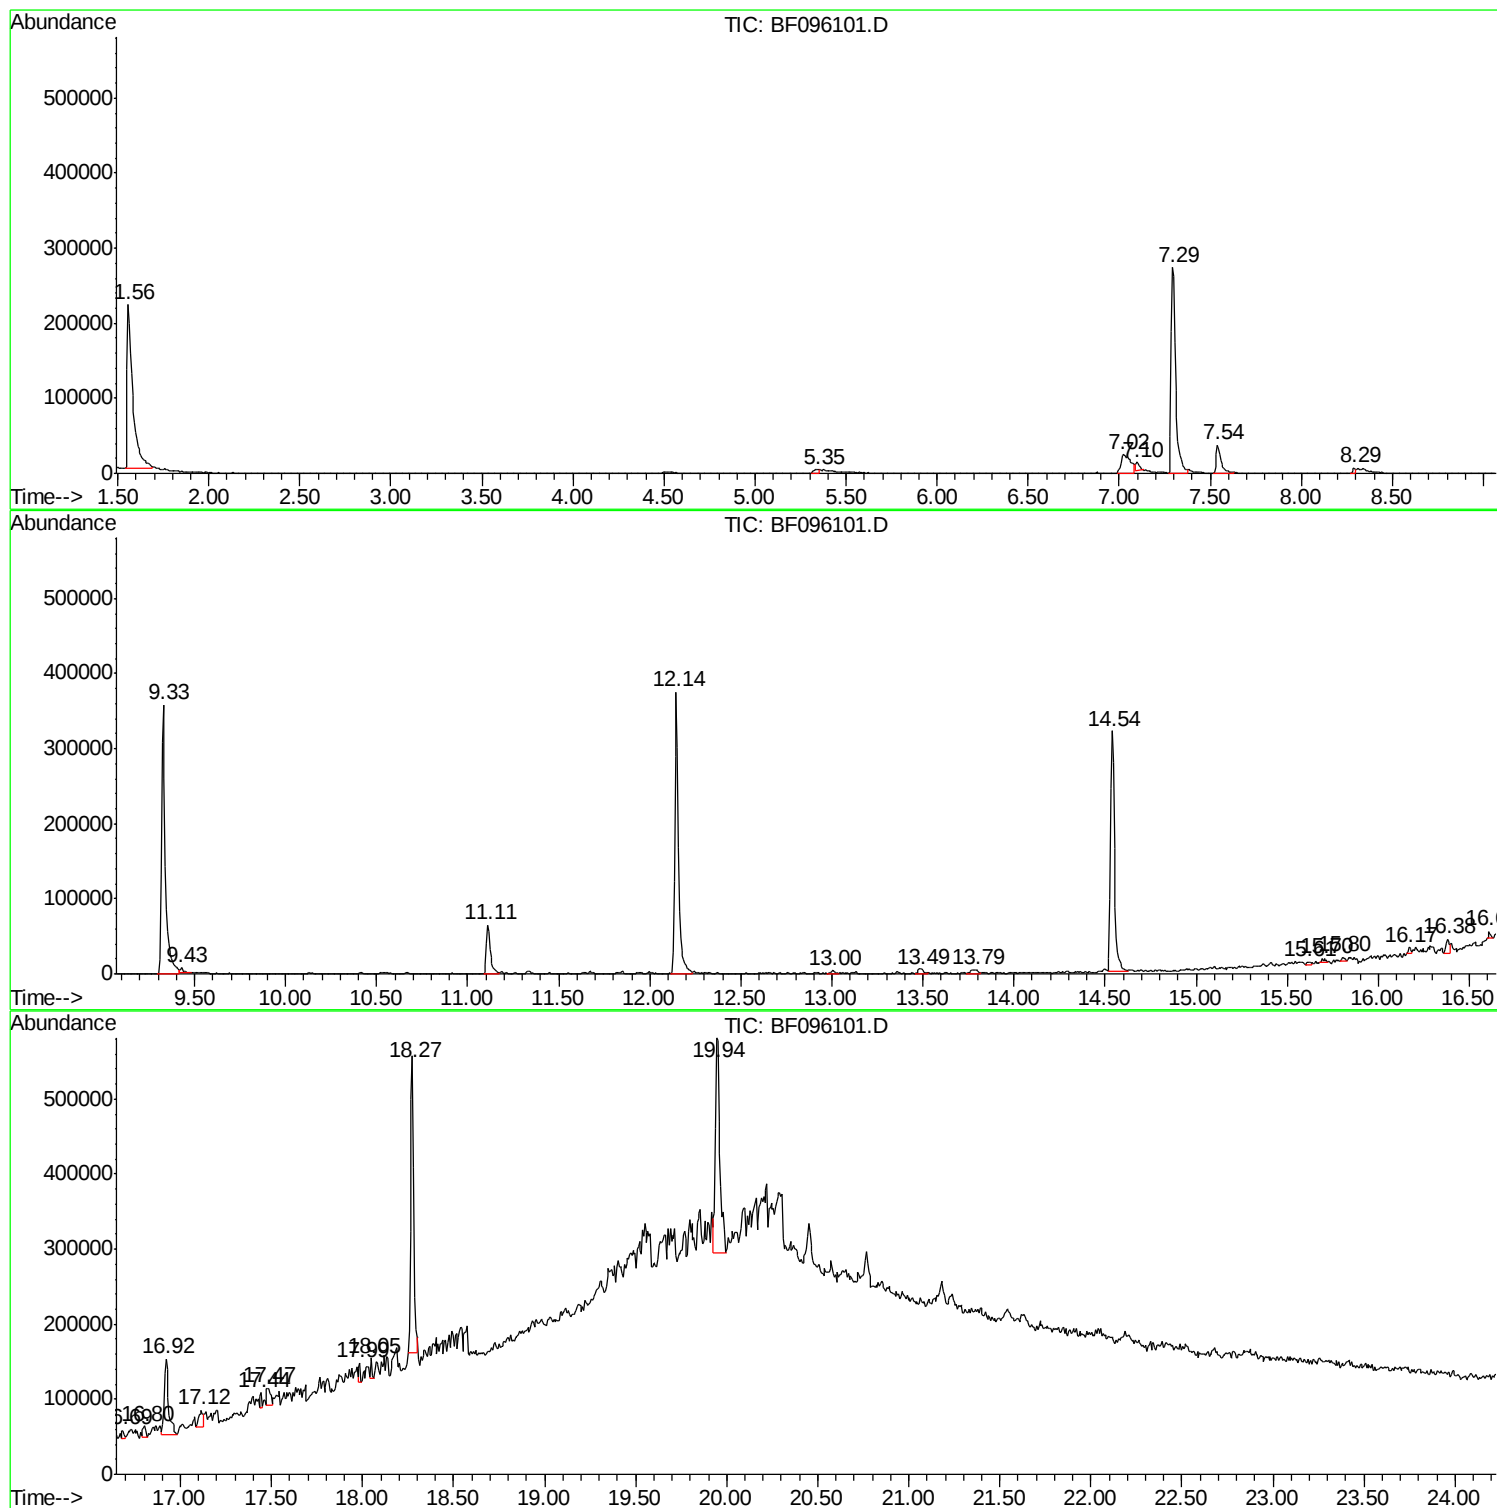

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF062117\
Data_File : BF096101.D
Acq_On : 22-Jun-2017 00:088
Operator : SJ/MAA
Sample : I3736-01_10XX
Misc :
ALS_Vial : 22 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
G24-0-1.5

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
