

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
 Data File : BF124393.D
 Acq On : 21 Jun 2021 14:55
 Operator : JU/CG
 Sample : M2773-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.992	492	494	501	rBB	10698	12820	1.58%	0.231%
2	5.410	562	565	582	rBV	651531	646086	79.46%	11.655%
3	6.428	735	738	751	rBV	730156	646716	79.53%	11.666%
4	6.786	795	799	804	rBB	231615	204023	25.09%	3.680%
5	7.351	891	895	898	rBV	503140	425540	52.33%	7.676%
6	7.980	999	1002	1006	rBV3	11311	15758	1.94%	0.284%
7	8.069	1013	1017	1022	rBV	320233	259303	31.89%	4.677%
8	9.145	1196	1200	1203	rBV	1045162	804507	98.94%	14.512%
9	9.263	1217	1220	1223	rBV	18555	14122	1.74%	0.255%
10	9.821	1312	1315	1319	rBV	398682	313379	38.54%	5.653%
11	10.616	1446	1450	1458	rBV	688957	585370	71.99%	10.559%
12	11.310	1565	1568	1575	rVB	414641	333039	40.96%	6.008%
13	12.898	1834	1838	1841	rBV	1018672	813137	100.00%	14.668%
14	13.957	2014	2018	2025	rVB	284820	235408	28.95%	4.246%
15	15.415	2261	2266	2276	rBV	189370	234425	28.83%	4.229%




Sum of corrected areas: 5543633

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124393.D
Acq On : 21 Jun 2021 14:55
Operator : JU/CG
Sample : M2773-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

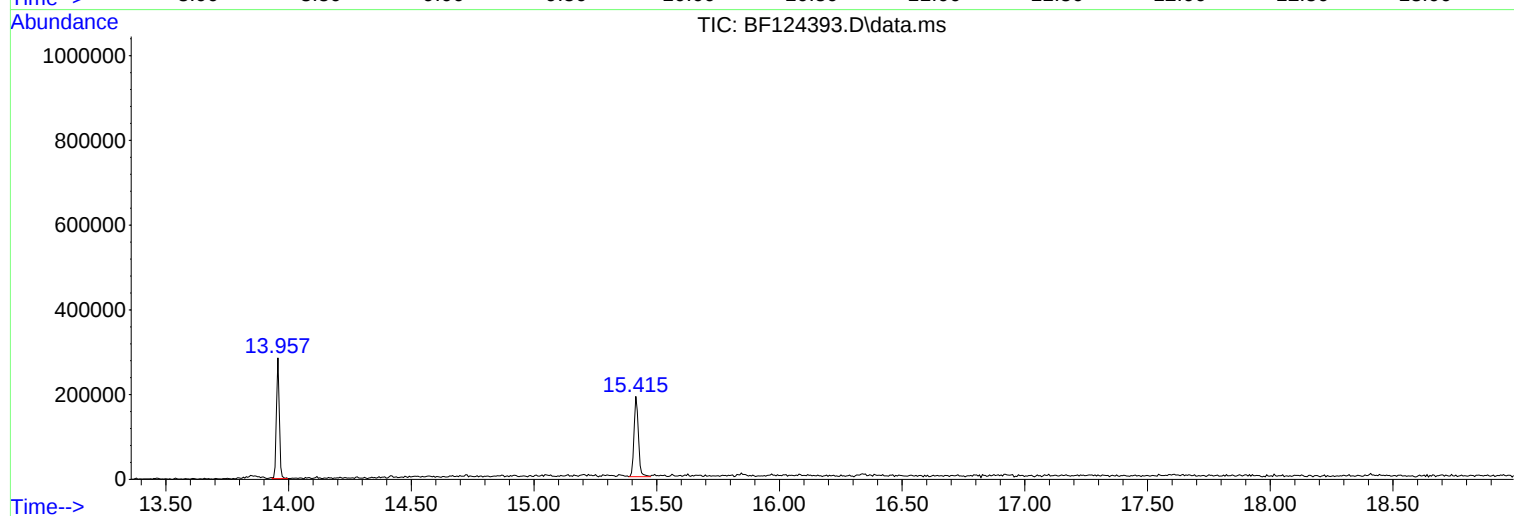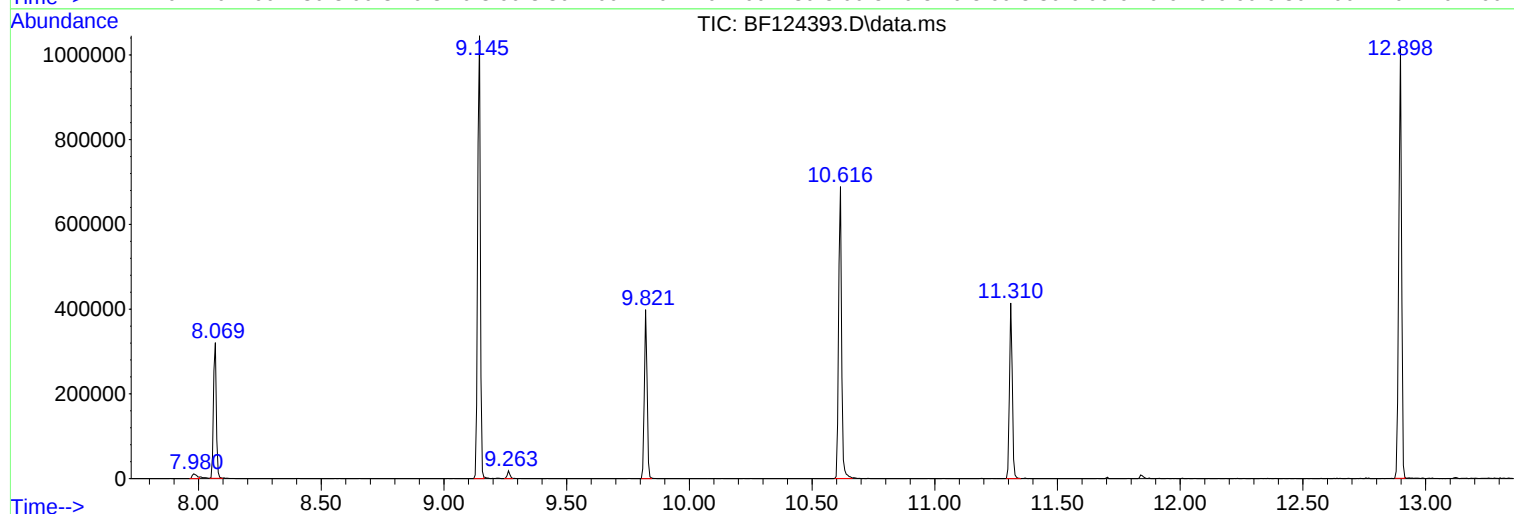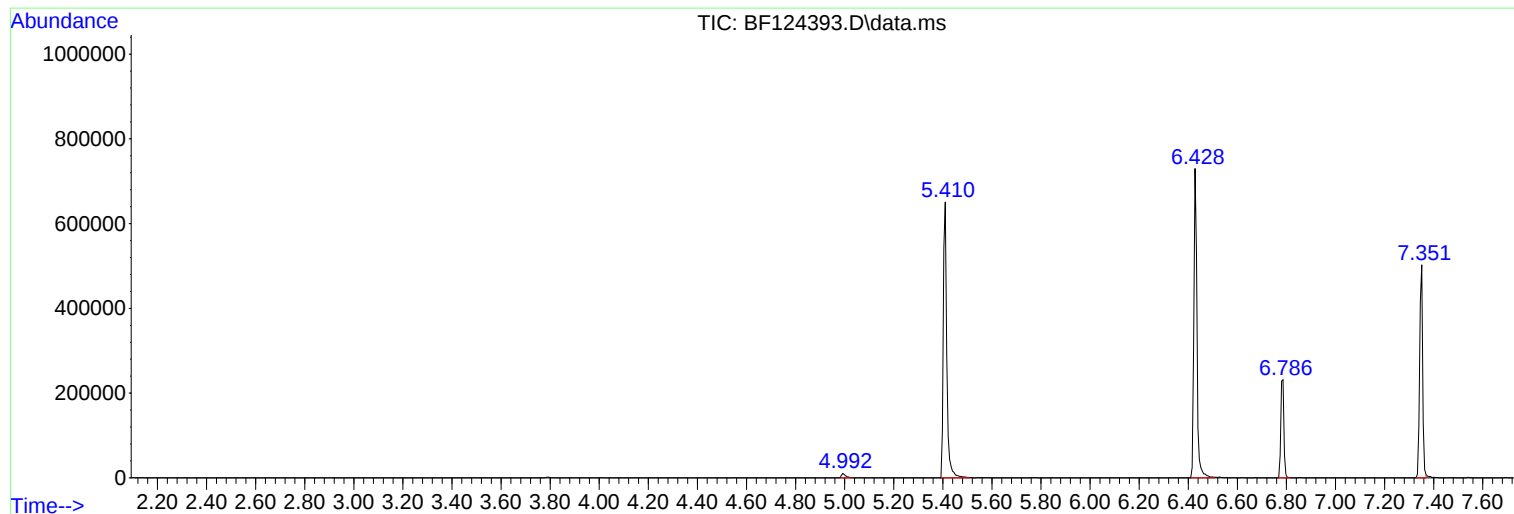

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124393.D
Acq On : 21 Jun 2021 14:55
Operator : JU/CG
Sample : M2773-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124393.D
Acq On : 21 Jun 2021 14:55
Operator : JU/CG
Sample : M2773-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
