

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
 Data File : BF124394.D
 Acq On : 21 Jun 2021 15:29
 Operator : JU/CG
 Sample : M2773-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.992	492	494	500	rBV2	9108	12362	1.61%	0.239%
2	5.410	561	565	578	rBV	574007	610725	79.67%	11.794%
3	6.428	735	738	750	rBV	678707	603353	78.71%	11.652%
4	6.786	795	799	804	rBB	224682	199095	25.97%	3.845%
5	7.351	891	895	898	rBV	485528	398763	52.02%	7.701%
6	8.069	1013	1017	1022	rVB	304234	252574	32.95%	4.878%
7	9.145	1196	1200	1203	rBV	1020794	766541	100.00%	14.804%
8	9.822	1312	1315	1321	rVB	390115	303075	39.54%	5.853%
9	10.616	1446	1450	1459	rBV	631120	534655	69.75%	10.325%
10	11.310	1565	1568	1572	rBV	360816	315249	41.13%	6.088%
11	12.898	1834	1838	1841	rBV	895061	727814	94.95%	14.056%
12	13.957	2015	2018	2022	rBV	240999	213529	27.86%	4.124%
13	15.415	2262	2266	2278	rBV	182099	240362	31.36%	4.642%




Sum of corrected areas: 5178097

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124394.D
Acq On : 21 Jun 2021 15:29
Operator : JU/CG
Sample : M2773-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

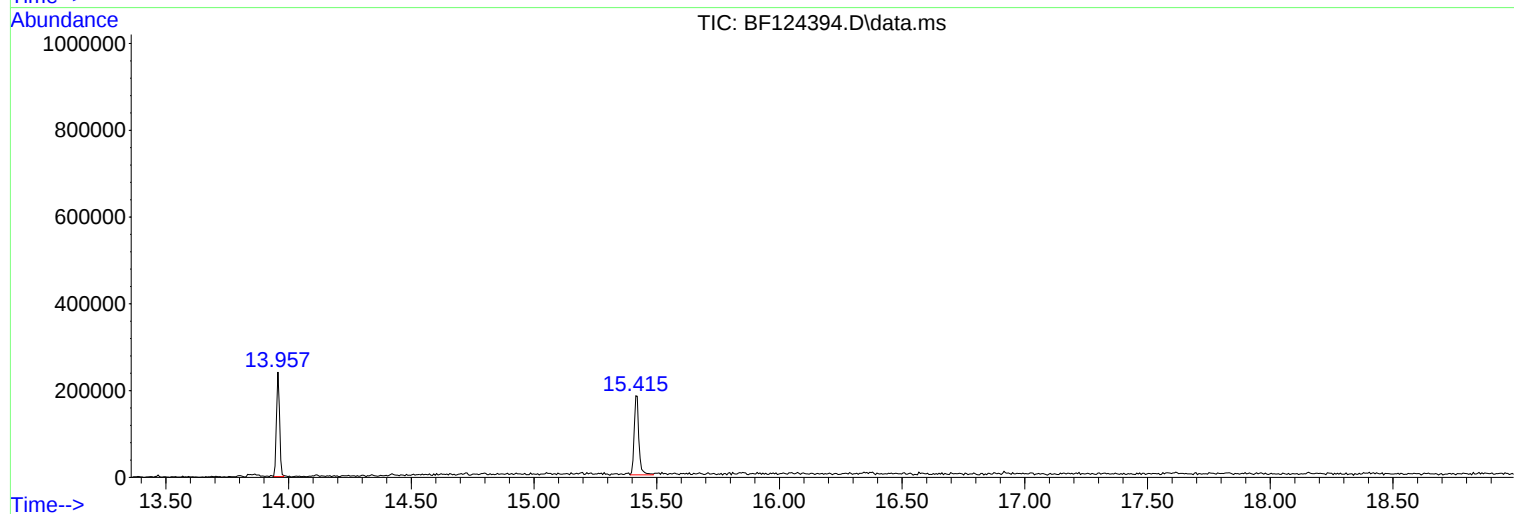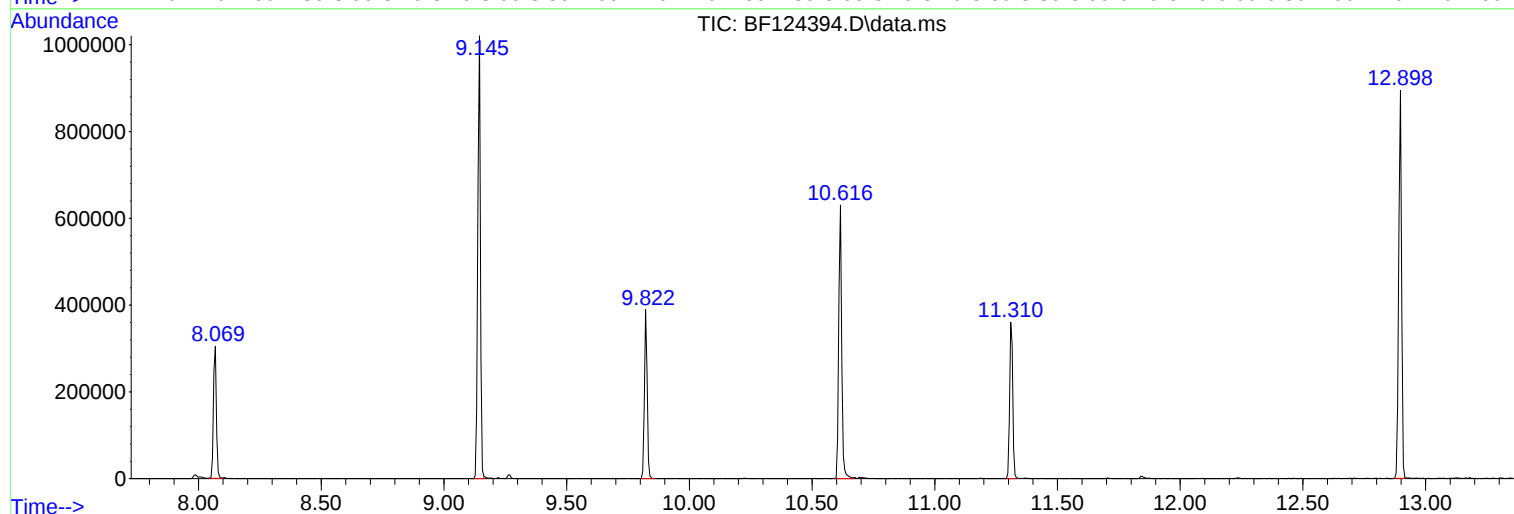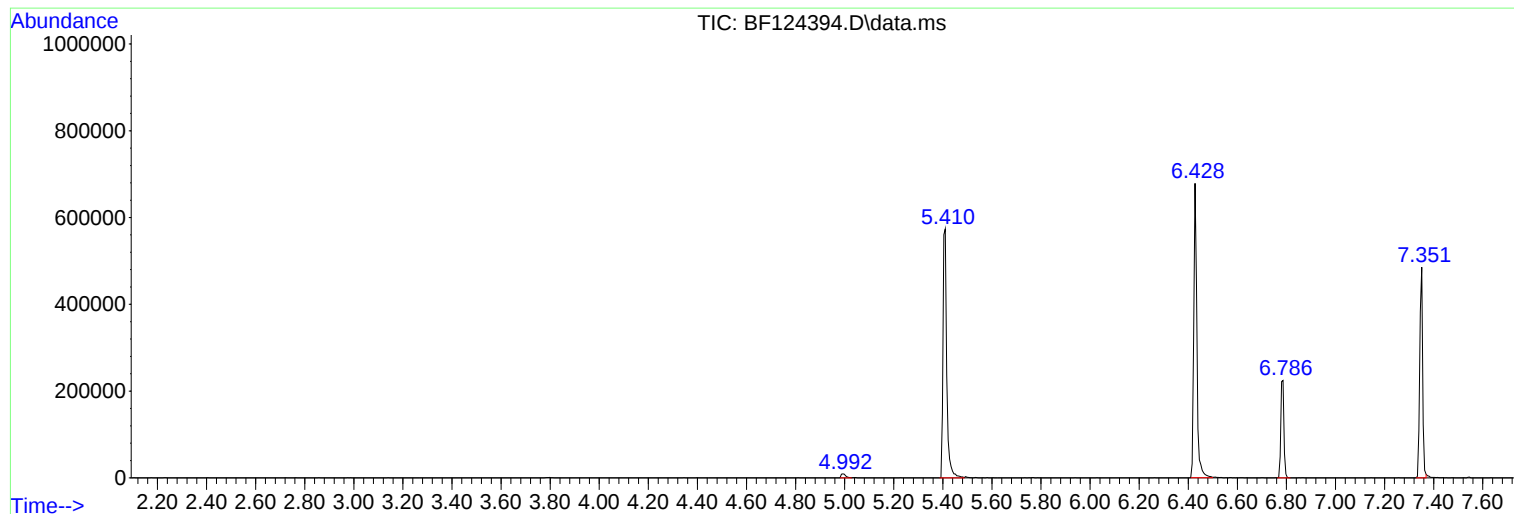

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124394.D
Acq On : 21 Jun 2021 15:29
Operator : JU/CG
Sample : M2773-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124394.D
Acq On : 21 Jun 2021 15:29
Operator : JU/CG
Sample : M2773-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
