

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
 Data File : BF124402.D
 Acq On : 21 Jun 2021 20:02
 Operator : JU/CG
 Sample : M2772-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124402.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.998	492	495	501	rBV2	14067	17691	1.53%	0.236%
2	5.410	561	565	577	rBV	915078	837046	72.36%	11.156%
3	6.434	735	739	752	rBV	935249	906264	78.35%	12.079%
4	6.781	795	798	805	rBB	236392	201797	17.45%	2.690%
5	7.351	891	895	898	rBV	690788	545520	47.16%	7.271%
6	7.975	998	1001	1008	rBV	91952	90019	7.78%	1.200%
7	8.069	1013	1017	1021	rVB	303473	262791	22.72%	3.503%
8	9.145	1196	1200	1203	rBV	1435377	1066153	92.17%	14.210%
9	9.822	1312	1315	1319	rBV	412090	311534	26.93%	4.152%
10	10.616	1446	1450	1459	rBV	863239	732440	63.32%	9.762%
11	11.310	1564	1568	1571	rBV	381433	313109	27.07%	4.173%
12	11.333	1571	1572	1575	rVB	42108	25727	2.22%	0.343%
13	11.698	1632	1634	1637	rBB2	20363	16874	1.46%	0.225%
14	11.839	1656	1658	1662	rBV	14093	15191	1.31%	0.202%
15	12.410	1749	1755	1759	rVB	26537	27607	2.39%	0.368%
16	12.527	1771	1775	1780	rVB	101660	83841	7.25%	1.117%
17	12.710	1803	1806	1809	rBV	35141	31554	2.73%	0.421%
18	12.757	1809	1814	1819	rVB	85933	84347	7.29%	1.124%
19	12.898	1834	1838	1841	rBV	1380143	1156732	100.00%	15.417%
20	12.921	1841	1842	1847	rVB	36032	17905	1.55%	0.239%
21	13.433	1926	1929	1932	rBV	22384	20190	1.75%	0.269%
22	13.957	2010	2018	2021	rBV	263128	251194	21.72%	3.348%
23	13.980	2021	2022	2028	rVB	31190	29787	2.58%	0.397%
24	14.992	2191	2194	2198	rBV2	35237	55807	4.82%	0.744%
25	15.292	2243	2245	2249	rBV2	21497	22827	1.97%	0.304%
26	15.357	2252	2256	2261	rBV2	32953	38679	3.34%	0.516%
27	15.415	2261	2266	2278	rVB	211005	274764	23.75%	3.662%
28	16.874	2509	2514	2519	rBV4	20839	38077	3.29%	0.507%
29	17.315	2583	2589	2594	rBV4	14154	27474	2.38%	0.366%




Sum of corrected areas: 7502941

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124402.D
Acq On : 21 Jun 2021 20:02
Operator : JU/CG
Sample : M2772-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
SB-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

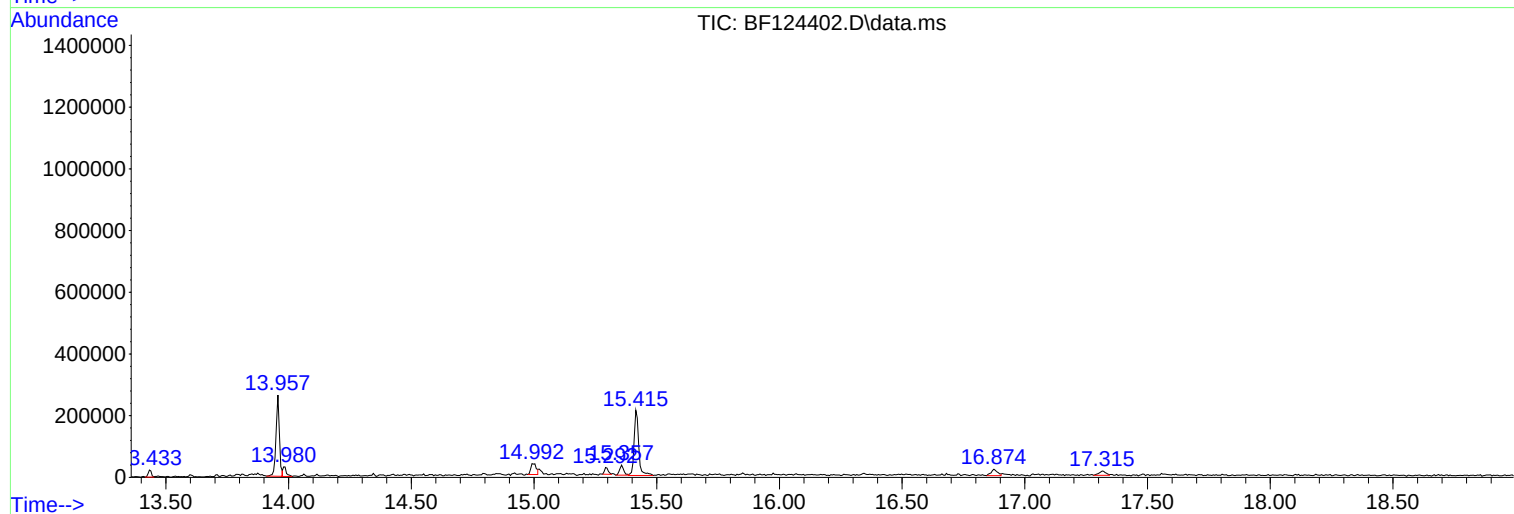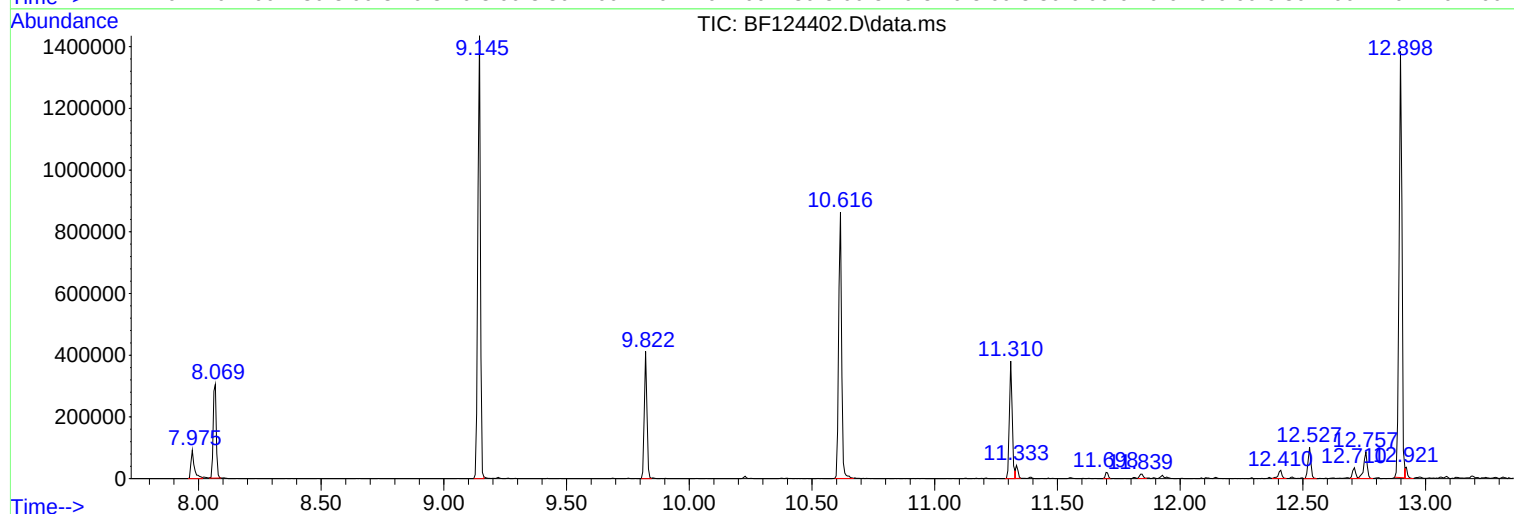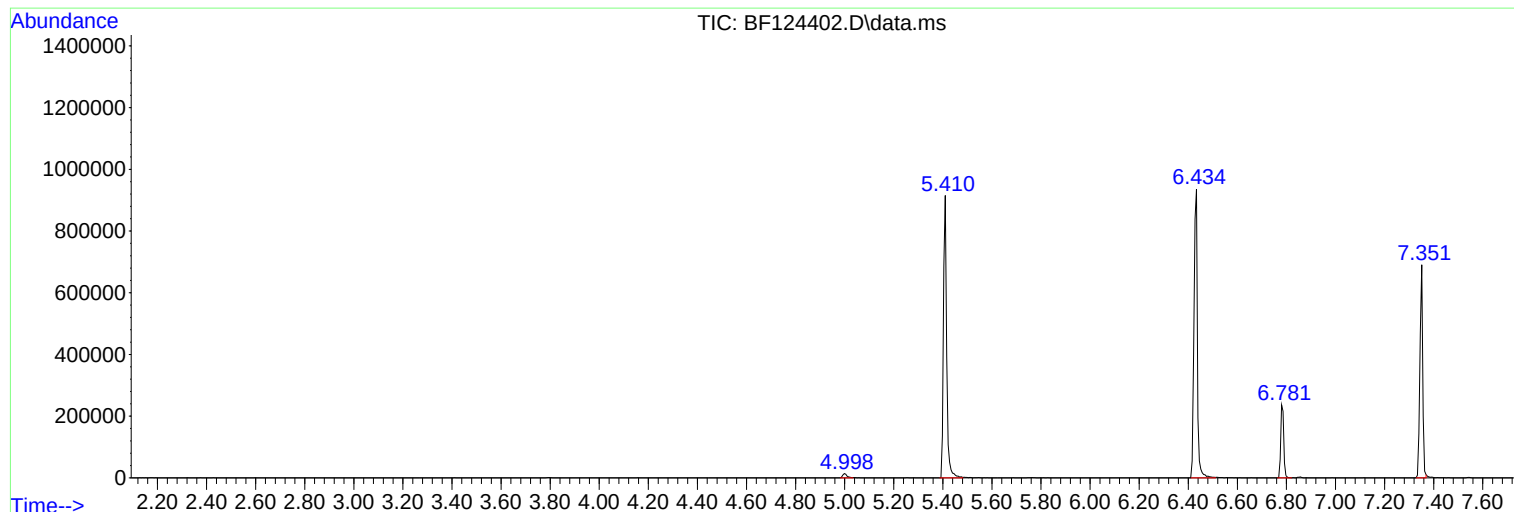

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124402.D
Acq On : 21 Jun 2021 20:02
Operator : JU/CG
Sample : M2772-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
SB-2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.975	6.85 ng	90019	Naphthalene-d8	8.069

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	86
3			2-Propanol, 1-(2-butoxyethoxy)-	176	C9H20O3	000124-16-3	83
4			Butane, 1,1'-[oxybis(2,1-ethaned...	218	C12H26O3	000112-73-2	56
5			Ethylene glycol monoisobutyl ether	118	C6H14O2	004439-24-1	45

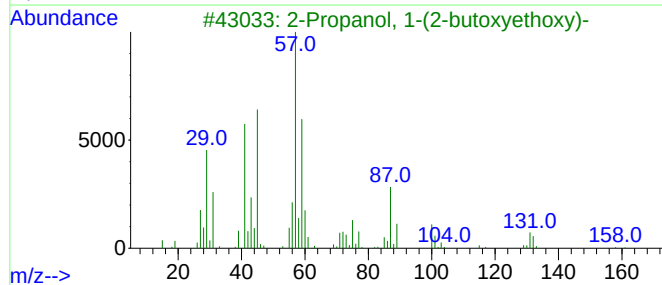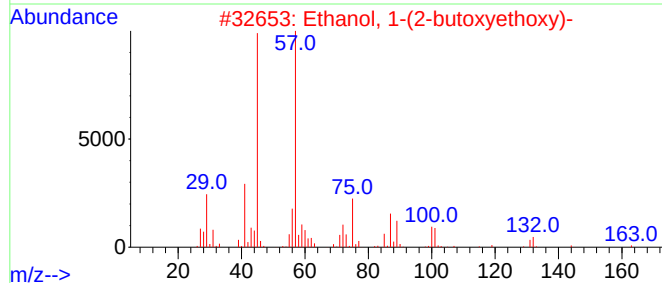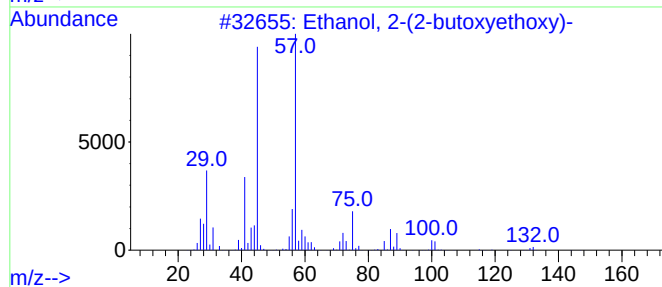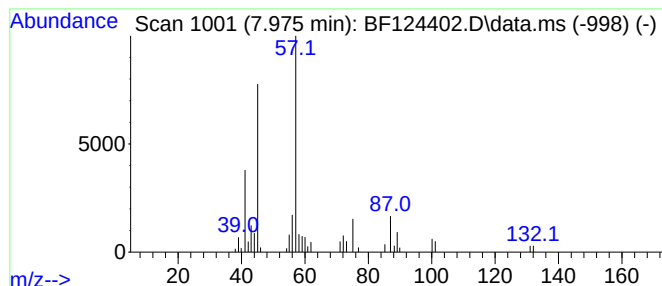

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124402.D
Acq On : 21 Jun 2021 20:02
Operator : JU/CG
Sample : M2772-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	7.975	6.8	ng	90019	2	8.069	262791	20.0