


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
 Data File : BF124386.D
 Acq On : 21 Jun 2021 10:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 15 20:09:26 2021

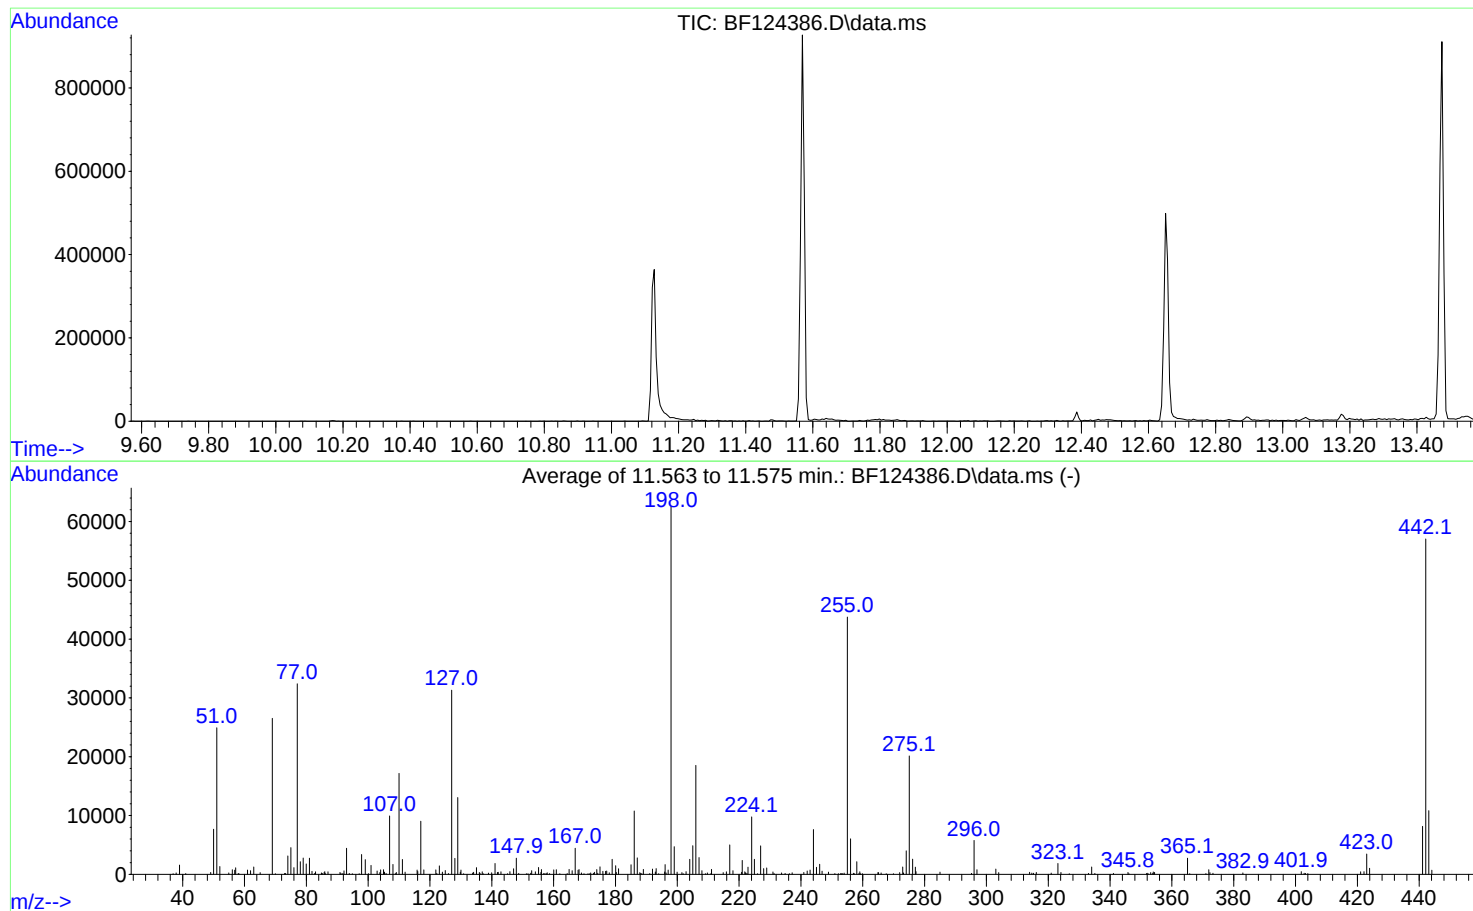




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	24932	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.4	26531	PASS
70	69	0.00	2	0.4	109	PASS
127	198	10	80	50.1	31307	PASS
197	198	0.00	2	1.2	744	PASS
198	198	100	100	100.0	62549	PASS
199	198	5	9	7.5	4701	PASS
275	198	10	60	32.2	20124	PASS
365	198	1	100	4.4	2763	PASS
441	198	0.01	100	13.1	8179	PASS
442	442	50	100	100.0	57037	PASS
443	442	15	24	19.0	10831	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124386.D
Acq On : 21 Jun 2021 10:47
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 21 11:16:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

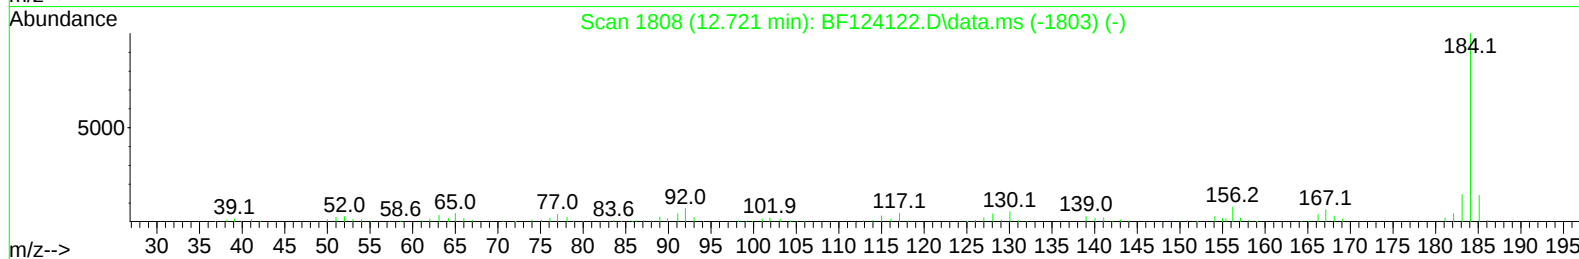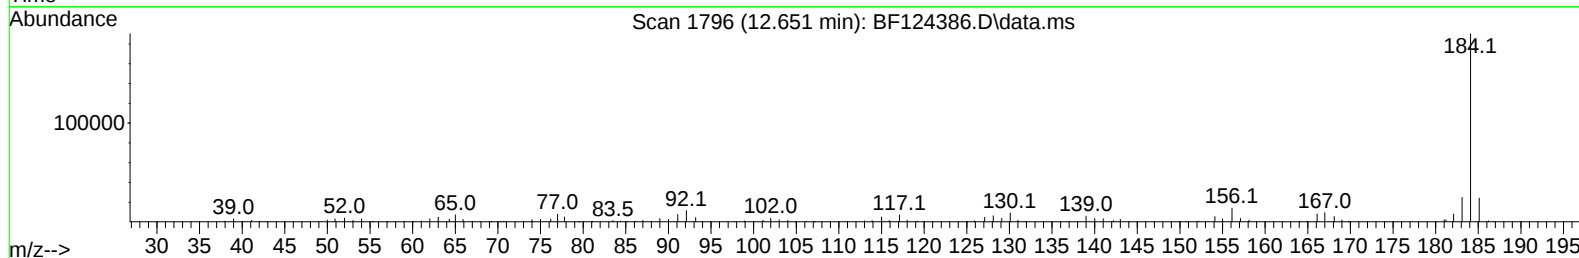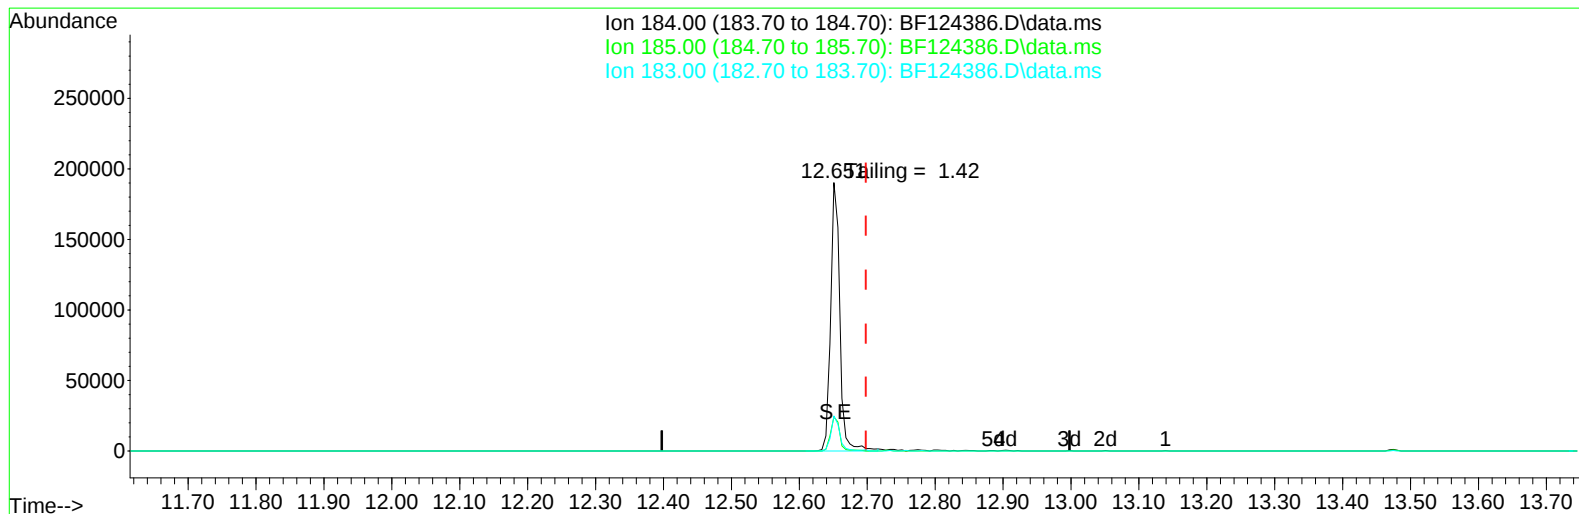

TIC: BF124386.D\data.ms

(77) Benzidine

12.651min (-0.047) 58297.16 ng m




response 176611

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	12.71
183.00	9.80	13.08#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062121\
Data File : BF124386.D
Acq On : 21 Jun 2021 10:47
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 21 11:16:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

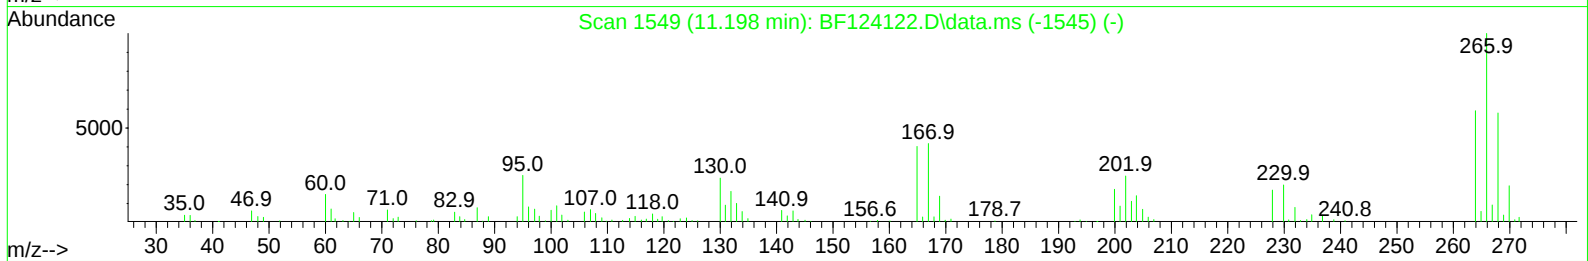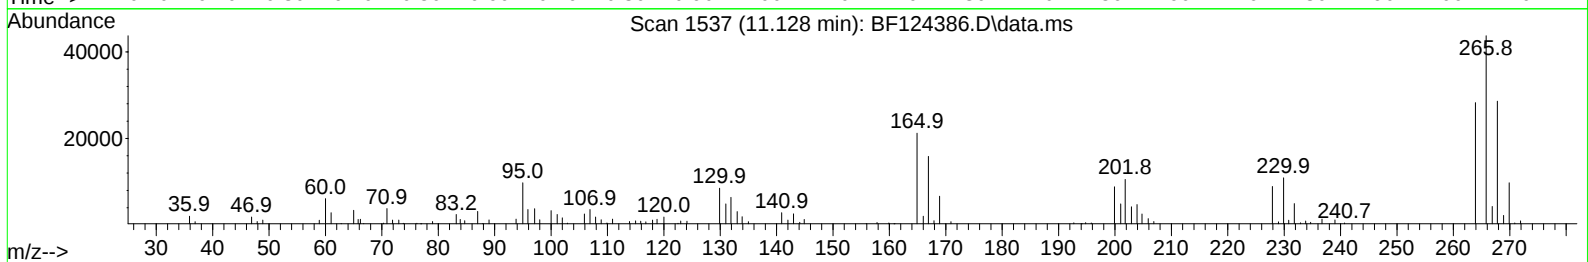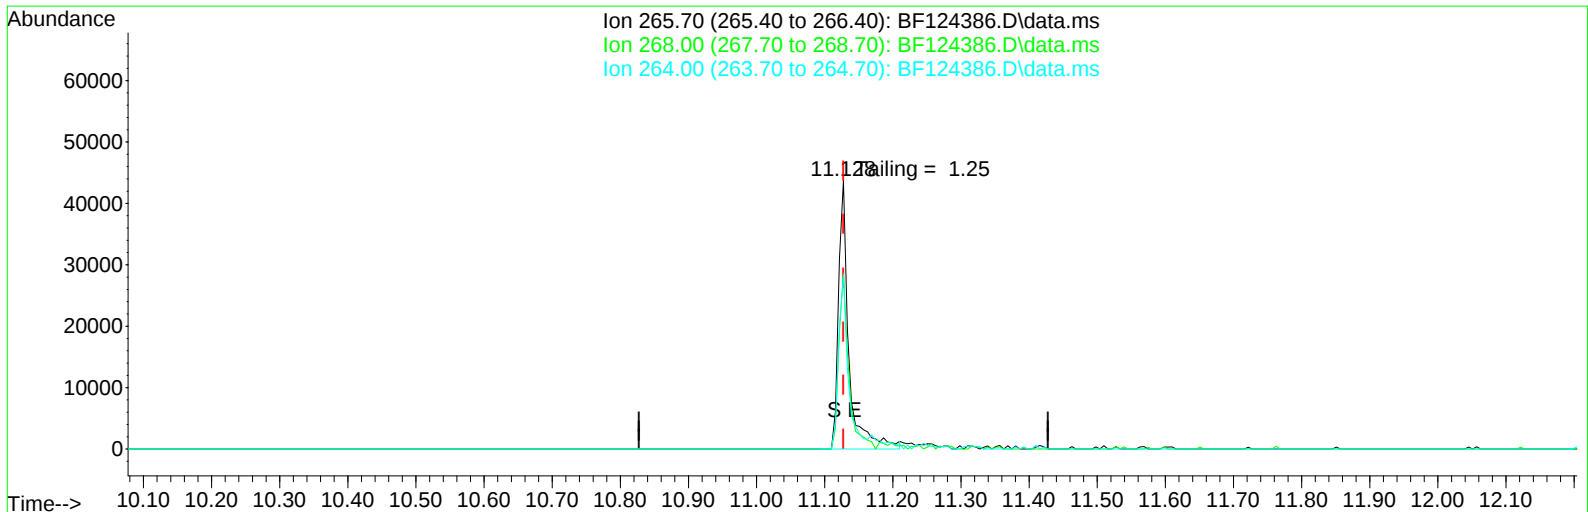

TIC: BF124386.D\data.ms

(70) Pentachlorophenol (C)

11.128min (+ 0.000) 8430.93 ng

response 46109

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.45
264.00	65.70	64.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/21/2021	BNA_F	<u>BF124386.D</u>
Compound Name	Response	Retention Time
DDT	134954	13.47
DDD	2984	13.17
DDE	847	12.83
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3831	138785	2.76