
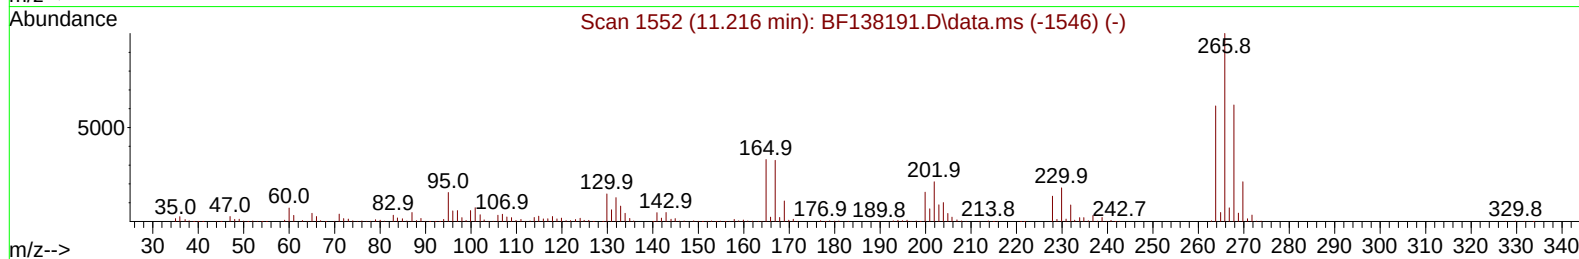
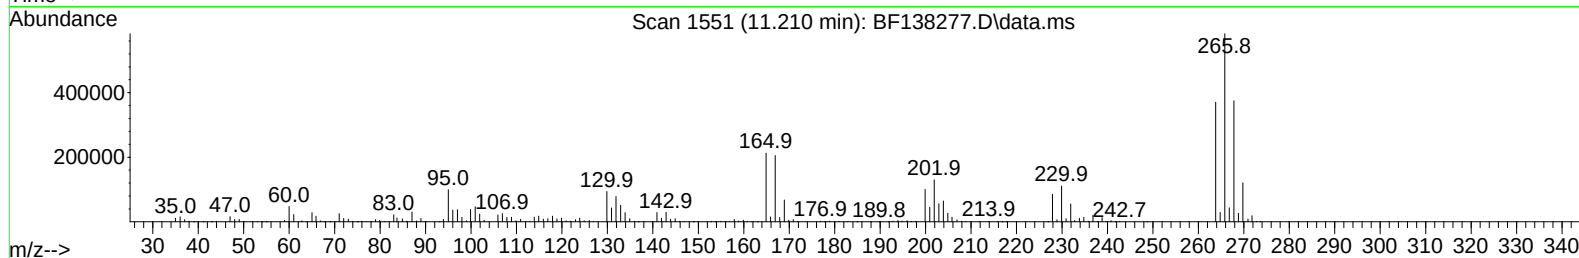


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062124\  
Data File : BF138277.D  
Acq On : 21 Jun 2024 10:11  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 12:06:31 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF061224.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 13 01:52:47 2024  
Response via : Initial Calibration

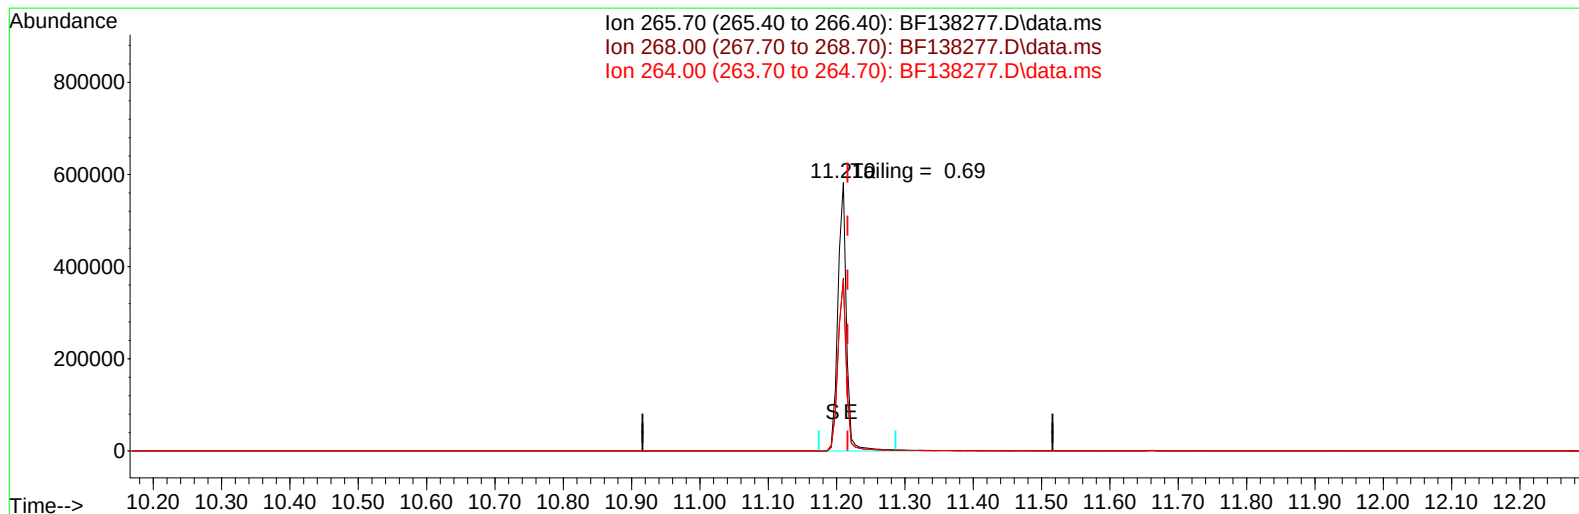

TIC: BF138277.D\data.ms

**(70) Pentachlorophenol (C)**




**11.210min (-0.006) 294697.59 ng**

**response 508523**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.90  | 64.38  |
| 264.00 | 61.50  | 63.56  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062124\  
Data File : BF138277.D  
Acq On : 21 Jun 2024 10:11  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 12:06:31 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF061224.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 13 01:52:47 2024  
Response via : Initial Calibration

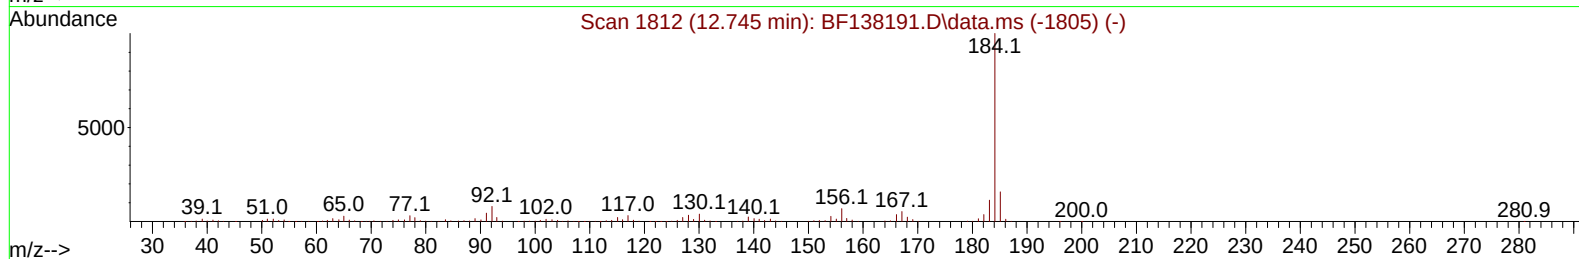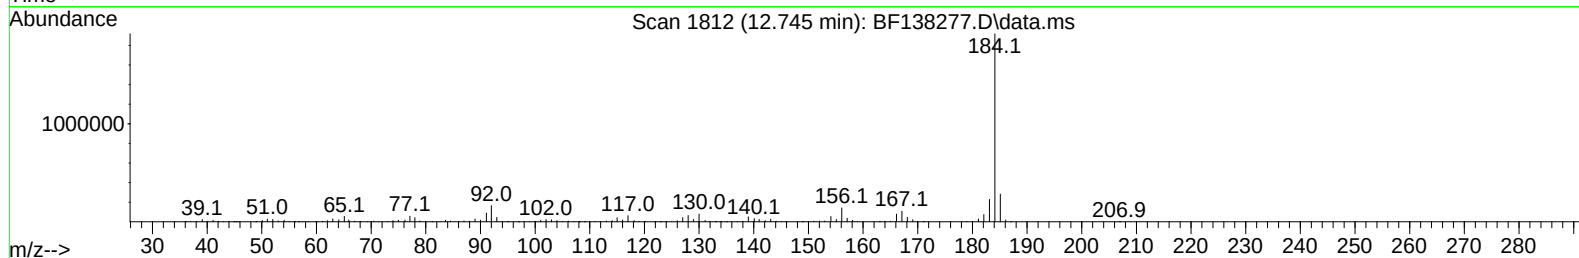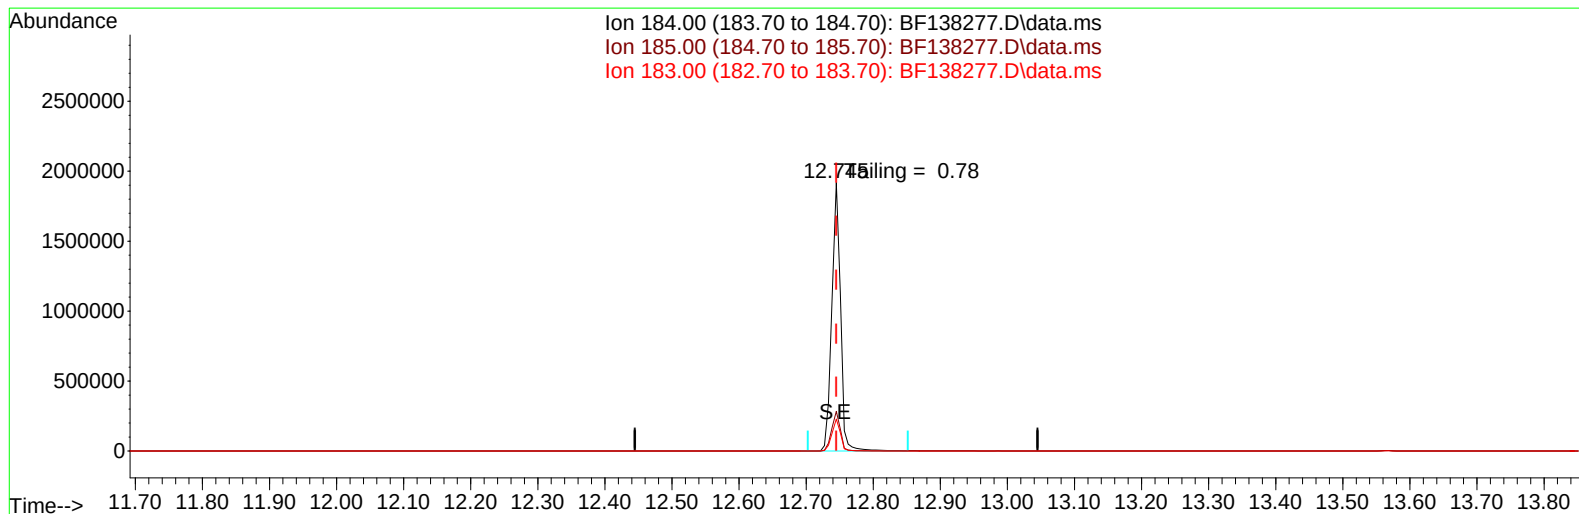

TIC: BF138277.D\data.ms

**(77) Benzidine**

12.745min (-0.000) 10172.05 ng m

response 1729208

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.80  | 14.78  |
| 183.00 | 11.30  | 11.96  |
| 0.00   | 0.00   | 0.00   |