
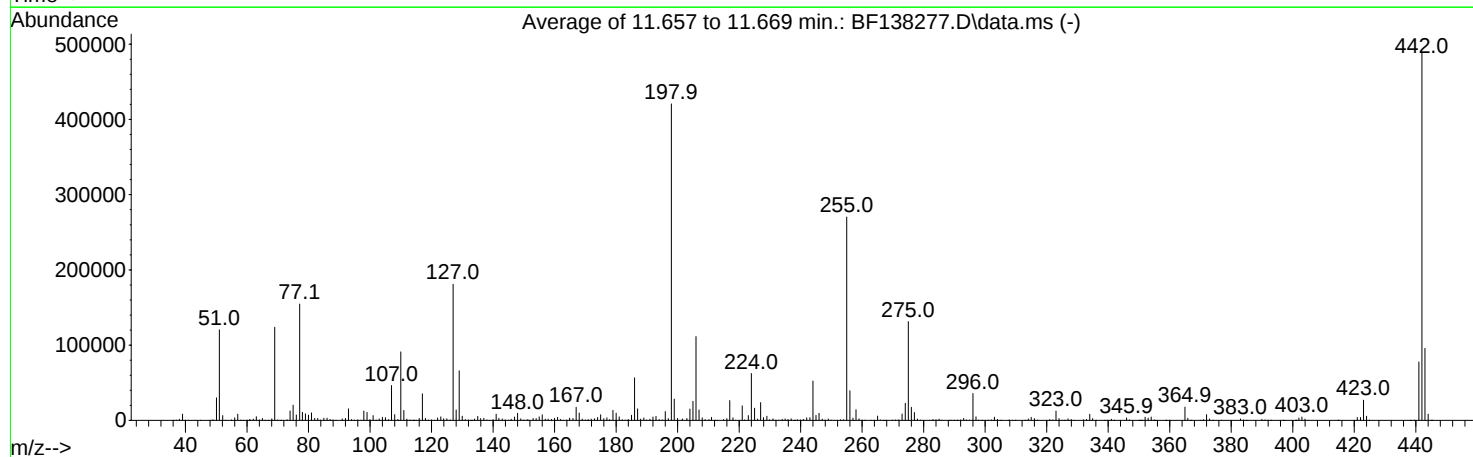


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062124\
Data File : BF138277.D
Acq On : 21 Jun 2024 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 13 01:52:47 2024

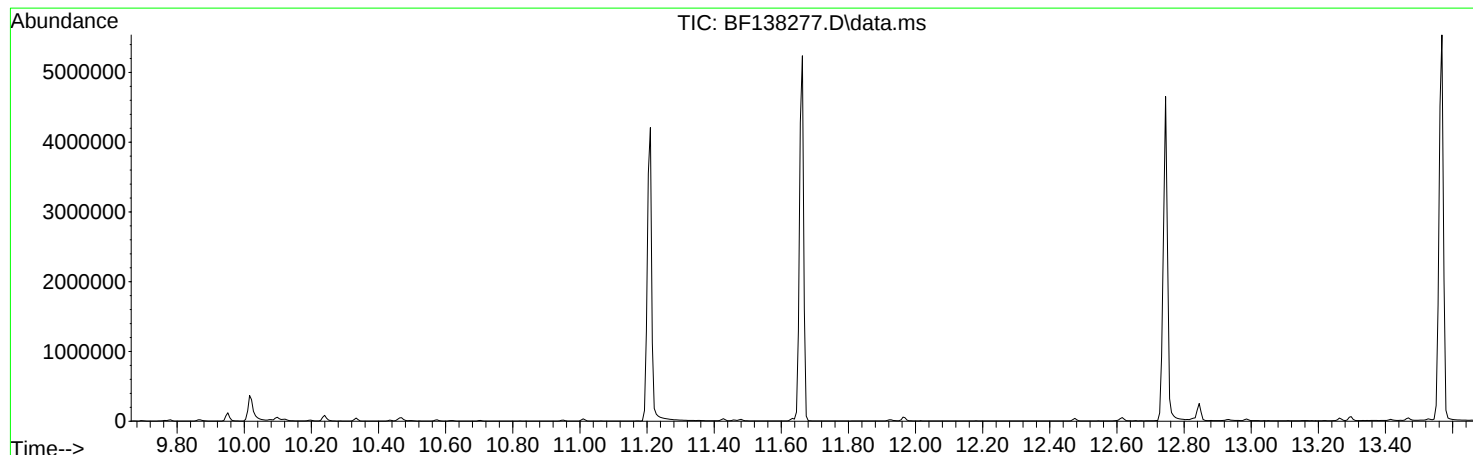

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	120412	PASS
68	69	0.00	2	1.7	2120	PASS
69	198	0.00	100	29.4	123872	PASS
70	69	0.00	2	0.5	564	PASS
127	198	10	80	43.0	180915	PASS
197	198	0.00	2	0.6	2413	PASS
198	198	100	100	100.0	420715	PASS
199	198	5	9	6.7	28317	PASS
275	198	10	60	31.2	131181	PASS
365	198	1	100	4.2	17775	PASS
441	198	0.01	100	18.4	77573	PASS
442	442	50	100	100.0	488960	PASS
443	442	15	24	19.6	95619	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/21/2024	BNA_F	<u>BF138277.D</u>
Compound Name	Response	Retention Time
DDT	1027266	13.568
DDD	15926	13.298
DDE	5286	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21212	1048478	2.02

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062124\
Data File : BF138277.D
Acq On : 21 Jun 2024 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 21 12:06:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

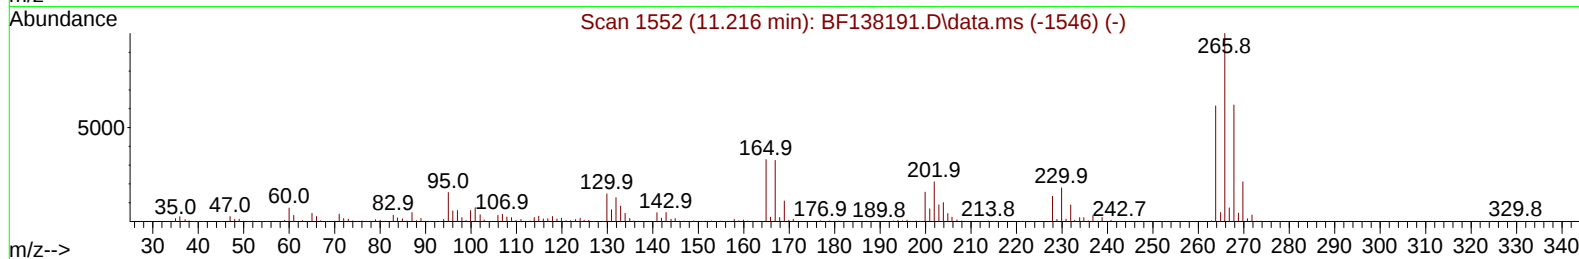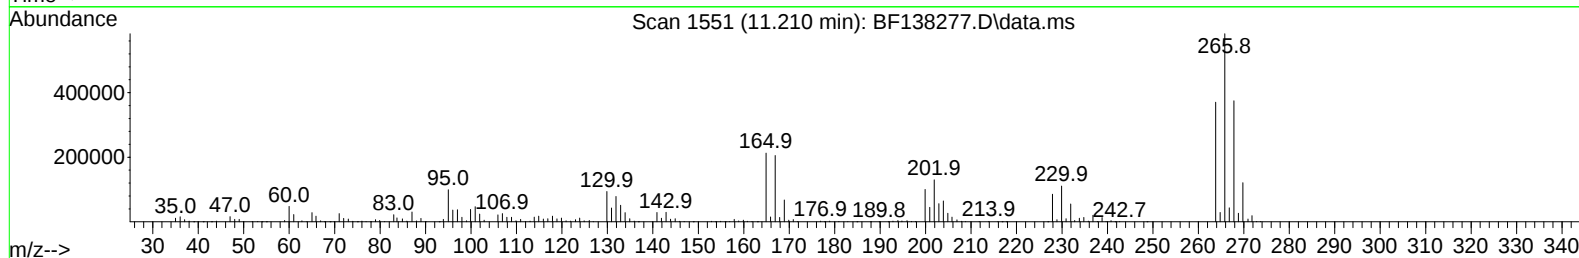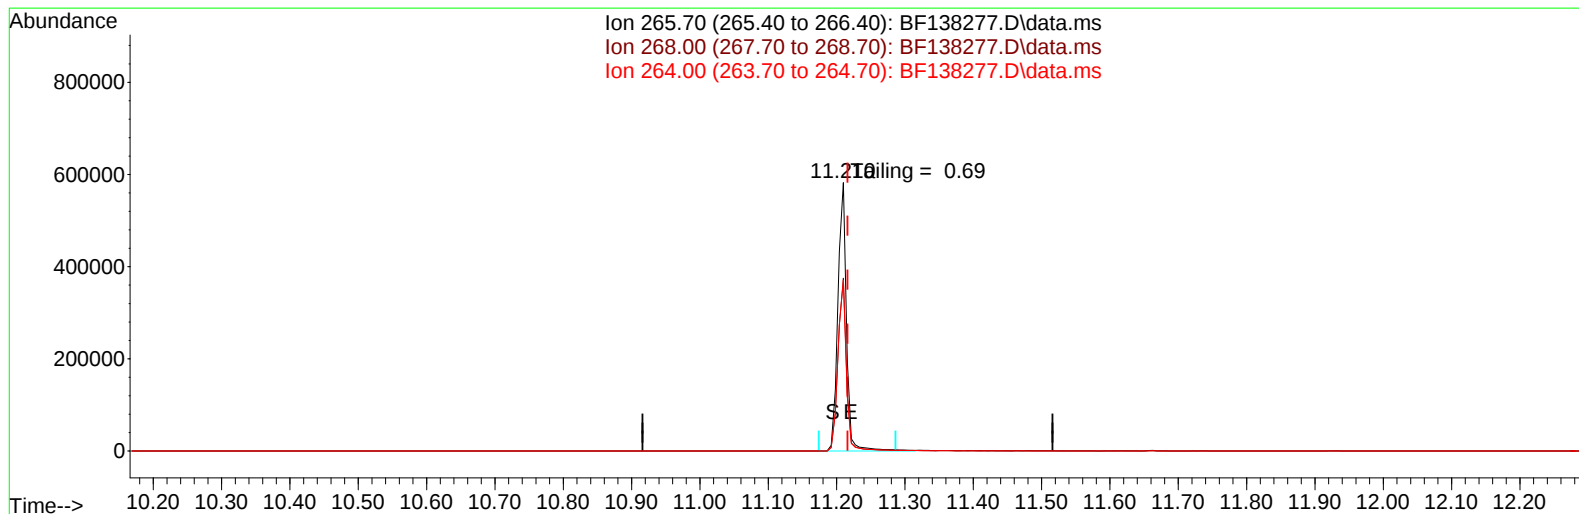

TIC: BF138277.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 294697.59 ng




response 508523

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	64.38
264.00	61.50	63.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062124\
Data File : BF138277.D
Acq On : 21 Jun 2024 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 21 12:06:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

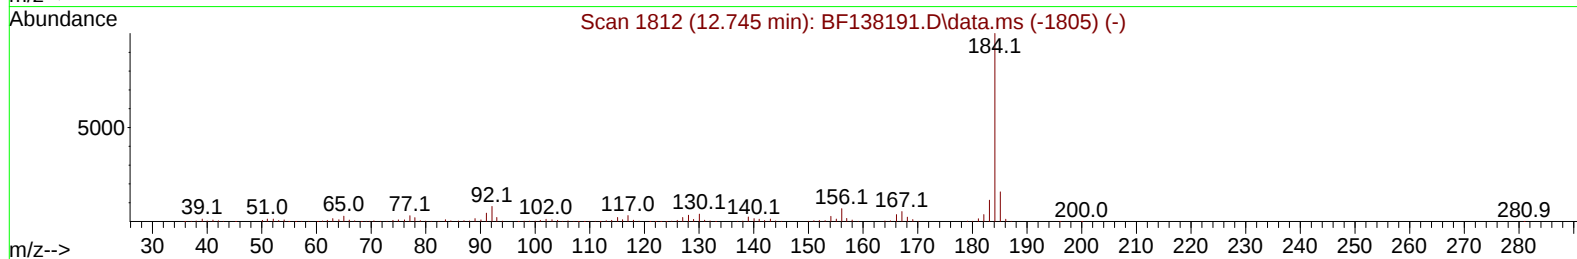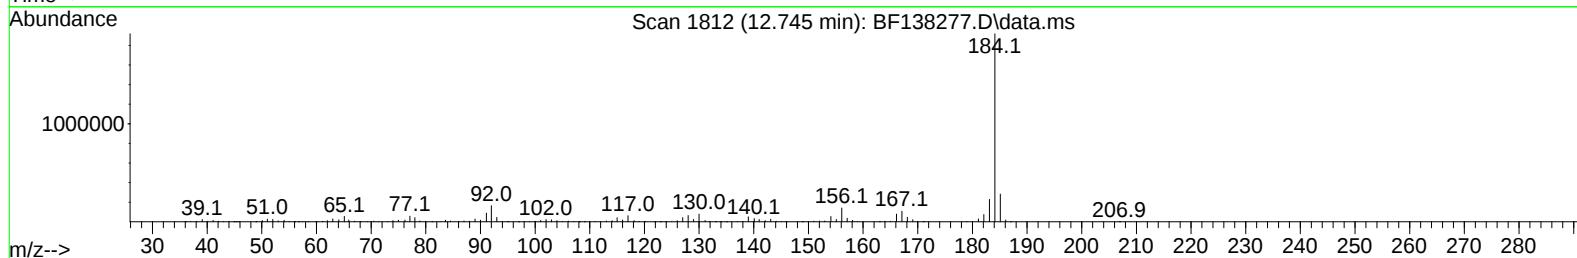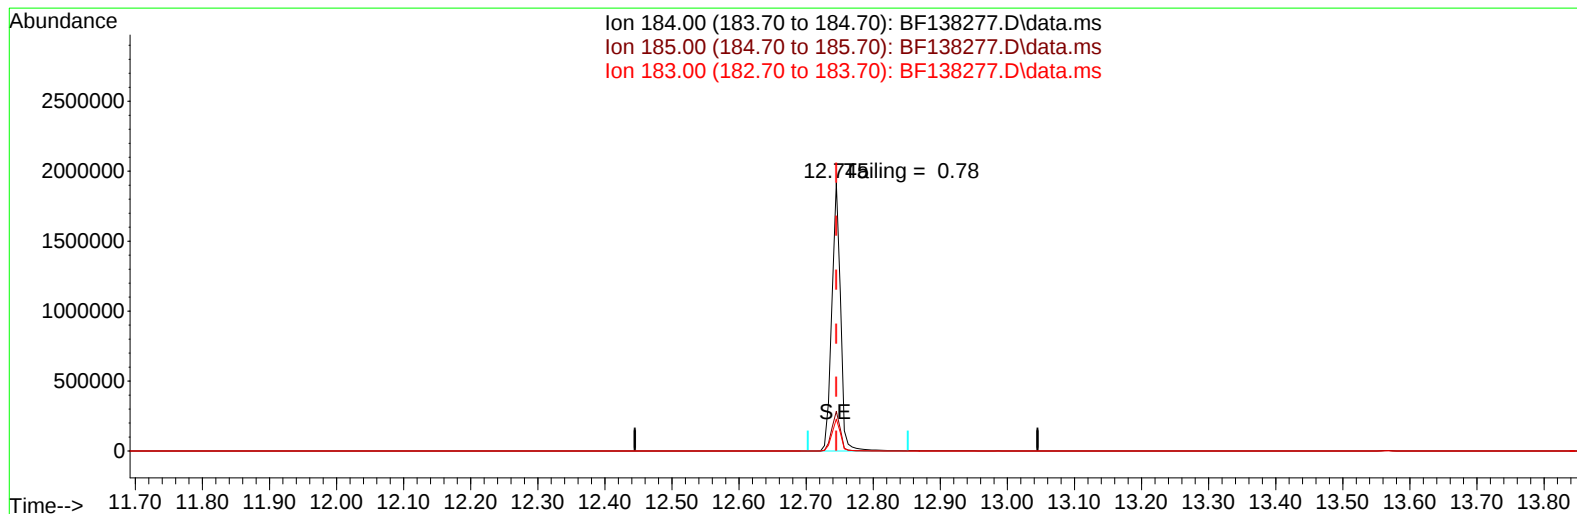

TIC: BF138277.D\data.ms

(77) Benzidine

12.745min (-0.000) 10172.05 ng m

response 1729208

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.78
183.00	11.30	11.96
0.00	0.00	0.00