

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062215\
 Data File : BF080109.D
 Acq On : 23 Jun 2015 00:33
 Operator : TP/IZ
 Sample : G2706-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SWD-1

Quant Time: Jun 23 01:41:33 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 23 00:53:56 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.33	152	52807	20.00	ng	0.00
21) Naphthalene-d8	8.61	136	221353	20.00	ng	-0.01
38) Acenaphthene-d10	10.38	164	116781	20.00	ng	-0.01
63) Phenanthrene-d10	11.89	188	258389	20.00	ng	-0.02
75) Chrysene-d12	14.80	240	266819	20.00	ng	-0.19
86) Perylene-d12	16.65	264	254629	20.00	ng	-0.27
System Monitoring Compounds						
5) 2-Fluorophenol	5.93	112	89311	29.94	ng	0.00
7) Phenol-d6	6.93	99	74900	18.87	ng	0.00
23) Nitrobenzene-d5	7.88	82	326117	85.77	ng	0.00
41) 2,4,6-Tribromophenol	11.18	330	82717	72.44	ng	0.00
44) 2-Fluorobiphenyl	9.69	172	682156	83.30	ng	0.00
78) Terphenyl-d14	13.56	244	729375	63.84	ng	-0.11
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.88	70	42450	15.40	ng	# 59
25) Isophorone	7.88	82	326150	42.62	ng	# 58
49) Dimethylphthalate	10.07	163	27469	3.13	ng	# 97
56) 2,4-Dinitrotoluene	10.38	165	14889	6.67	ng	# 31
66) 4-Bromophenyl-phenylether	11.18	248	5614	2.04	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062215\
Data File : BF080109.D
Acq On : 23 Jun 2015 00:33
Operator : TP/IZ
Sample : G2706-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SWD-1

Quant Time: Jun 23 01:41:33 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

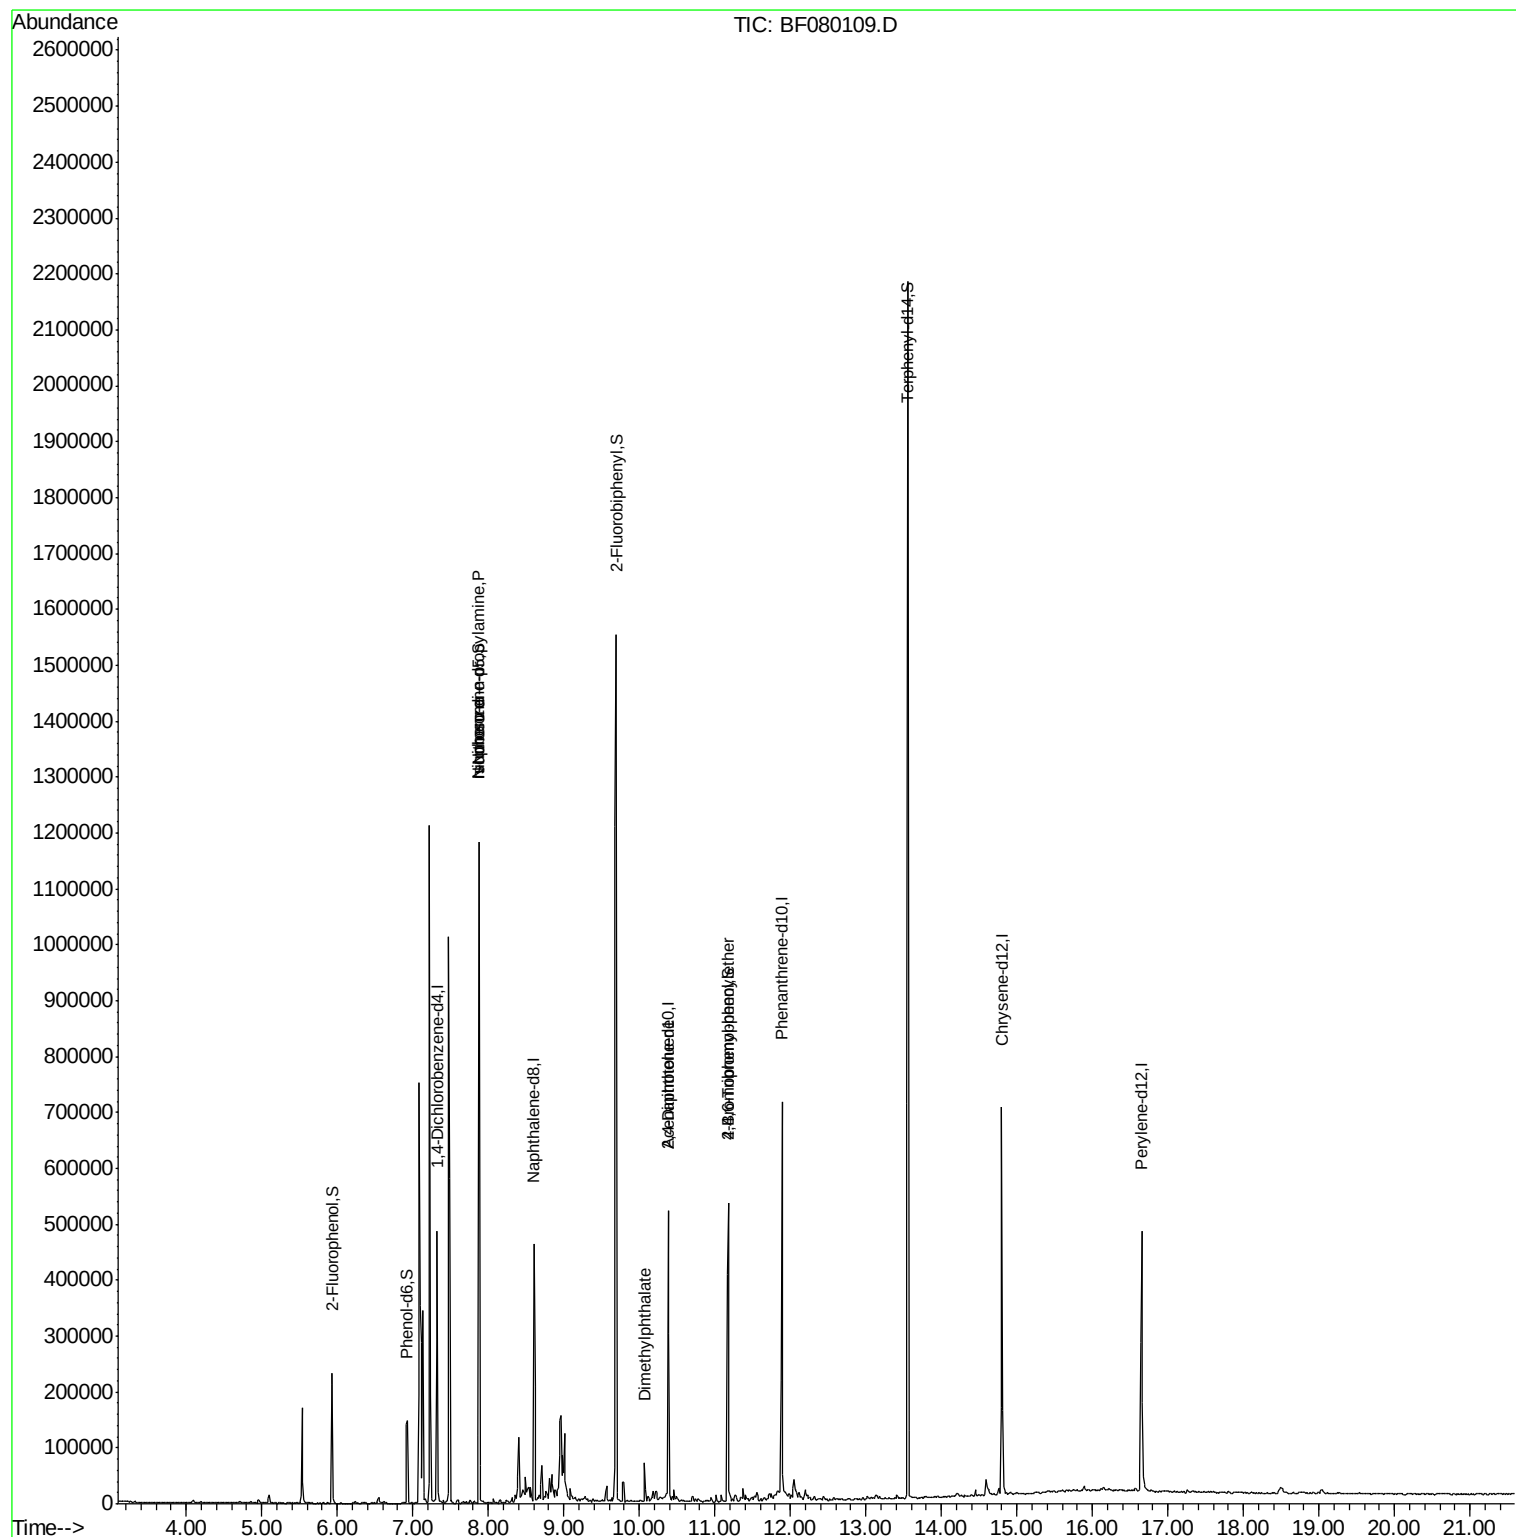

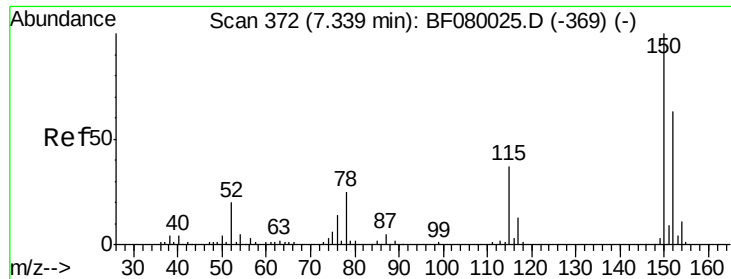


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.33 min Scan# 371
Delta R.T. -0.00 min
Lab File: BF080109.D
Acq: 23 Jun 2015 00:33

Instrument :
BNA_F
ClientSampleId :
SWD-1

Tgt Ion:152 Resp: 52807
Ion Ratio Lower Upper
152 100
150 154.5 124.7 187.1
115 47.0 39.0 58.4

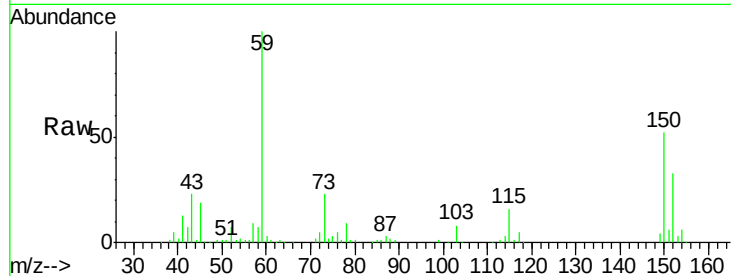


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

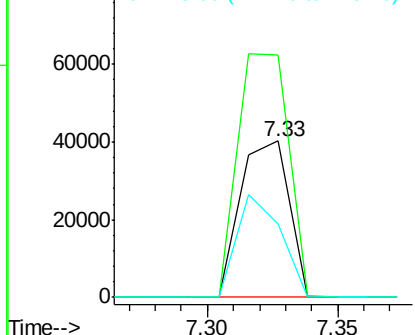



#5


2-Fluorophenol
Concen: 29.94 ng
RT: 5.93 min Scan# 249
Delta R.T. -0.00 min
Lab File: BF080109.D
Acq: 23 Jun 2015 00:33

Tgt Ion:112 Resp: 89311
Ion Ratio Lower Upper
112 100
64 50.9 39.7 59.5
63 25.0 17.4 26.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

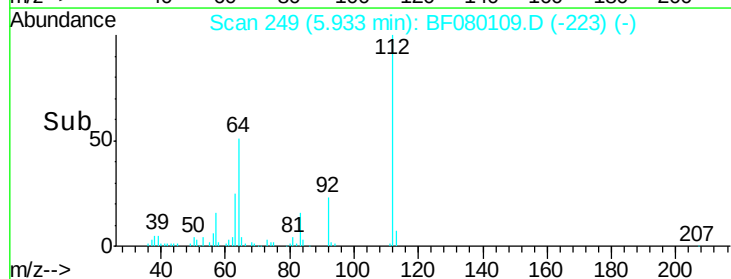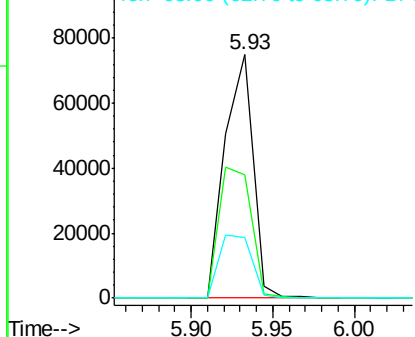

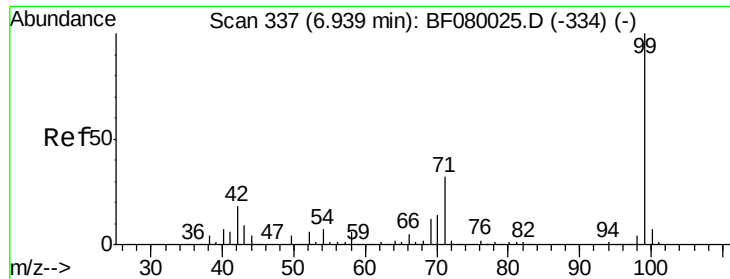

#7

Phenol-d6

Concen: 18.87 ng

RT: 6.93 min Scan# 336

Delta R.T. -0.00 min

Lab File: BF080109.D

Acq: 23 Jun 2015 00:33

Instrument :

BNA_F

ClientSampleId :

SWD-1


Tgt Ion: 99 Resp: 74900

Ion Ratio Lower Upper

99 100

42 15.3 13.7 20.5




71 28.1 14.2 21.2#

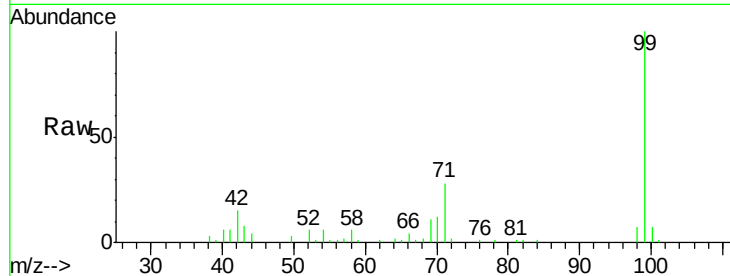

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

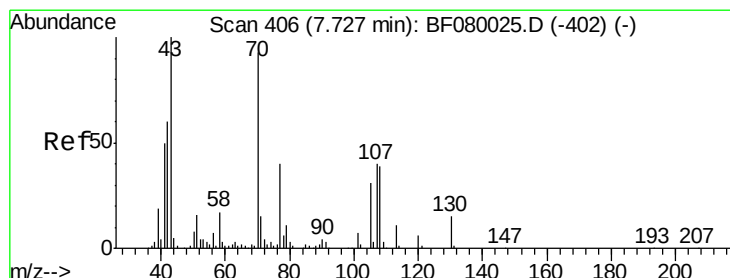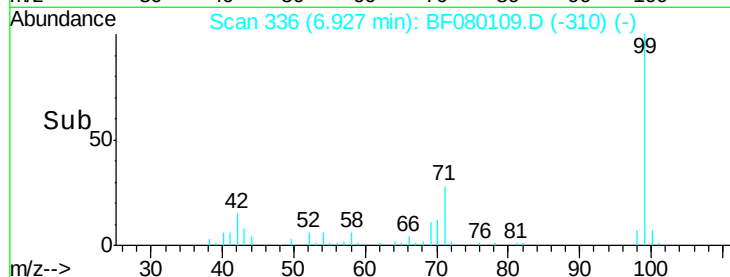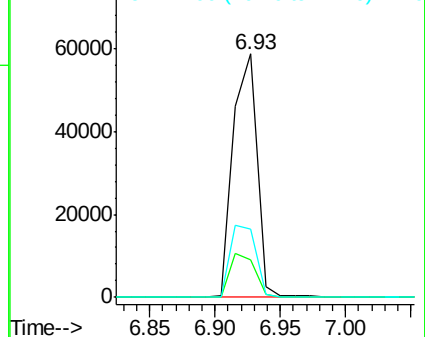

#19

n-Nitroso-di-n-propylamine

Concen: 15.40 ng

RT: 7.88 min Scan# 419

Delta R.T. 0.16 min

Lab File: BF080109.D

Acq: 23 Jun 2015 00:33

Tgt Ion: 70 Resp: 42450


Ion Ratio Lower Upper

70 100

42 47.6 63.8 95.6#

101 0.0 9.2 13.8#

130 2.0 27.3 40.9#


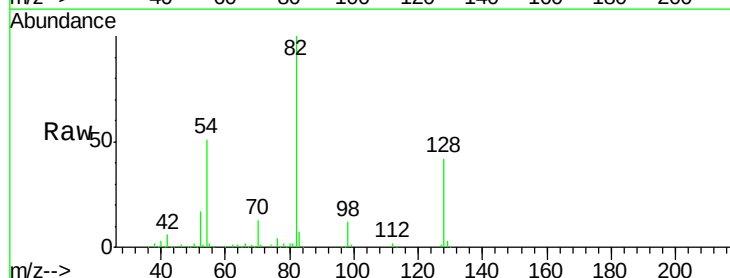



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

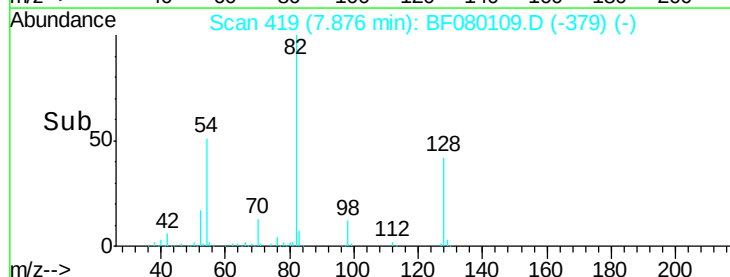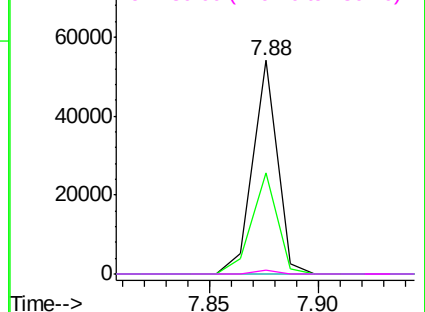


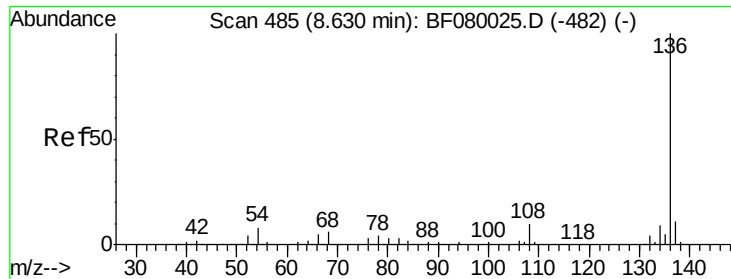




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.61 min Scan# 483
Delta R.T. -0.01 min
Lab File: BF080109.D
Acq: 23 Jun 2015 00:33

Instrument :
BNA_F
ClientSampleId :
SWD-1

Tgt Ion:	136	Resp:	221353
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.0	13.6
54	11.0	8.2	12.2
68	7.7	5.8	8.6




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

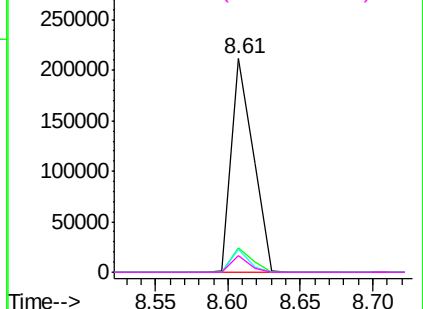




#23
Nitrobenzene-d5
Concen: 85.77 ng
RT: 7.88 min Scan# 419
Delta R.T. -0.00 min
Lab File: BF080109.D
Acq: 23 Jun 2015 00:33

Tgt Ion:	82	Resp:	326117
Ion	Ratio	Lower	Upper
82	100		
128	42.1	51.0	76.6#
54	51.4	47.5	71.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

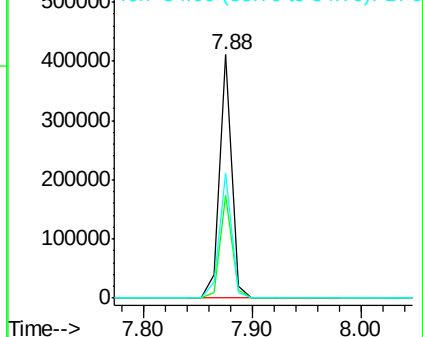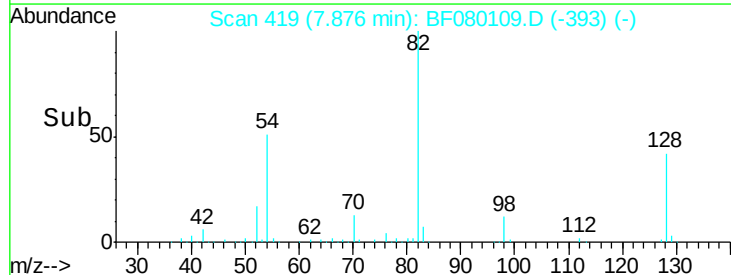

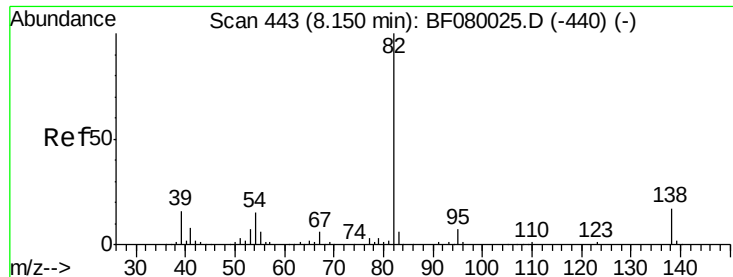

#25

Isophorone

Concen: 42.62 ng

RT: 7.88 min Scan# 419

Delta R.T. -0.26 min

Lab File: BF080109.D

Acq: 23 Jun 2015 00:33

Instrument :

BNA_F

ClientSampled :

SWD-1


Tgt Ion: 82 Resp: 326150

Ion Ratio Lower Upper




82 100

95 0.0 4.0 6.0#

138 0.0 18.3 27.5#

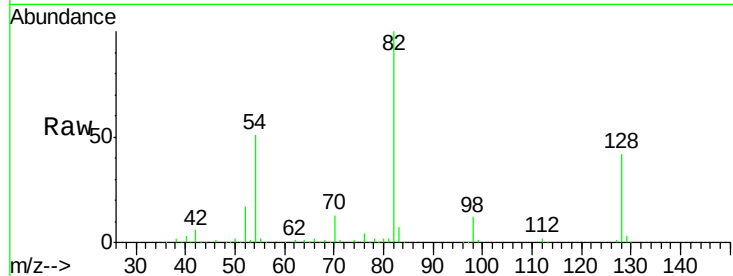

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): E

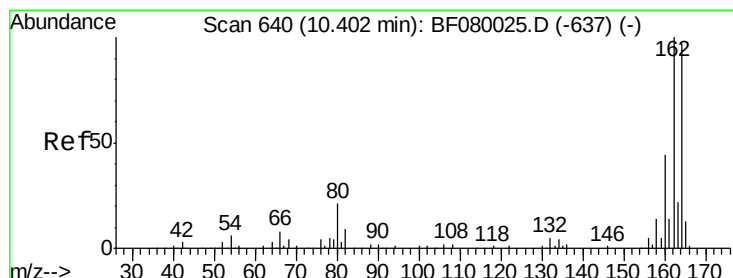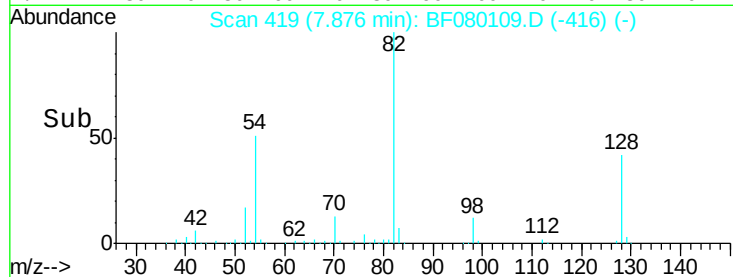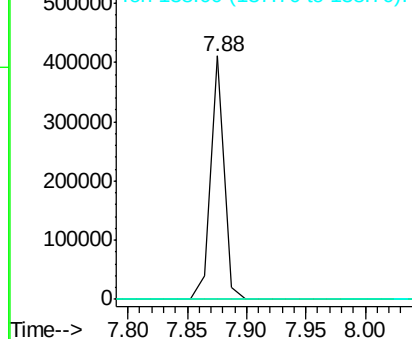

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 10.38 min Scan# 638

Delta R.T. -0.01 min

Lab File: BF080109.D

Acq: 23 Jun 2015 00:33


Tgt Ion: 164 Resp: 116781

Ion Ratio Lower Upper



164 100


162 104.5 75.2 112.8

160 46.4 31.5 47.3

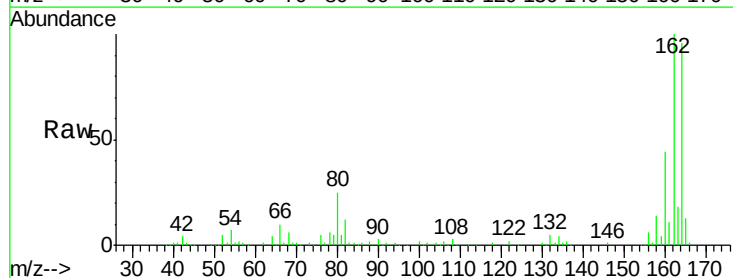

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

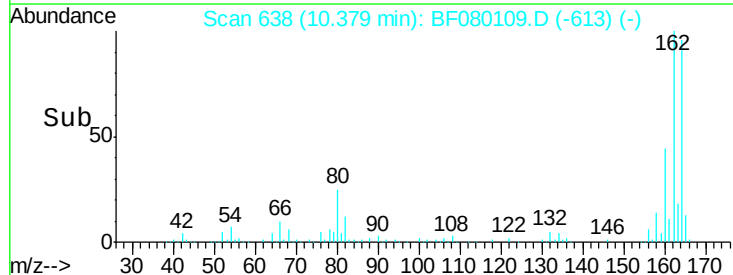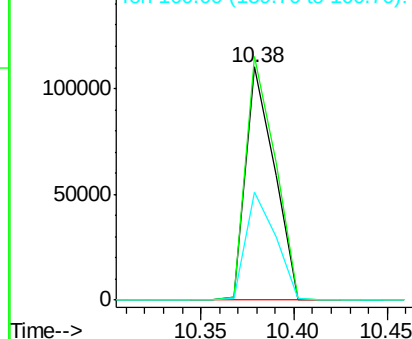







#41
 2,4,6-Tribromophenol
 Concen: 72.44 ng
 RT: 11.18 min Scan# 708
 Delta R.T. -0.00 min
 Lab File: BF080109.D
 Acq: 23 Jun 2015 00:33

Instrument :
 BNA_F
 ClientSampleId :
 SWD-1

Tgt Ion:330 Resp: 82717
 Ion Ratio Lower Upper
 330 100
 332 94.3 76.6 114.8
 141 34.5 29.7 44.5

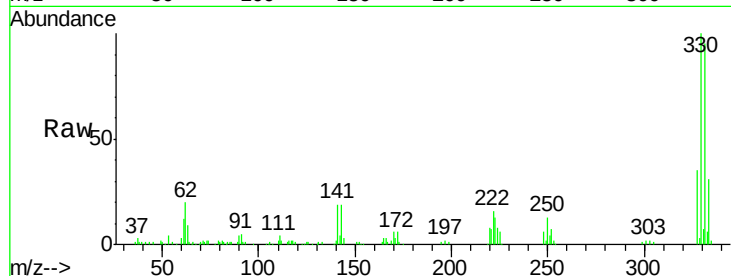


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


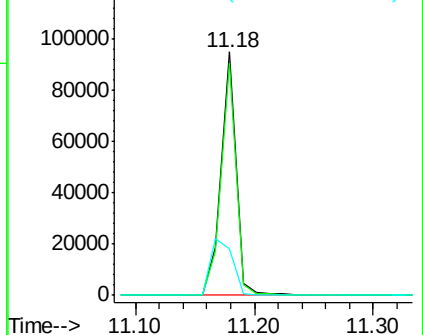



#44
 2-Fluorobiphenyl
 Concen: 83.30 ng
 RT: 9.69 min Scan# 578
 Delta R.T. -0.00 min
 Lab File: BF080109.D
 Acq: 23 Jun 2015 00:33

Tgt Ion:172 Resp: 682156
 Ion Ratio Lower Upper
 172 100
 171 34.8 26.1 39.1
 170 23.1 17.4 26.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

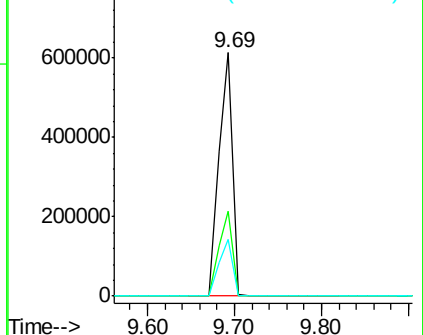


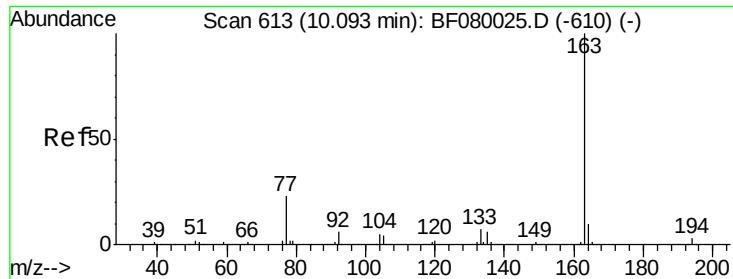




#49
Dimethylphthalate
Concen: 3.13 ng
RT: 10.07 min Scan# 611
Delta R.T. -0.01 min
Lab File: BF080109.D
Acq: 23 Jun 2015 00:33

Instrument :
BNA_F
ClientSampleId :
SWD-1

Tgt Ion:163 Resp: 27469
Ion Ratio Lower Upper
163 100
194 3.9 4.4 6.6#
164 11.2 8.3 12.5

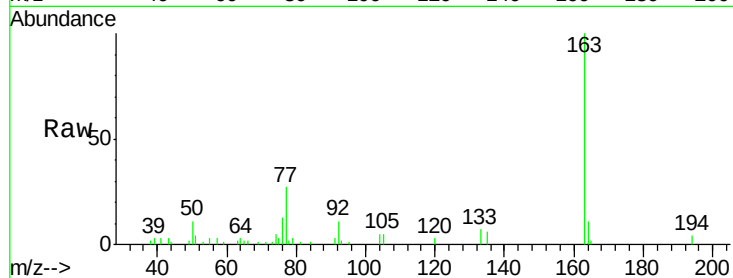


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

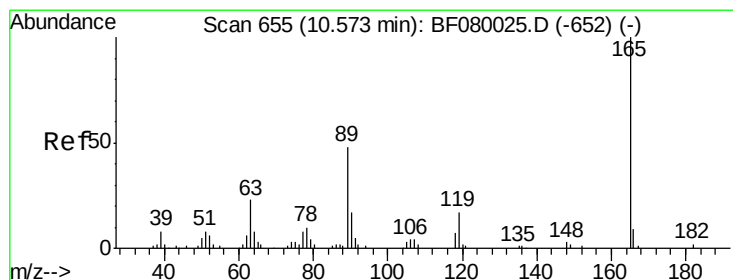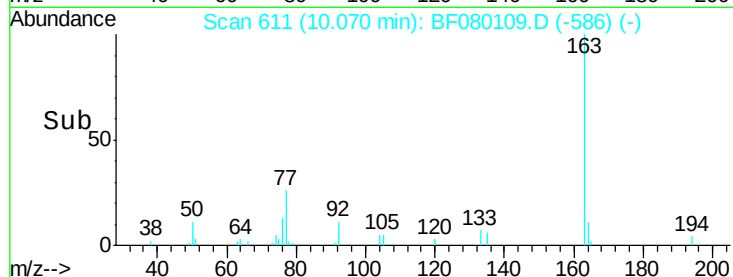
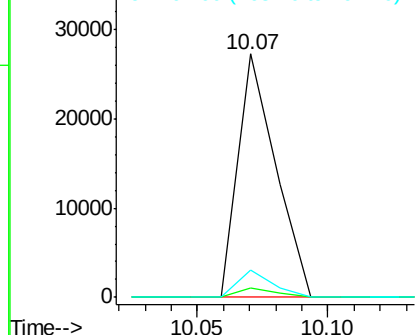



#56
2,4-Dinitrotoluene
Concen: 6.67 ng
RT: 10.38 min Scan# 638
Delta R.T. -0.17 min
Lab File: BF080109.D
Acq: 23 Jun 2015 00:33

Tgt Ion:165 Resp: 14889
Ion Ratio Lower Upper
165 100
63 0.0 29.8 44.6#
89 0.0 44.5 66.7#
182 0.0 3.0 4.4#

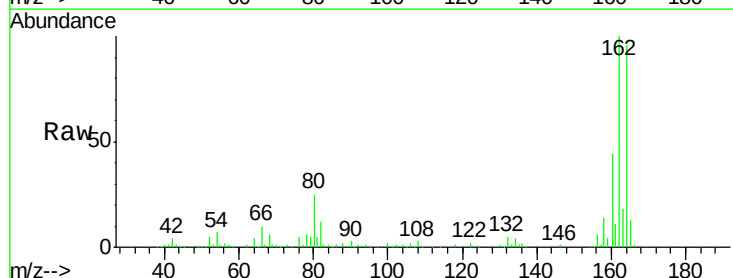

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF0
Ion 89.00 (88.70 to 89.70): BF0
Ion 182.00 (181.70 to 182.70): E

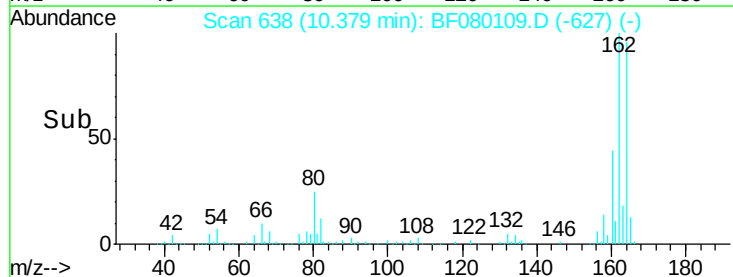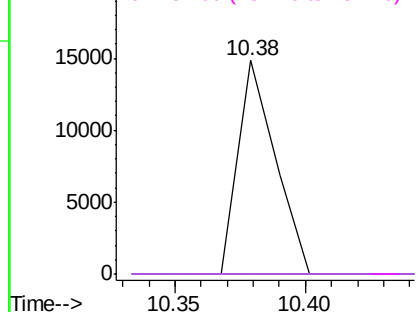


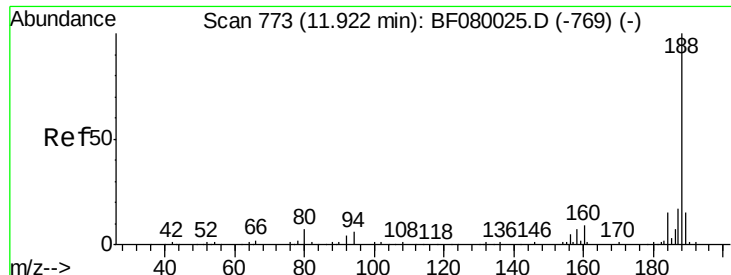




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.89 min Scan# 770
 Delta R.T. -0.02 min
 Lab File: BF080109.D
 Acq: 23 Jun 2015 00:33

Instrument :
 BNA_F
 ClientSampleId :
 SWD-1

Tgt Ion:188 Resp: 258389
 Ion Ratio Lower Upper
 188 100
 94 7.3 11.1 16.7#
 80 8.0 11.0 16.4#

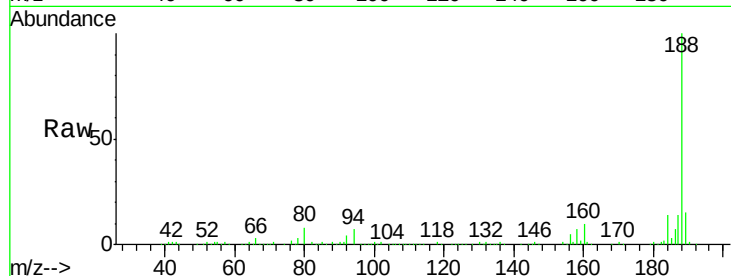


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0


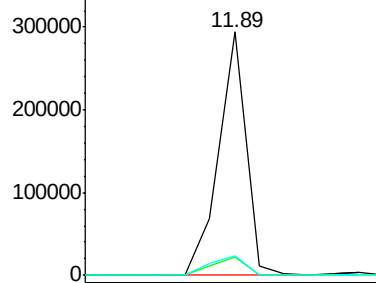



#66
 4-Bromophenyl-phenylether
 Concen: 2.04 ng
 RT: 11.18 min Scan# 708
 Delta R.T. -0.24 min
 Lab File: BF080109.D
 Acq: 23 Jun 2015 00:33

Tgt Ion:248 Resp: 5614
 Ion Ratio Lower Upper
 248 100
 250 203.6 78.5 117.7#
 141 314.6 59.0 88.6#



Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

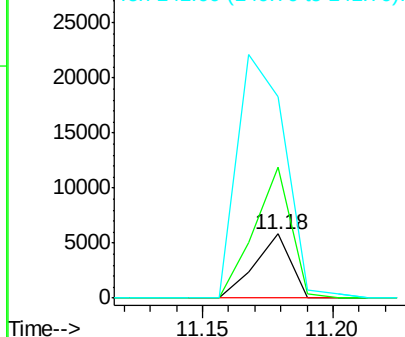



#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.80 min Scan# 1025

Delta R.T. -0.19 min

Lab File: BF080109.D

Acq: 23 Jun 2015 00:33

Instrument :

BNA_F

ClientSampleId :

SWD-1


Tgt Ion:240 Resp: 266819

Ion Ratio Lower Upper

240 100

120 10.1 16.2 24.2#




236 26.2 18.4 27.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

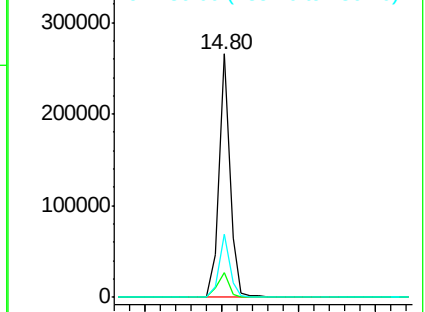

#78

Terphenyl-d14

Concen: 63.84 ng

RT: 13.56 min Scan# 916

Delta R.T. -0.11 min

Lab File: BF080109.D

Acq: 23 Jun 2015 00:33


Tgt Ion:244 Resp: 729375

Ion Ratio Lower Upper

244 100

212 7.0 4.3 6.5#



122 9.9 17.4 26.2#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

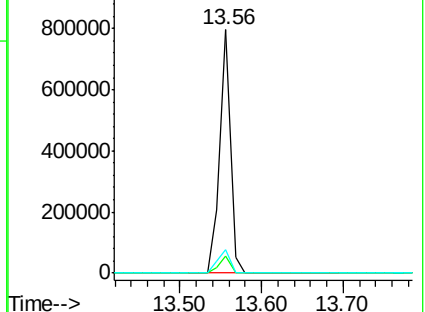


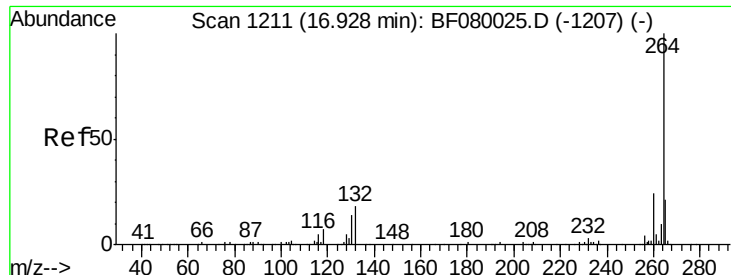

#86
Perylene-d12
Concen: 20.00 ng
RT: 16.65 min Scan# 1187
Delta R.T. -0.27 min
Lab File: BF080109.D
Acq: 23 Jun 2015 00:33

Instrument :
BNA_F
ClientSampleId :
SWD-1

Tgt Ion: 264 Resp: 254629
Ion Ratio Lower Upper
264 100
260 24.4 16.7 25.1
265 21.5 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

