
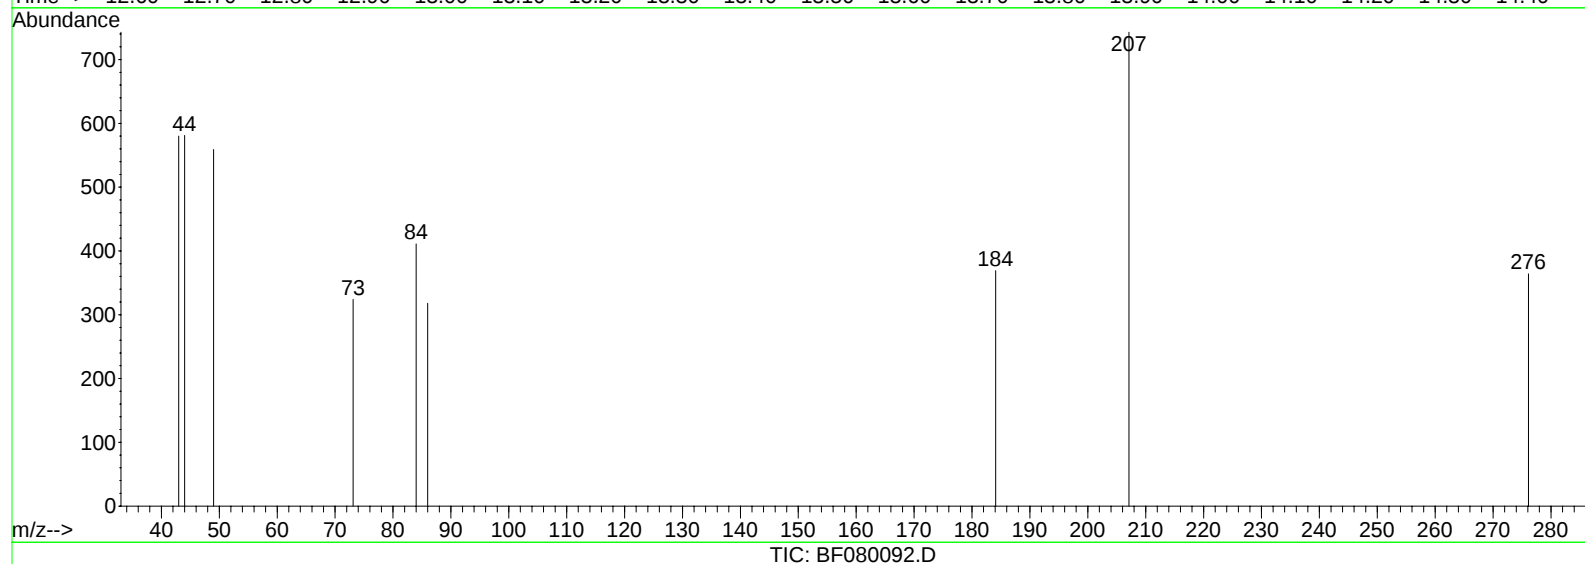


Data Path : Z:\HPCHEM1\BNA F\Data\BF062215\
Data File : BF080092.D
Acq On : 22 Jun 2015 11:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 11:34:47 2015
Quant Method : C:\msdchem\1\METHODS\8270-BF060415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 19:33:57 2015
Response via : Initial Calibration

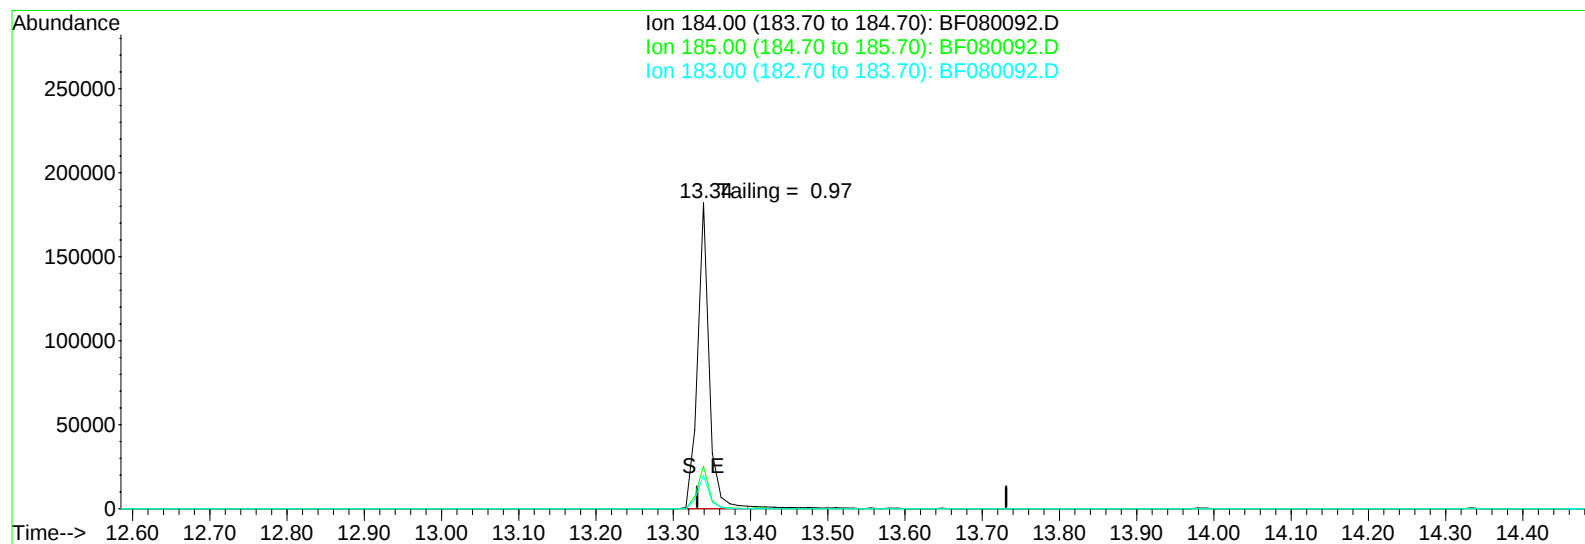

(76) Benzidine



13.531min (-13.531) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.20	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF062215\
Data File : BF080092.D
Acq On : 22 Jun 2015 11:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 11:34:47 2015
Quant Method : C:\msdchem\1\METHODS\8270-BF060415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 19:33:57 2015
Response via : Initial Calibration

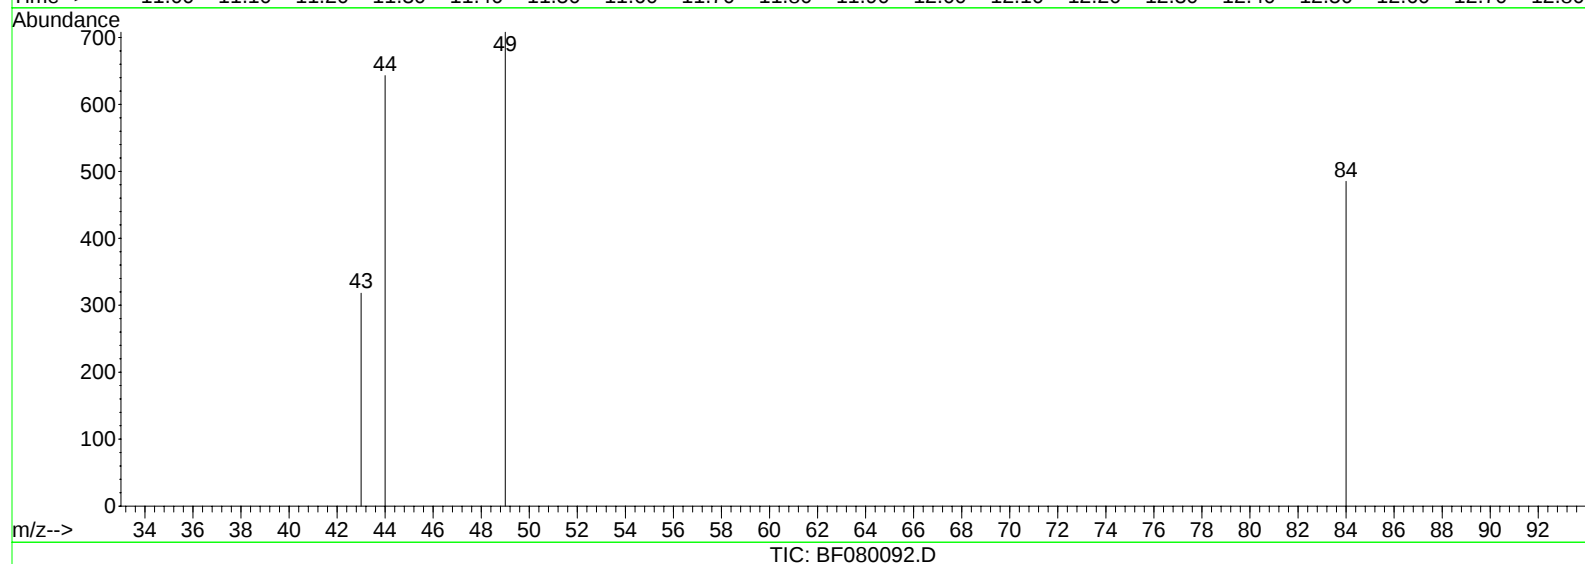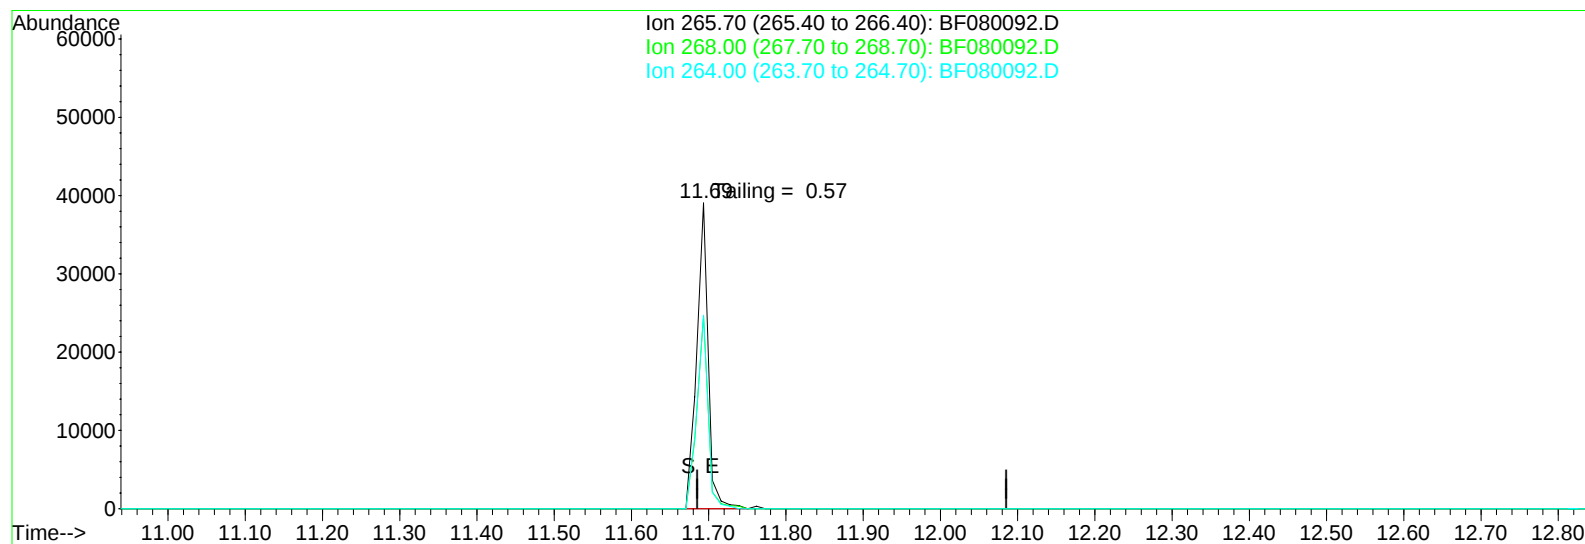

(69) Pentachlorophenol (C)

11.885min (-11.885) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	63.00	0.00#
264.00	64.10	0.00#
0.00	0.00	0.00