
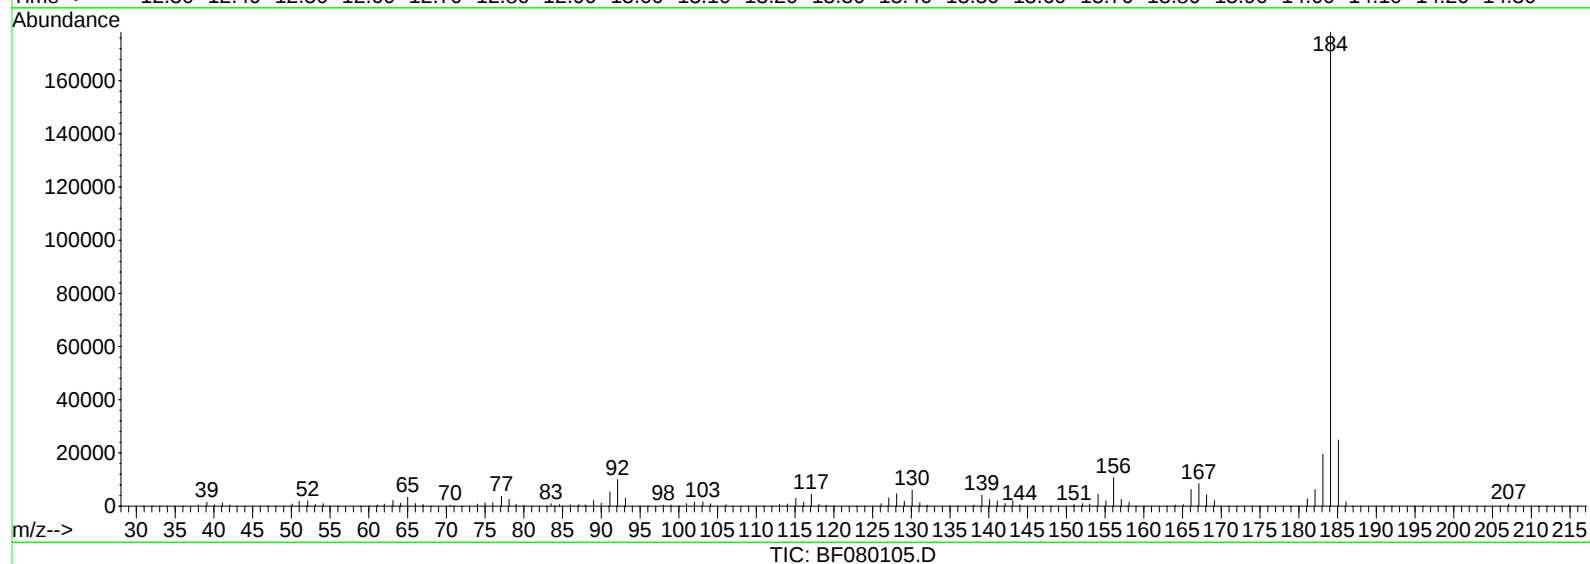


Data Path : Z:\HPCHEM1\BNA F\Data\BF062215\
Data File : BF080105.D
Acq On : 22 Jun 2015 22:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 08:35:16 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

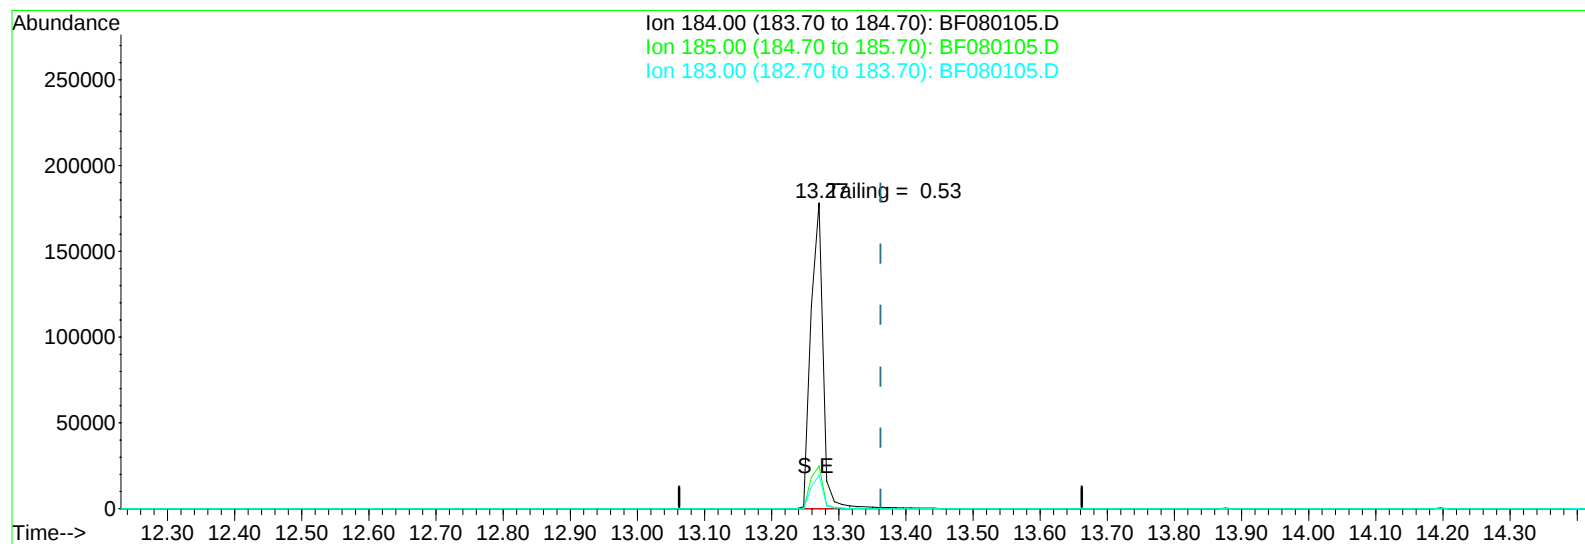

(76) Benzidine



13.271min (-0.092) 15347.76ng

response 224798

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.95
183.00	9.50	10.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF062215\
Data File : BF080105.D
Acq On : 22 Jun 2015 22:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 08:35:16 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 00:53:56 2015
Response via : Initial Calibration

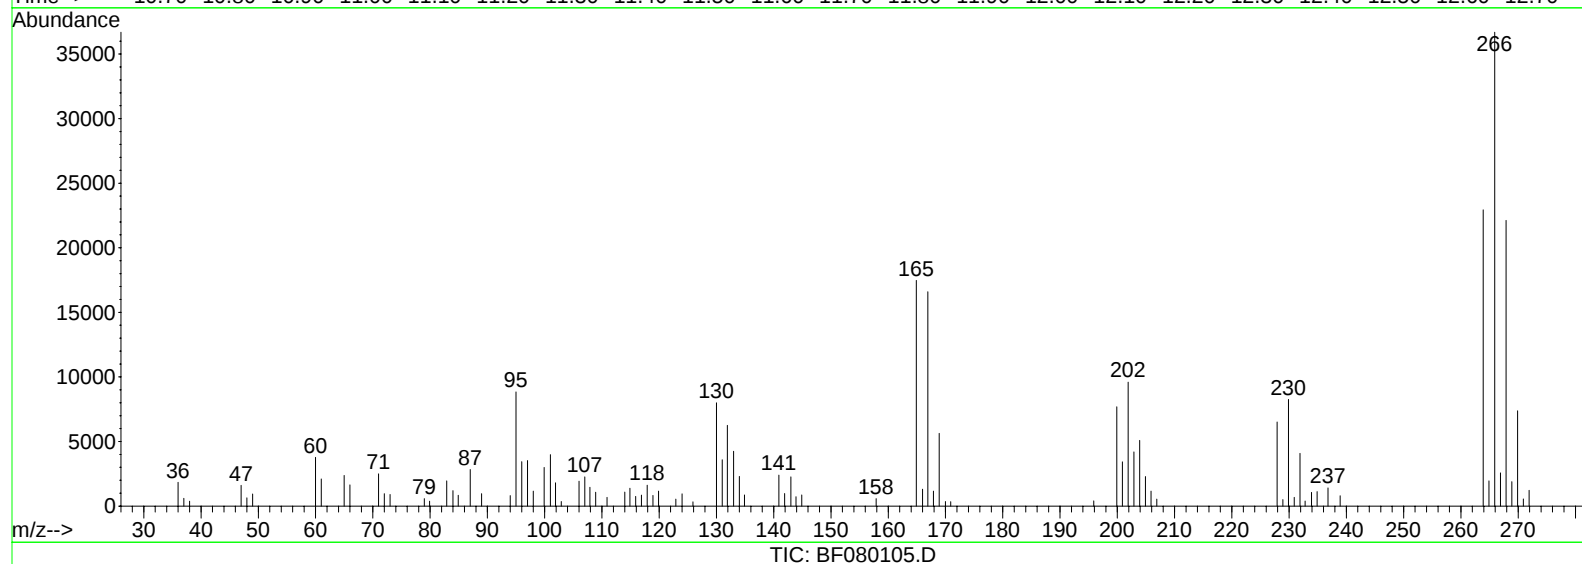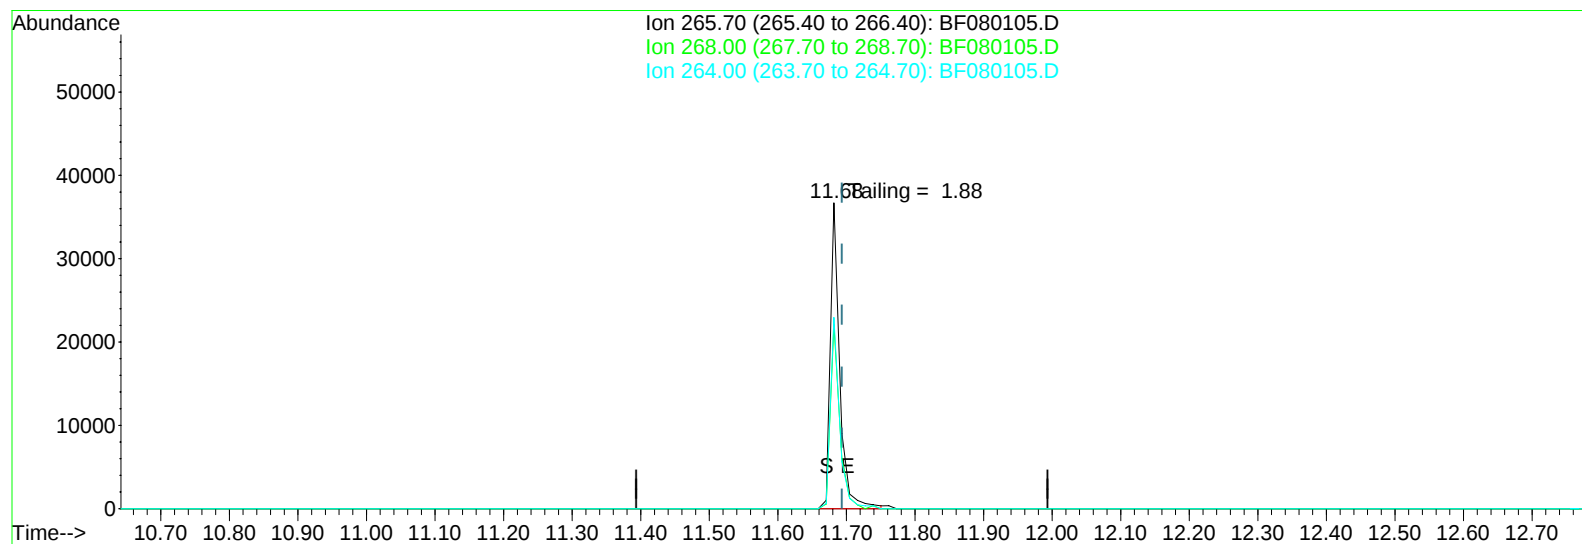

(69) Pentachlorophenol (C)

11.682min (-0.012) 0.00ng

response 35150

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	60.28
264.00	62.70	62.50
0.00	0.00	0.00