

Data Path : Z:\HPCHEM1\BNA_F\Data\BF062215\
Data File : BF080101.D
Acq On : 22 Jun 2015 18:36
Operator : TP/IZ
Sample : G2728-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.316	369	370	373	rBV	192238	197833	43.94%	9.333%
2	8.607	481	483	486	rVB	288512	283163	62.89%	13.359%
3	10.379	636	638	641	rBV2	315015	341597	75.87%	16.115%
4	11.888	768	770	772	rBV	484043	418667	92.99%	19.751%
5	14.837	1025	1028	1030	rBV	359188	450241	100.00%	21.241%
6	16.700	1188	1191	1198	rVB	290461	428179	95.10%	20.200%


Sum of corrected areas: 2119680

Data Path : Z:\HPCHEM1\BNA_F\Data\BF062215\
Data File : BF080101.D
Acq On : 22 Jun 2015 18:36
Operator : TP/IZ
Sample : G2728-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

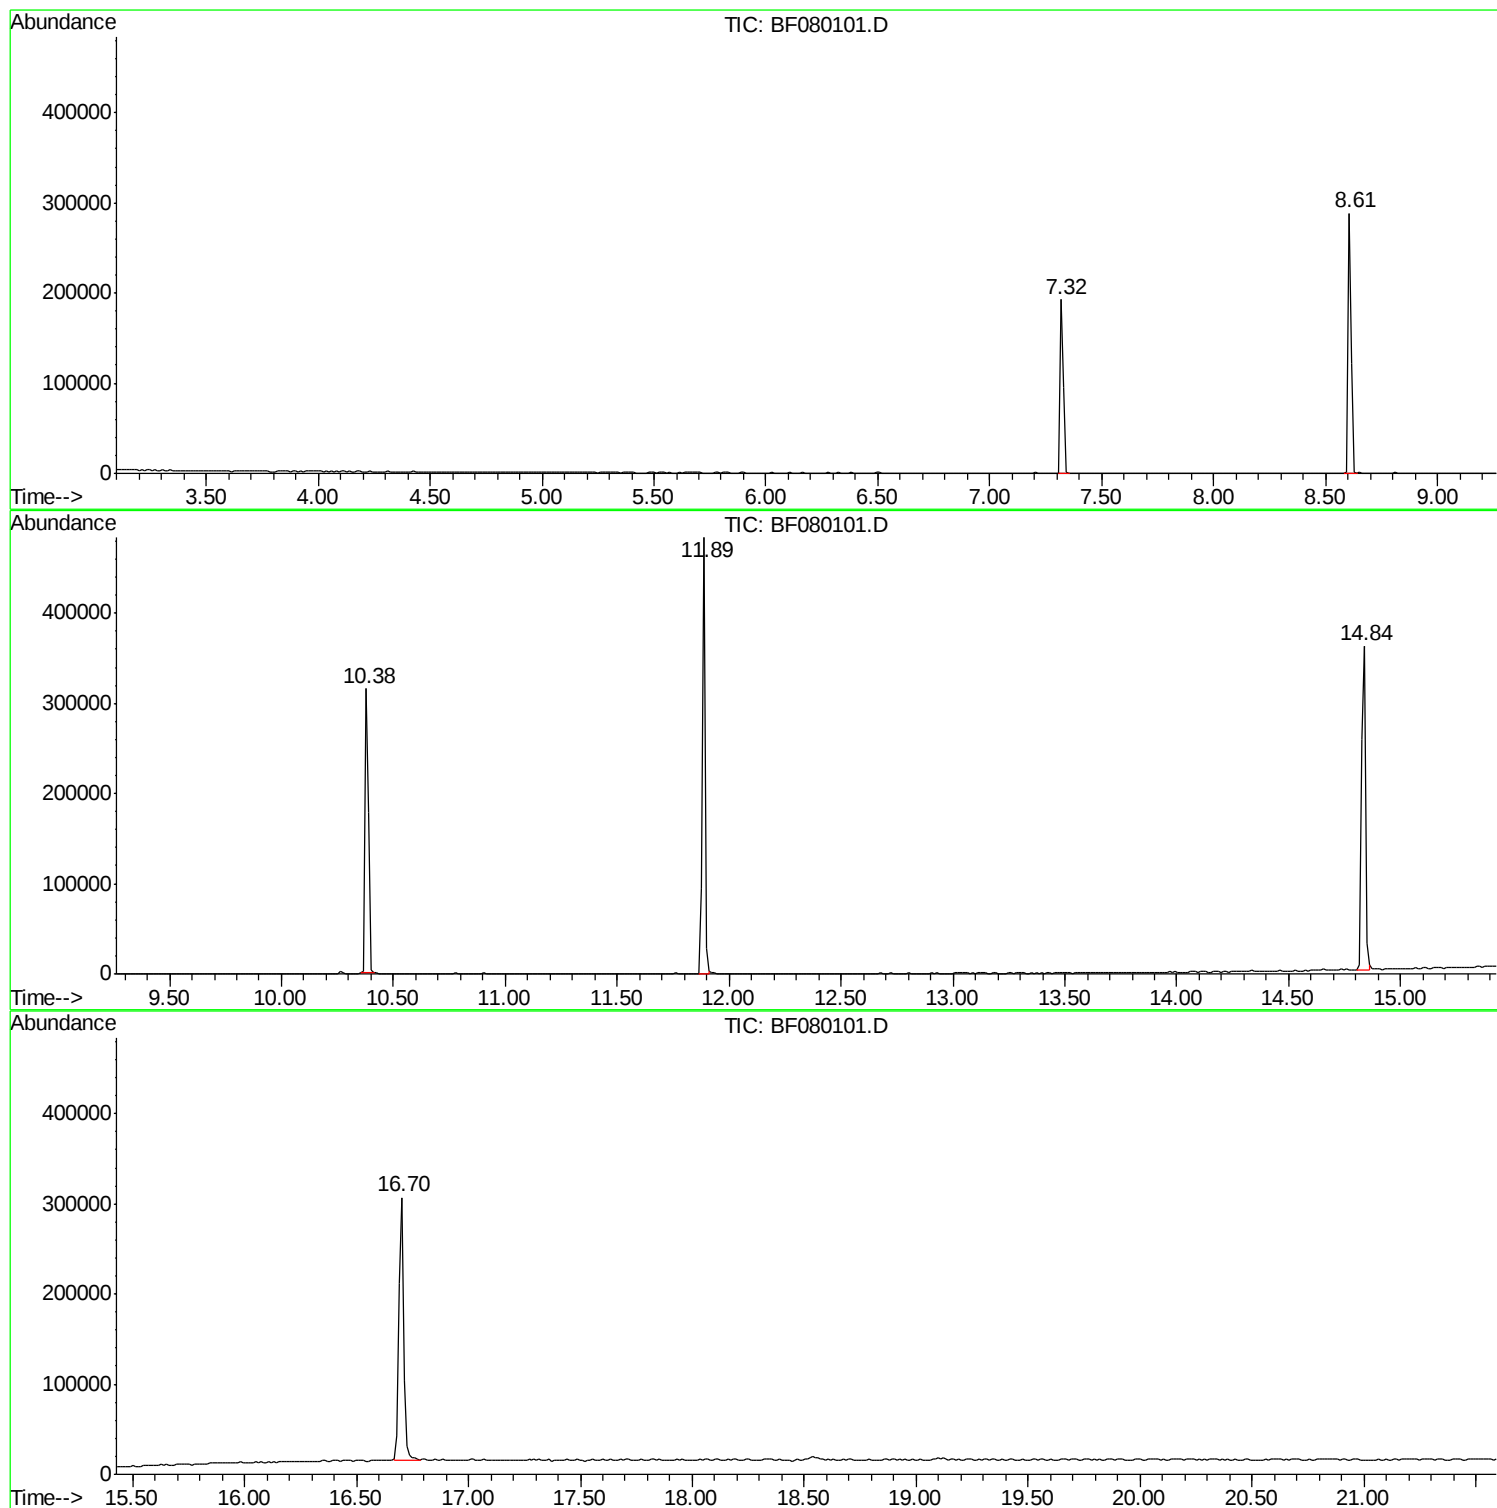

Data Path : Z:\HPCHEM1\BNA_F\Data\BF062215\
Data File : BF080101.D
Acq On : 22 Jun 2015 18:36
Operator : TP/IZ
Sample : G2728-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\Data\BF062215\
Data File : BF080101.D
Acq On : 22 Jun 2015 18:36
Operator : TP/IZ
Sample : G2728-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF061715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc