
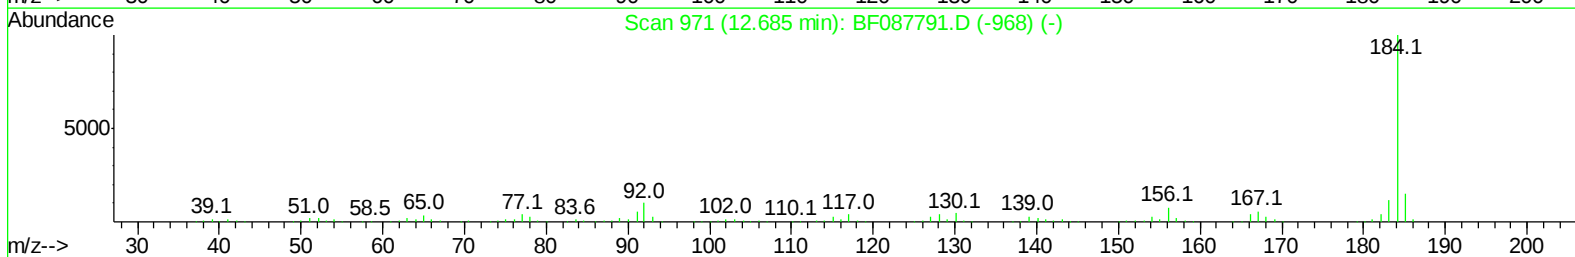
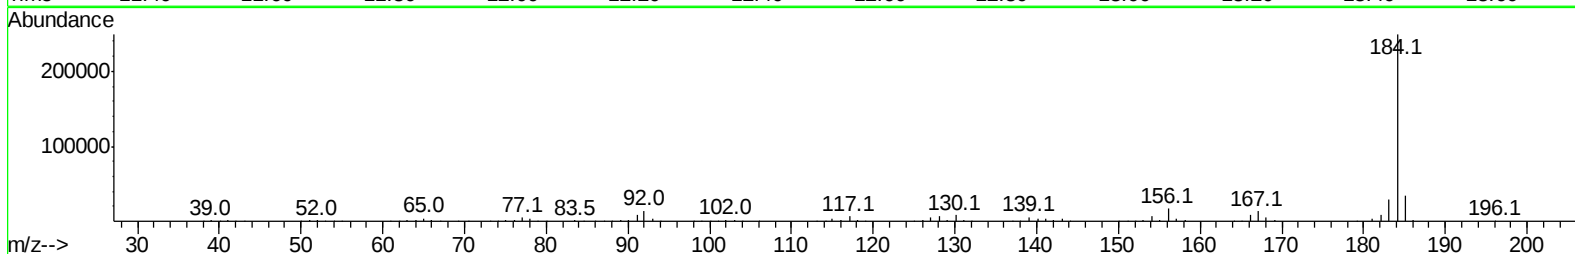


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062216\
Data File : BF088246.D
Acq On : 22 Jun 2016 13:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 08:54:22 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

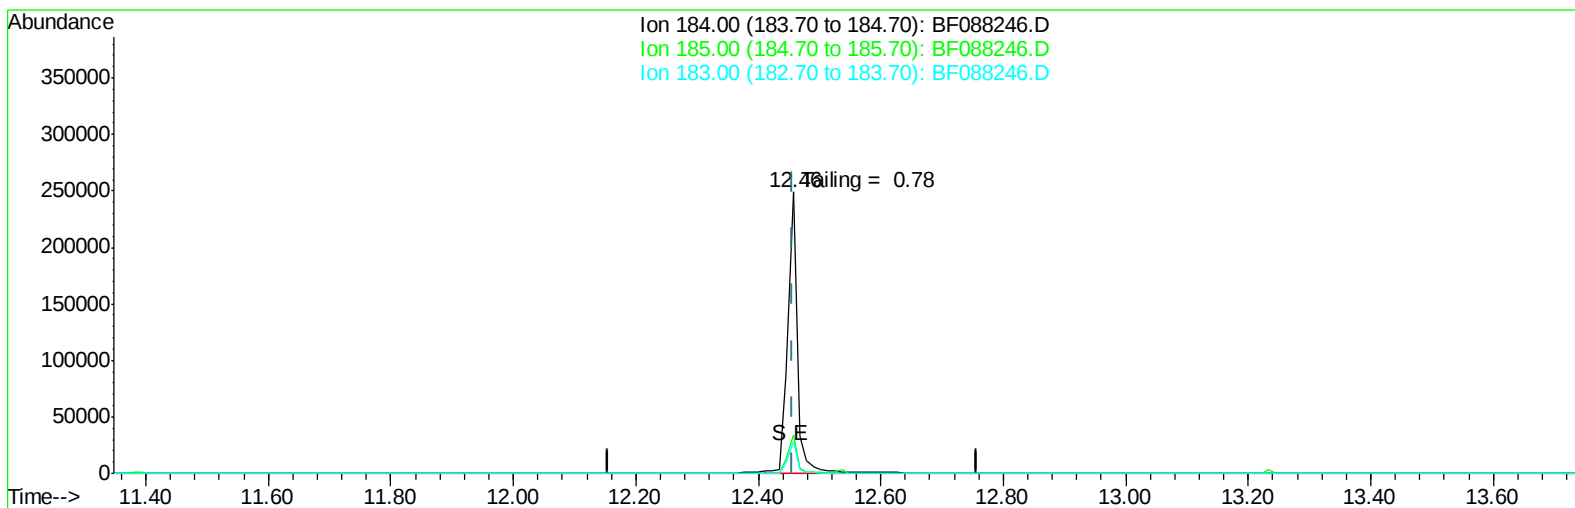

TIC: BF088246.D

(76) Benzidine




12.456min (-0.000) 47783.53ng

response 287108

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	13.85
183.00	11.60	11.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062216\
Data File : BF088246.D
Acq On : 22 Jun 2016 13:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 08:54:22 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

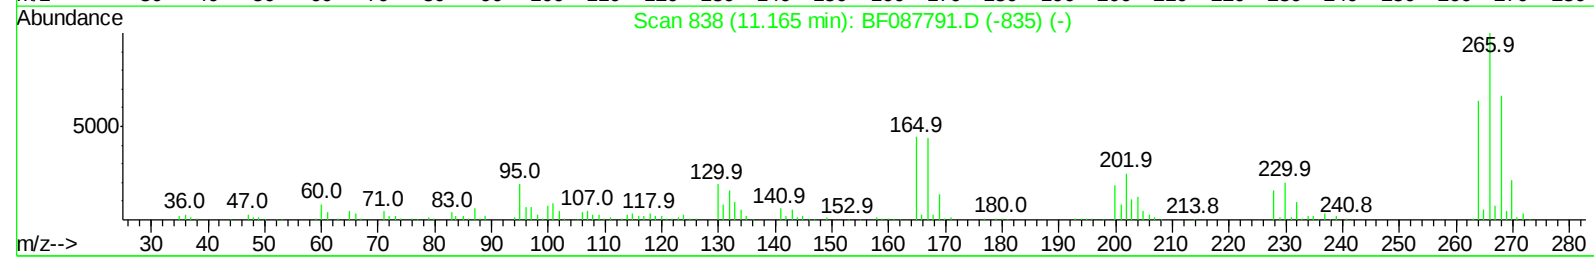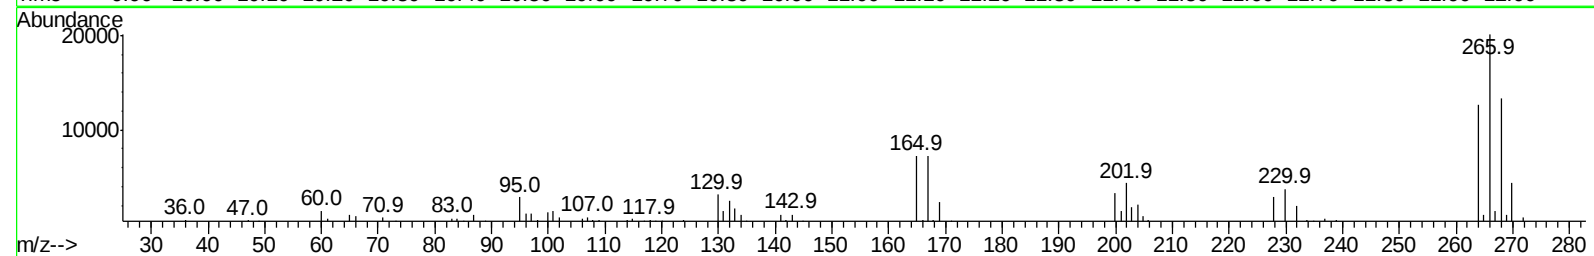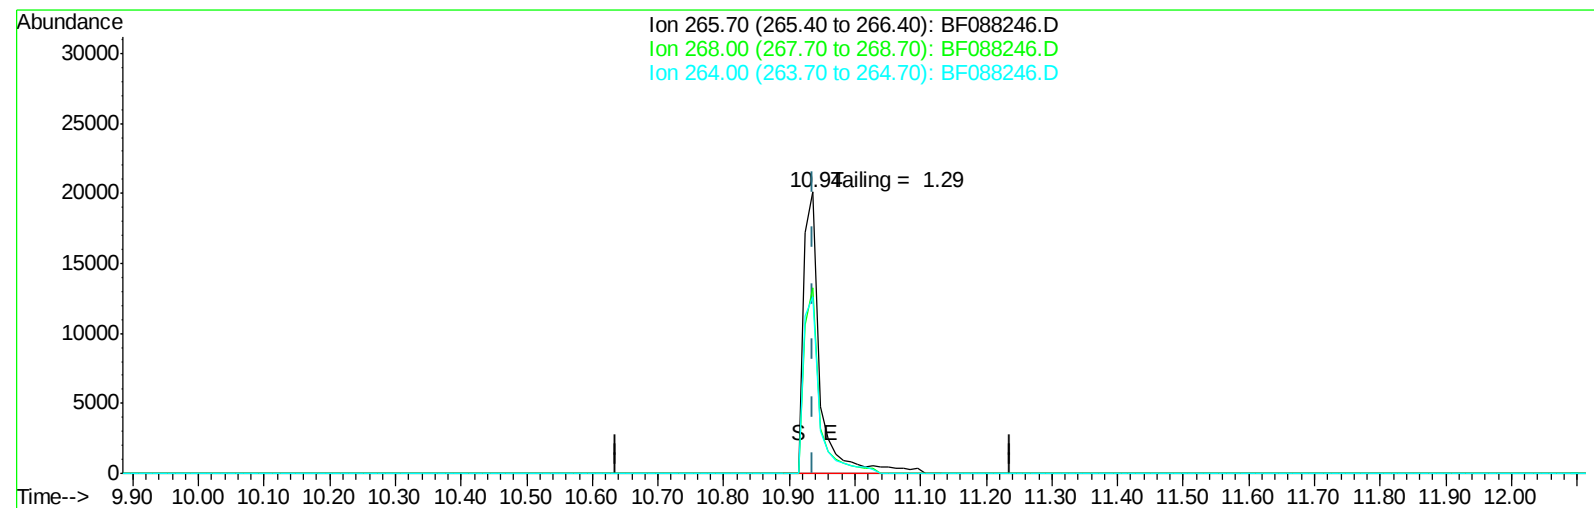

TIC: BF088246.D

(69) Pentachlorophenol (C)

10.936min (-0.000) 0.00ng

response 35392

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	66.05
264.00	62.00	62.75
0.00	0.00	0.00