
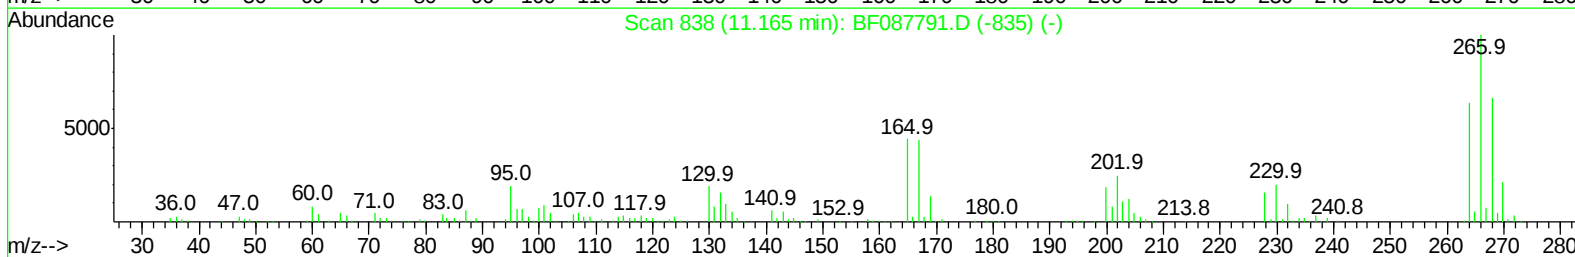
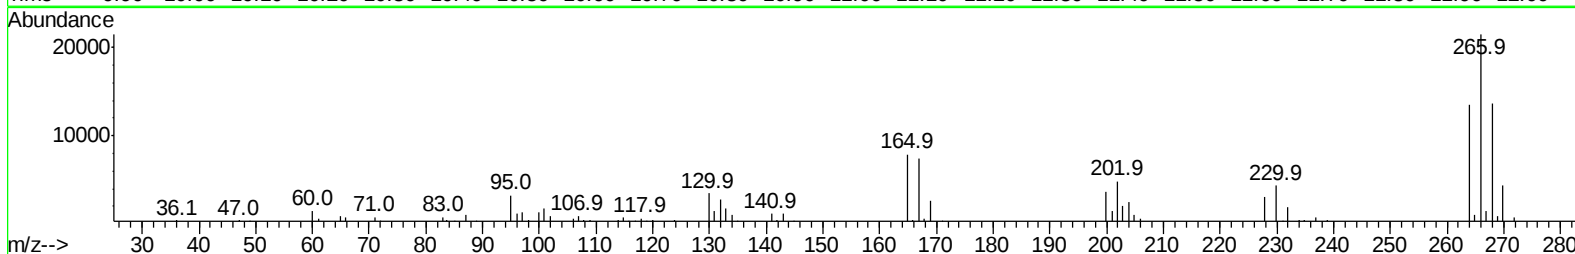


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062216\
Data File : BF088271.D
Acq On : 23 Jun 2016 2:22
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 08:55:09 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

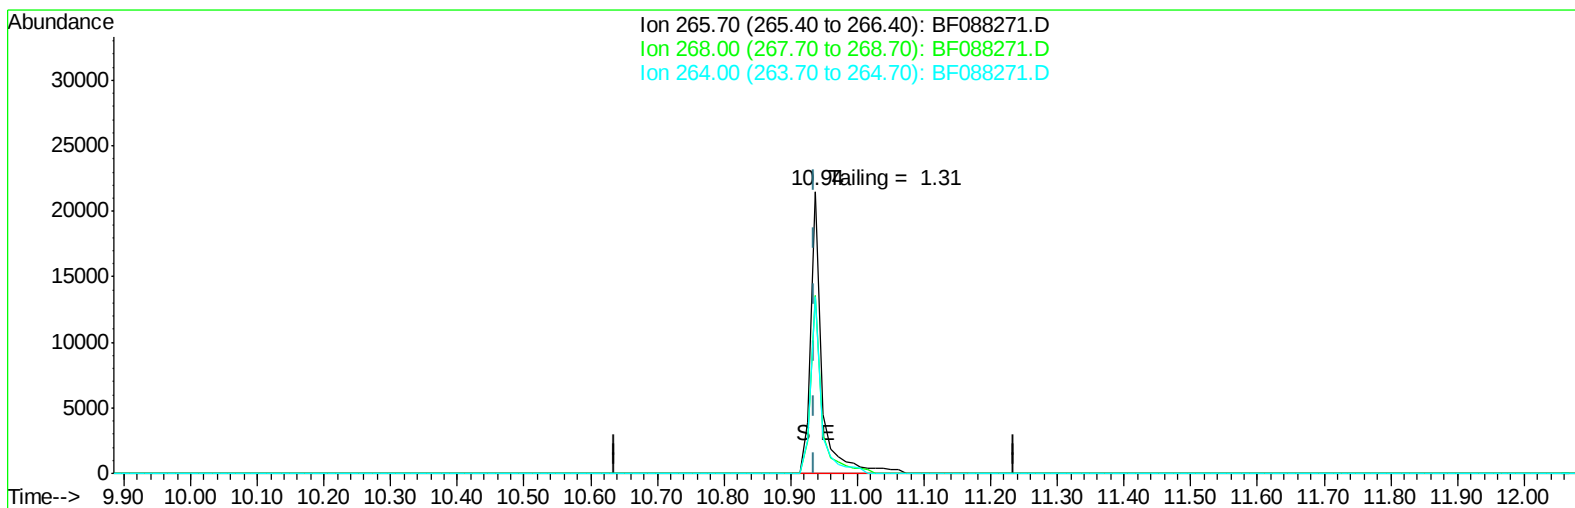

TIC: BF088271.D

(69) Pentachlorophenol (C)




10.936min (+0.000) 0.00ng

response 25493

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	63.28
264.00	62.00	62.58
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062216\
 Data File : BF088271.D
 Acq On : 23 Jun 2016 2:22
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 08:55:09 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 22 14:55:14 2016
 Response via : Initial Calibration

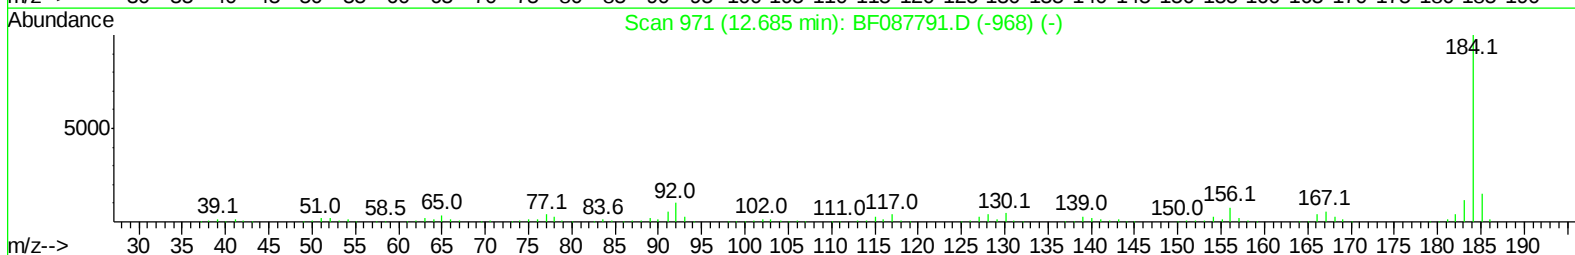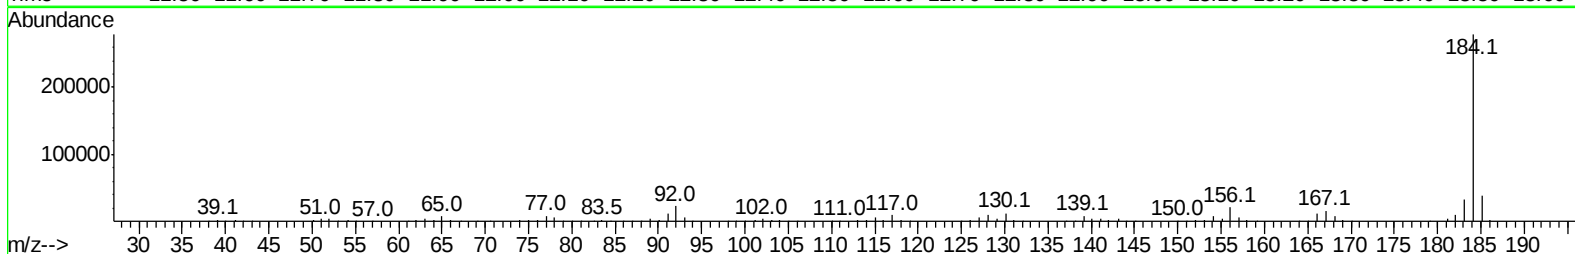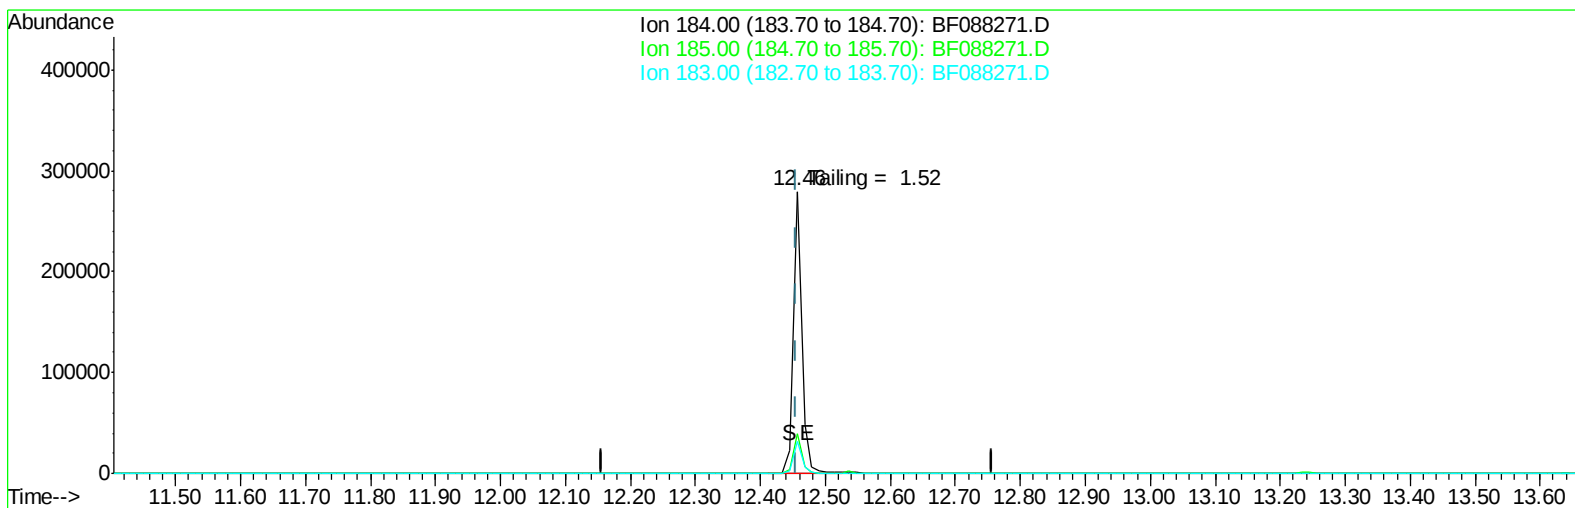

TIC: BF088271.D

(76) Benzidine

12.456min (+0.000) 21233.84ng

response 251640

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.04
183.00	11.60	11.55
0.00	0.00	0.00