


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062216\
 Data File : BF088271.D
 Acq On : 23 Jun 2016 2:22
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 22 14:55:14 2016

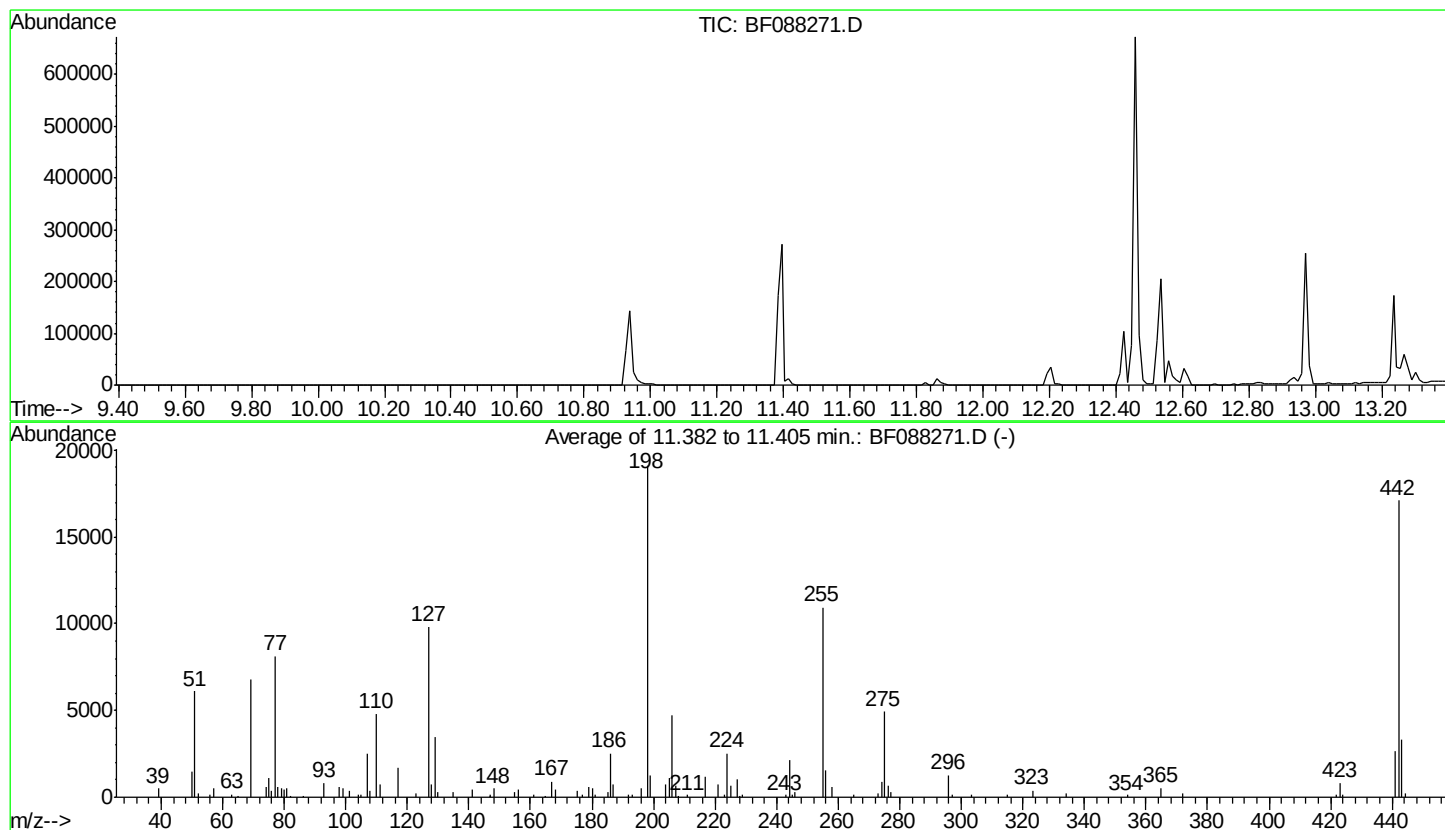

AutoFind: Scans 857, 858, 859; Background Corrected with Scan 854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	6122	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.4	6768	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.4	9828	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19109	PASS
199	198	5	9	6.6	1261	PASS
275	198	10	60	25.8	4929	PASS
365	198	1	100	2.8	534	PASS
441	442	0.01	24	15.7	2687	PASS
442	198	50	100	89.5	17110	PASS
443	442	15	24	19.4	3321	PASS