
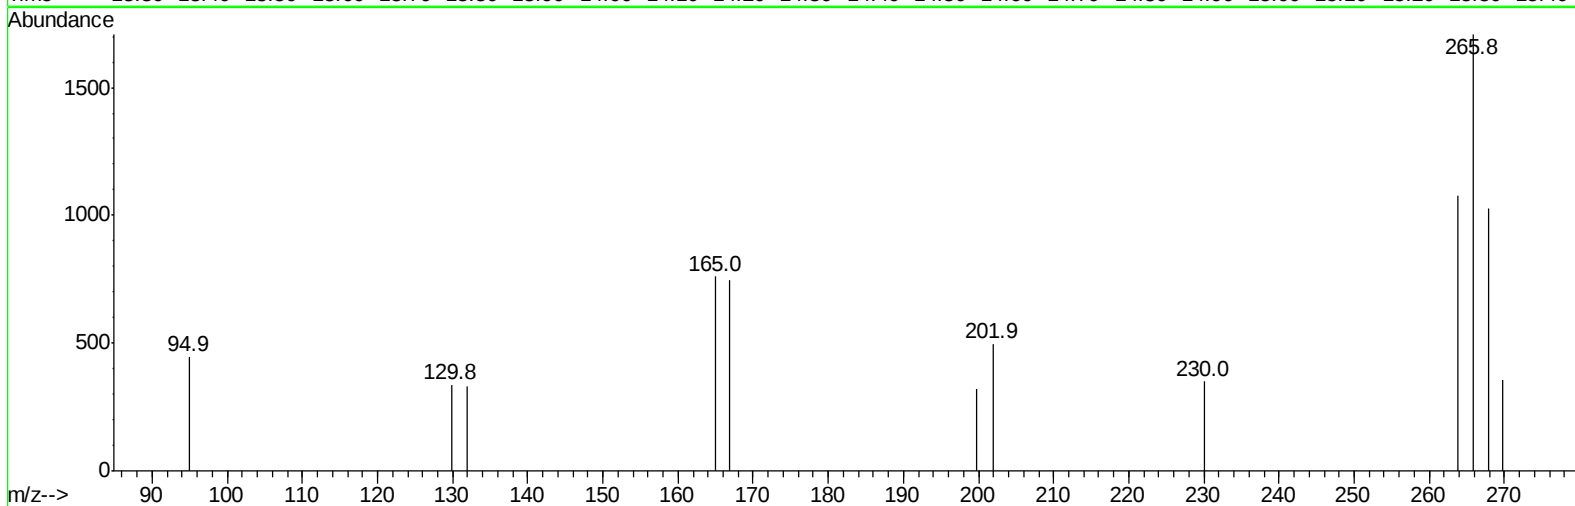


Data Path : Z:\HPCHEM1\BNA F\DATA\BF062217\
Data File : BF096137.D
Acq On : 22 Jun 2017 23:51
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 07:26:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

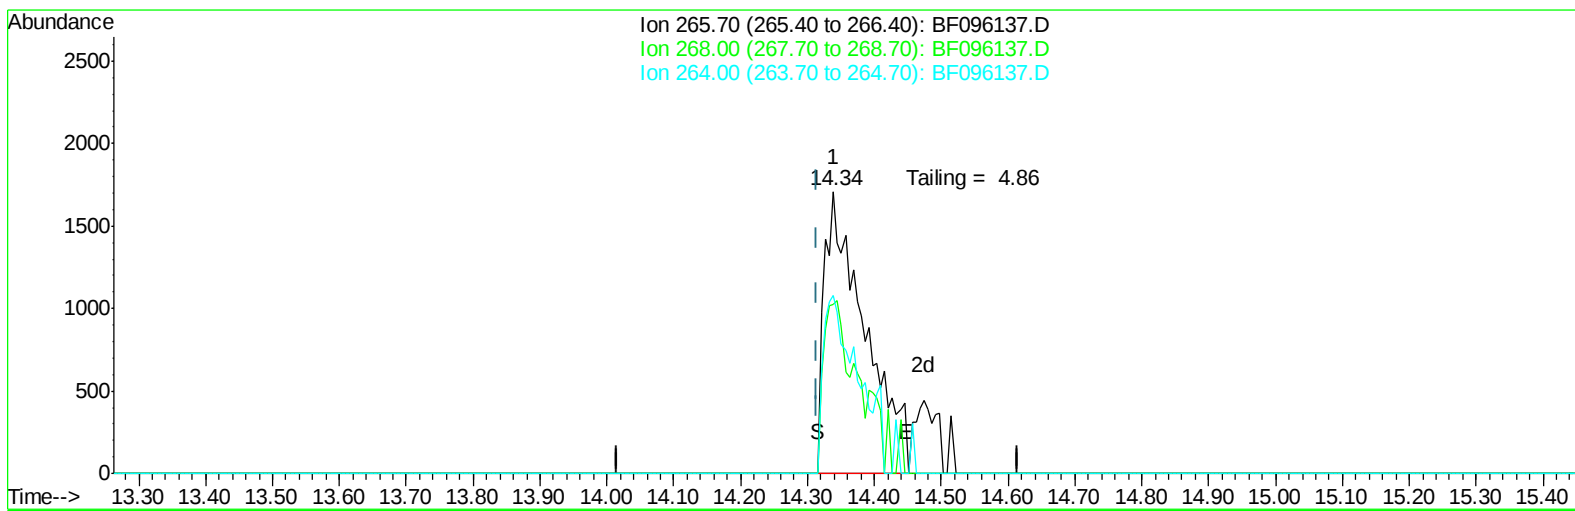

TIC: BF096137.D

(69) Pentachlorophenol (C)



14.339min (+0.024) 0.00ng

response 7102

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.13
264.00	64.60	63.06
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF062217\
Data File : BF096137.D
Acq On : 22 Jun 2017 23:51
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 07:26:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

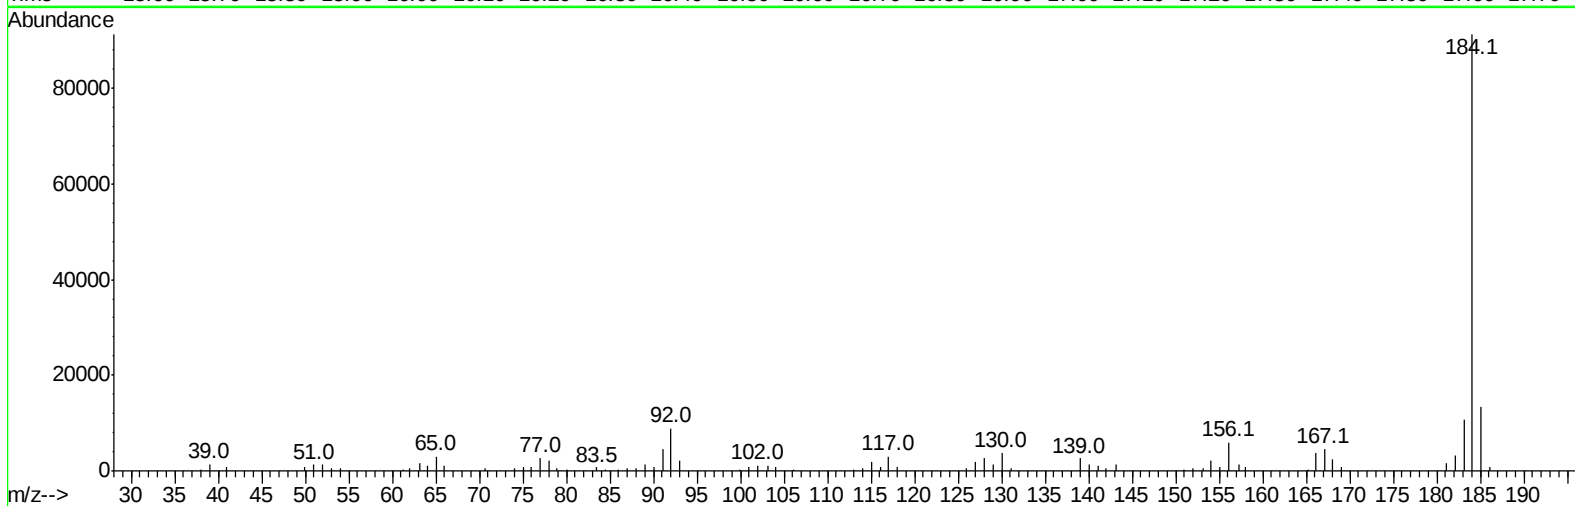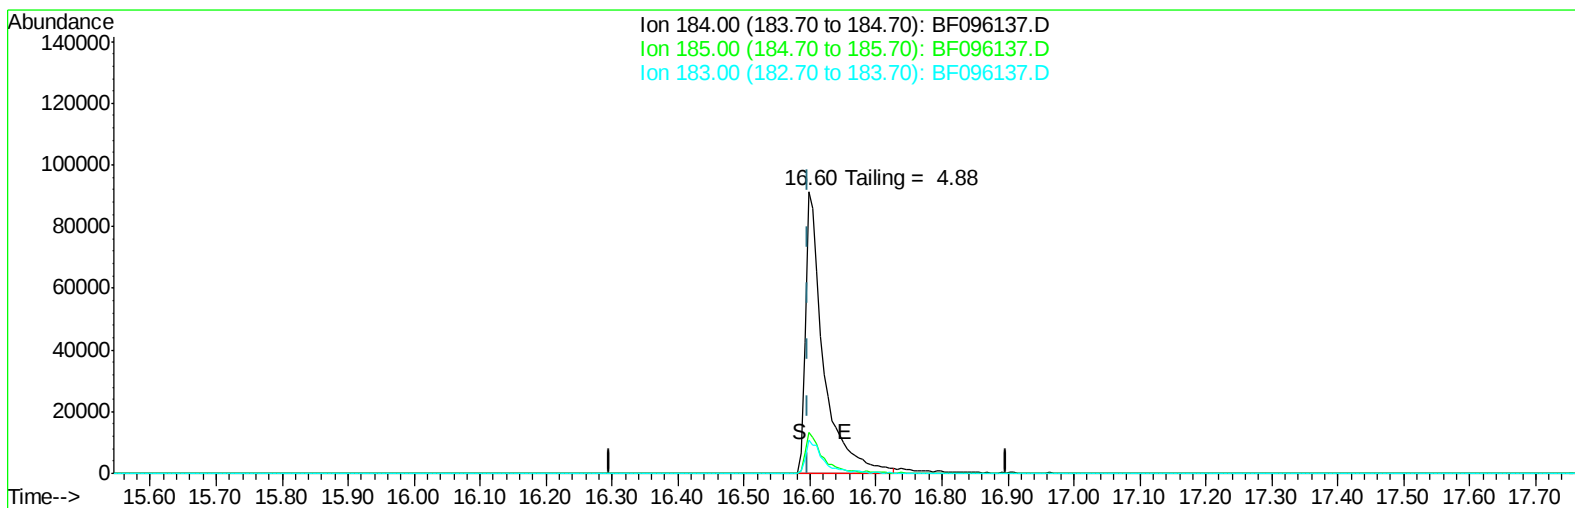

TIC: BF096137.D

(76) Benzidine

16.598min (+0.000) 0.00ng

response 177014

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.64#
183.00	12.20	11.71
0.00	0.00	0.00