

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF062217\
 Data File : BF096130.D
 Acq On : 22 Jun 2017 19:32
 Operator : SJ/MA
 Sample : I3844-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-008

Quant Time: Jun 23 01:42:18 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 16:05:47 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.27	152	93979	20.00	ng	-0.02
21) Naphthalene-d8	9.31	136	351799	20.00	ng	-0.02
38) Acenaphthene-d10	12.13	164	153269	20.00	ng	-0.02
63) Phenanthrene-d10	14.53	188	250866	20.00	ng	-0.01
75) Chrysene-d12	18.27	240	185701	20.00	ng	0.00
86) Perylene-d12	19.94	264	155144	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	695556	117.93	ng	-0.02
7) Phenol-d6	6.86	99	842263	119.29	ng	-0.02
23) Nitrobenzene-d5	8.20	82	469465	82.88	ng	-0.02
41) 2,4,6-Tribromophenol	13.43	330	118127	87.11	ng	-0.02
44) 2-Fluorobiphenyl	11.09	172	836383	75.94	ng	-0.02
78) Terphenyl-d14	16.92	244	488935	65.34	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	11.79	163	156929	13.49	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF062217\
Data File : BF096130.D
Acq On : 22 Jun 2017 19:32
Operator : SJ/MA
Sample : I3844-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-008

Quant Time: Jun 23 01:42:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 16:05:47 2017
Response via : Initial Calibration

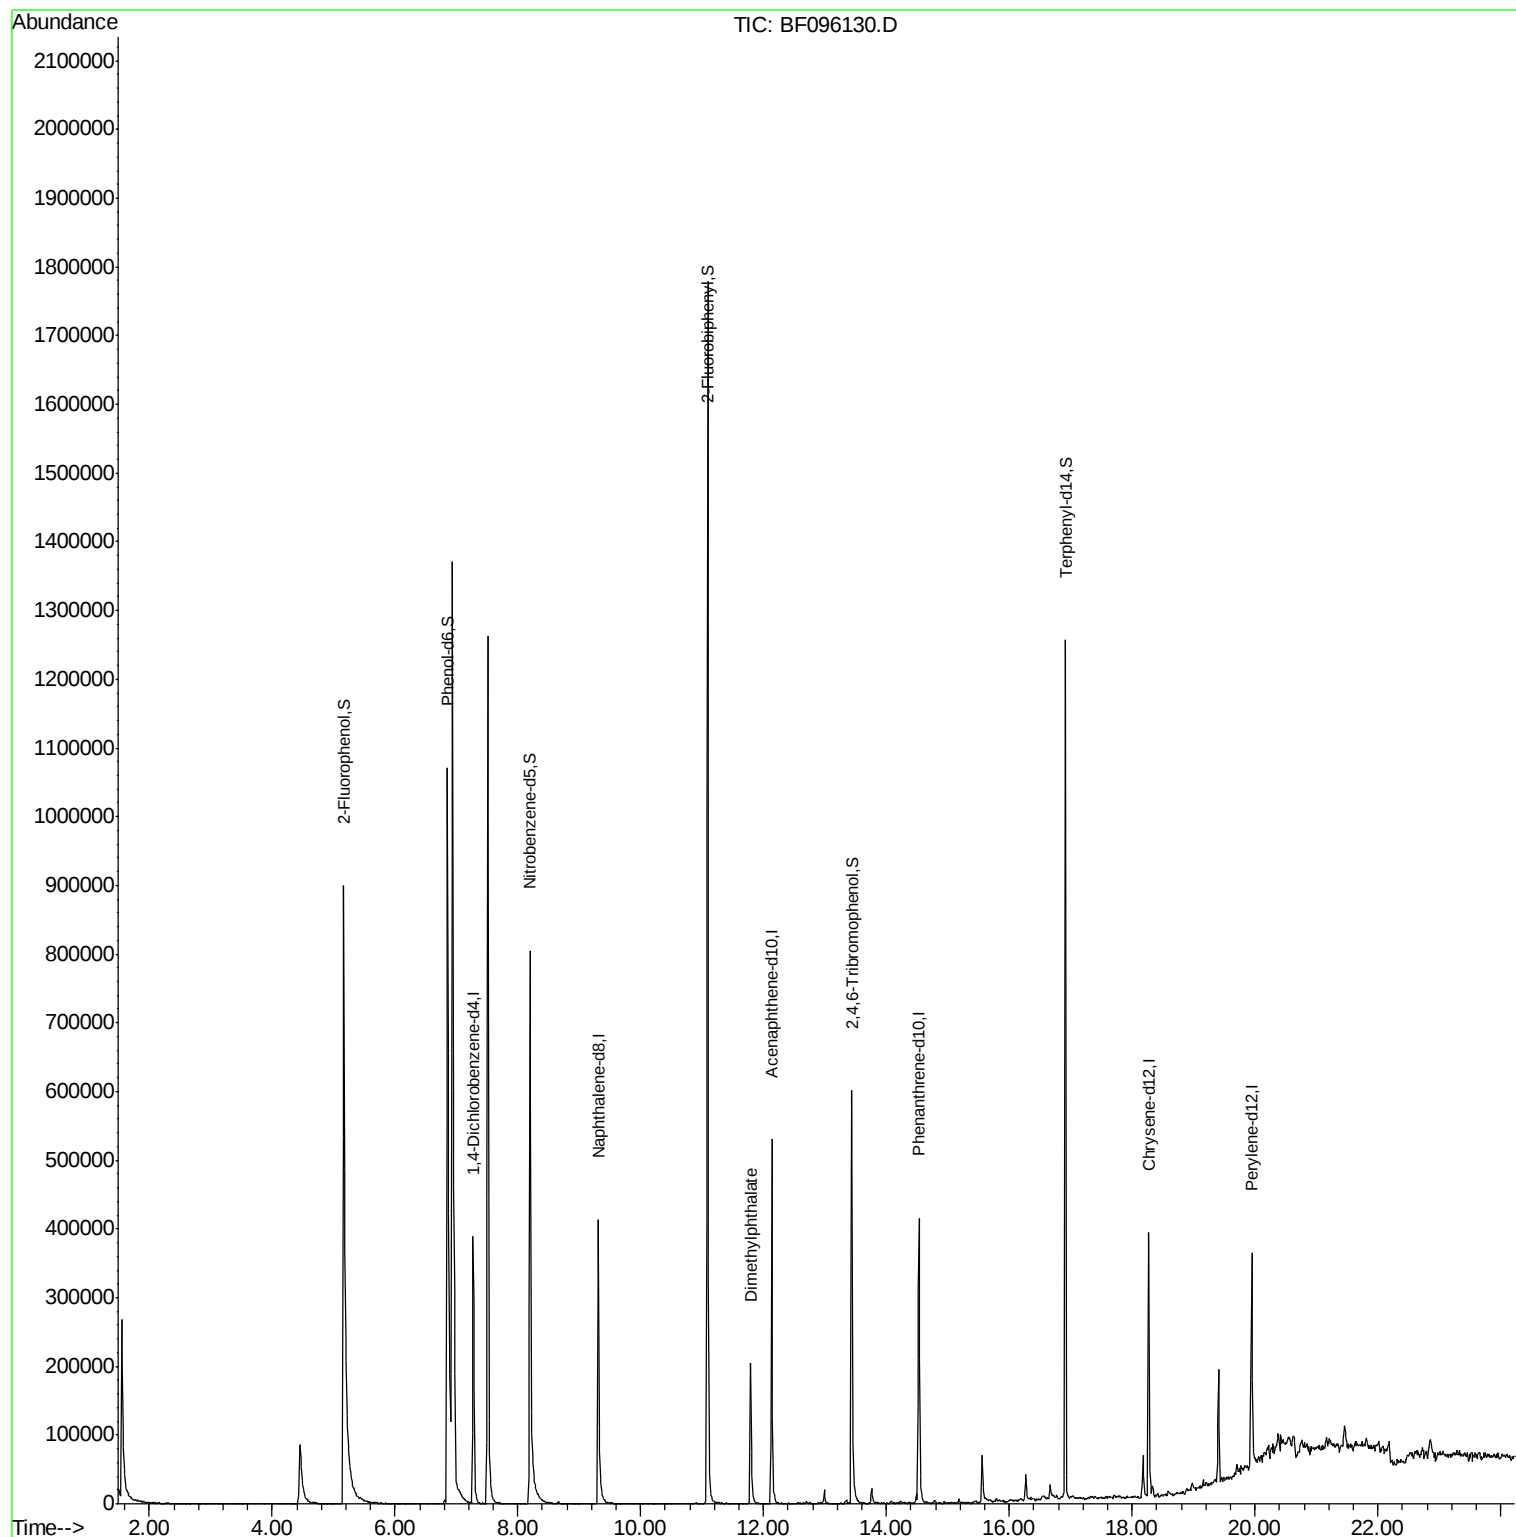

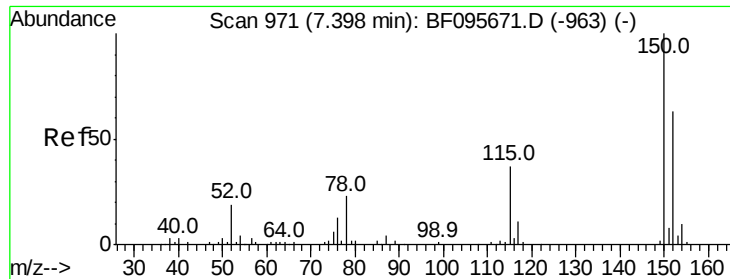


#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.27 min Scan# 984
Delta R.T. -0.02 min
Lab File: BF096130.D
Acq: 22 Jun 2017 19:32

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-008

Tot Ion:152 Resp: 93979
Ion Ratio Lower Upper
152 100
150 159.0 126.2 189.2
115 62.1 52.2 78.2

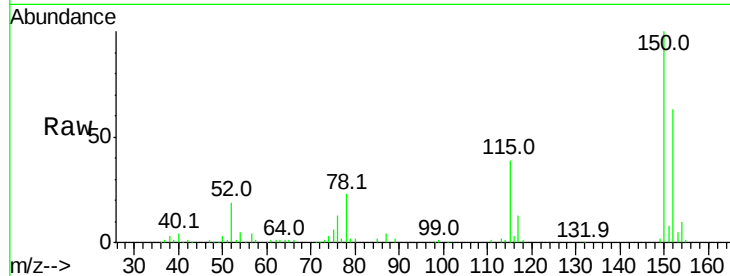


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

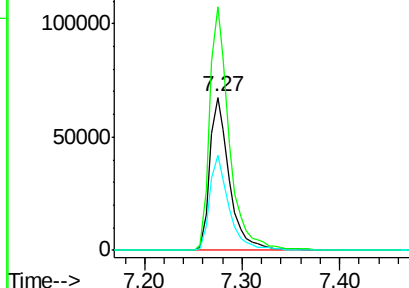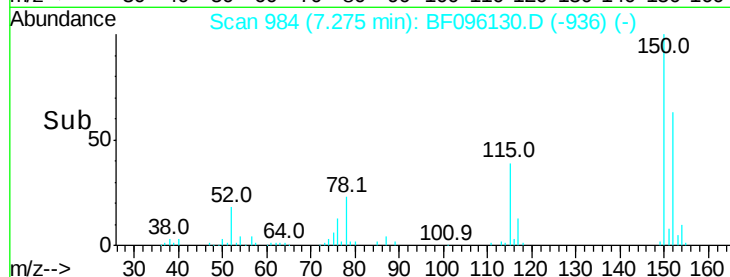



#5

2-Fluorophenol
Concen: 117.93 ng
RT: 5.16 min Scan# 625
Delta R.T. -0.02 min
Lab File: BF096130.D
Acq: 22 Jun 2017 19:32

Tgt Ion:112 Resp: 695556
Ion Ratio Lower Upper
112 100
64 57.7 46.0 69.0
63 27.0 23.4 35.0

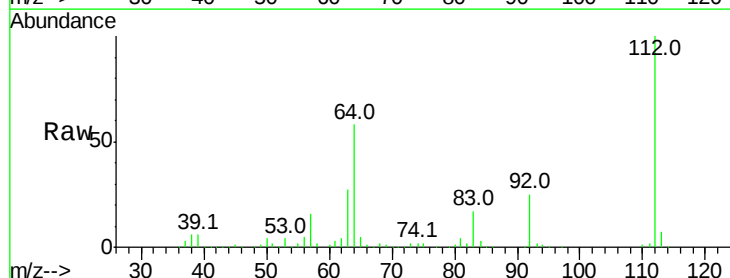

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

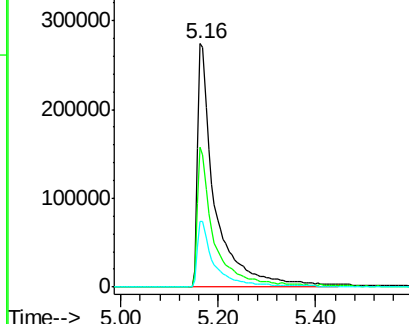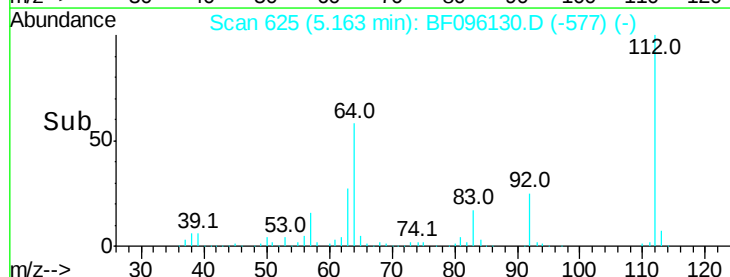



#7

Phenol-d6

Concen: 119.29 ng

RT: 6.86 min Scan# 913

Delta R.T. -0.02 min

Lab File: BF096130.D

Acq: 22 Jun 2017 19:32

Instrument :

BNA_F

ClientSampleId :

FK-PS-01-008


Tot Ion: 99 Resp: 842263

Ion Ratio Lower Upper

99 100

42 15.8 13.5 20.3




71 30.6 24.5 36.7

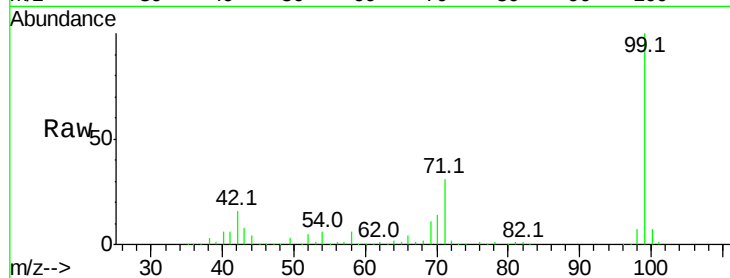

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

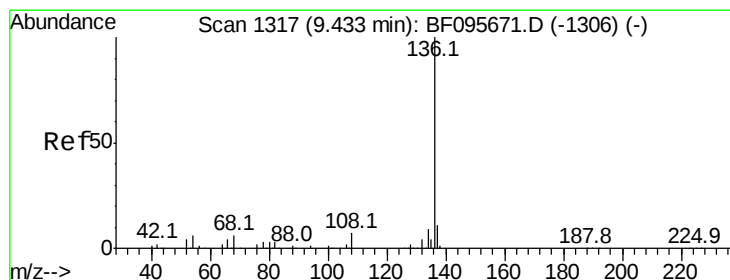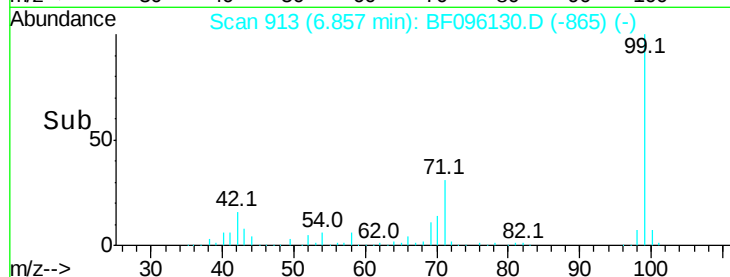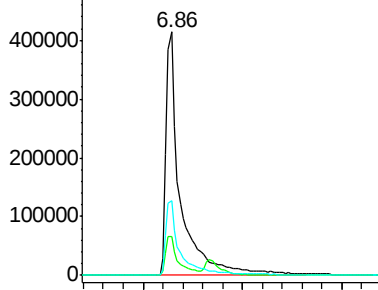

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.31 min Scan# 1330

Delta R.T. -0.02 min

Lab File: BF096130.D

Acq: 22 Jun 2017 19:32

Tgt Ion: 136 Resp: 351799


Ion Ratio Lower Upper

136 100

137 10.7 8.5 12.7

54 6.8 4.9 7.3

68 6.1 4.1 6.1#


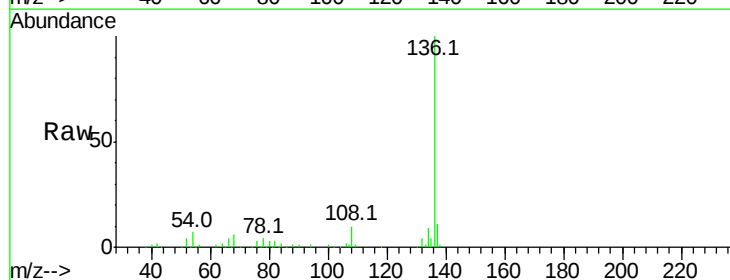



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



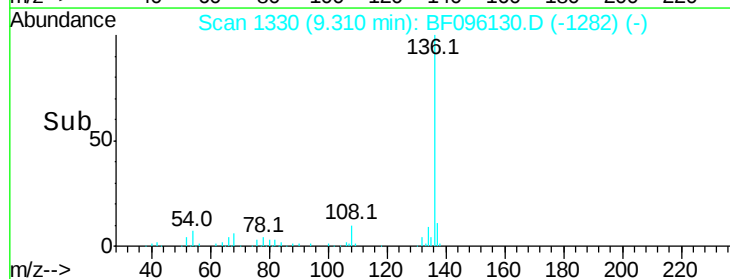
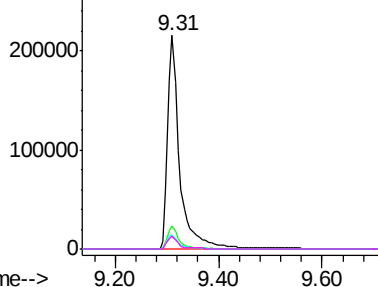


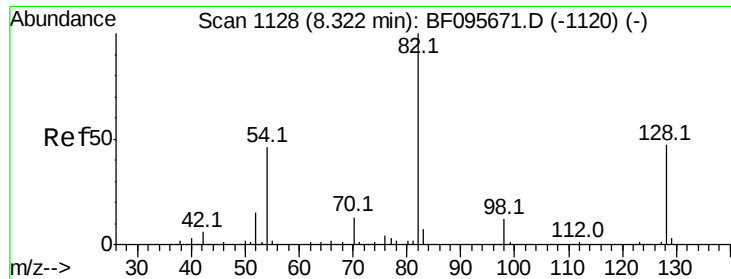

#23
 Nitrobenzene-d5
 Concen: 82.88 ng
 RT: 8.20 min Scan# 1141
 Delta R.T. -0.02 min
 Lab File: BF096130.D
 Acq: 22 Jun 2017 19:32




Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-008


Tot Ion	82	Resp	469465
Ion Ratio	Lower	Upper	
82	100		
128	47.4	34.0	51.0
54	48.2	42.2	63.2

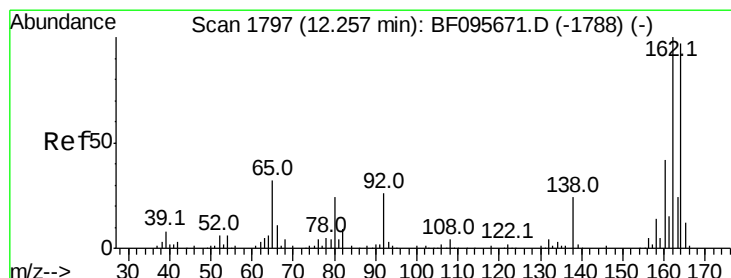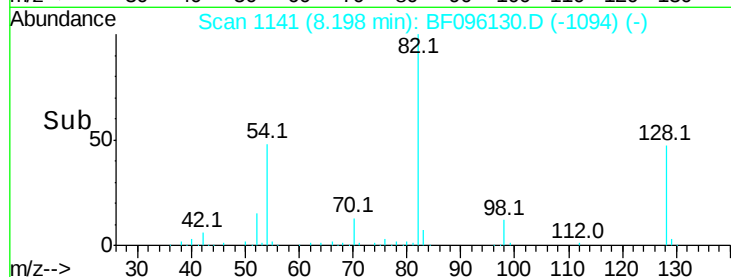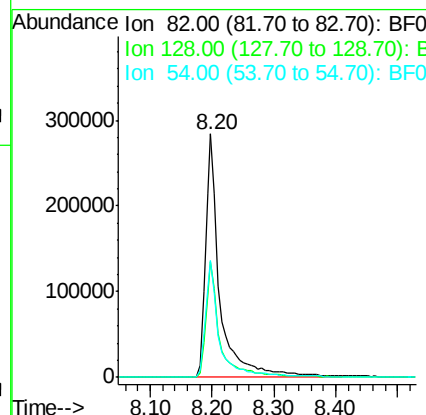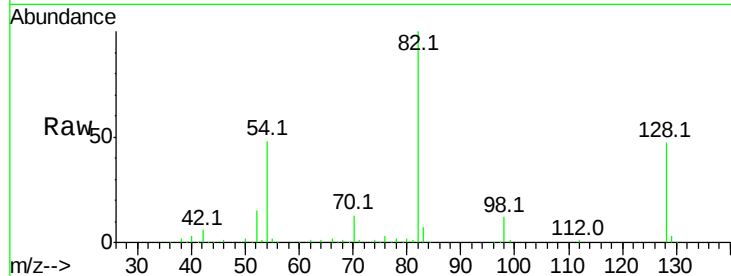

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.13 min Scan# 1809
 Delta R.T. -0.02 min
 Lab File: BF096130.D
 Acq: 22 Jun 2017 19:32

Tgt Ion	164	Resp	153269
Ion Ratio	Lower	Upper	
164	100		
162	105.0	82.6	123.8
160	45.8	36.2	54.2

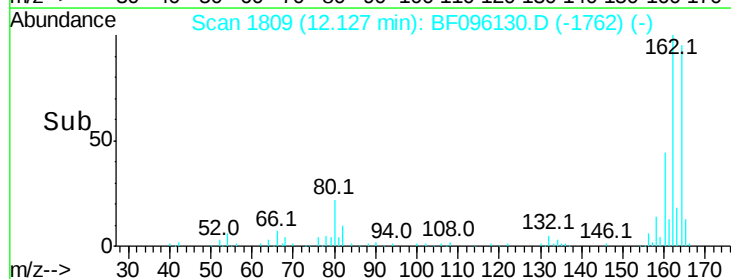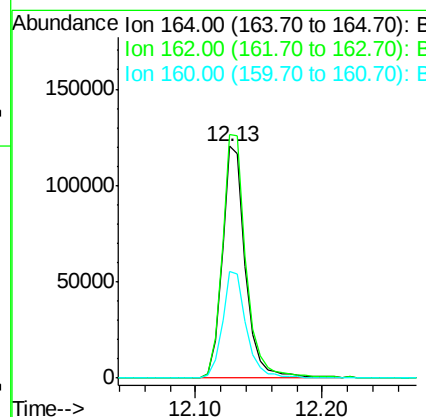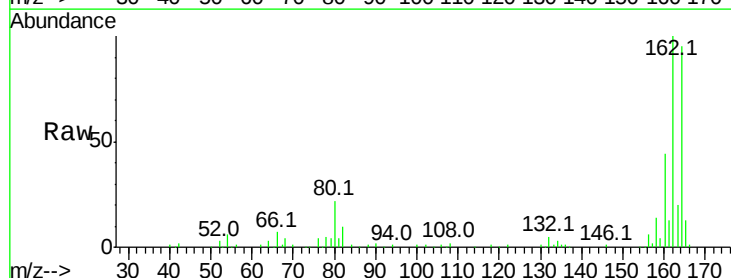


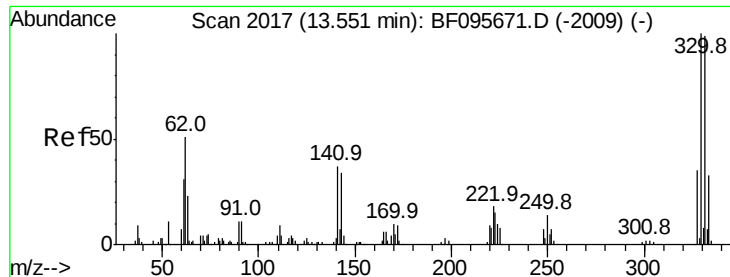




#41
 2,4,6-Tribromophenol
 Concen: 87.11 ng
 RT: 13.43 min Scan# 2031
 Delta R.T. -0.02 min
 Lab File: BF096130.D
 Acq: 22 Jun 2017 19:32

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-008

Tot Ion:330 Resp: 118127
 Ion Ratio Lower Upper
 330 100
 332 98.6 76.6 115.0
 141 39.9 31.4 47.2

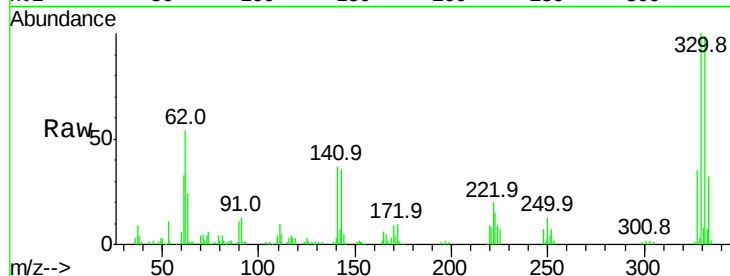


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

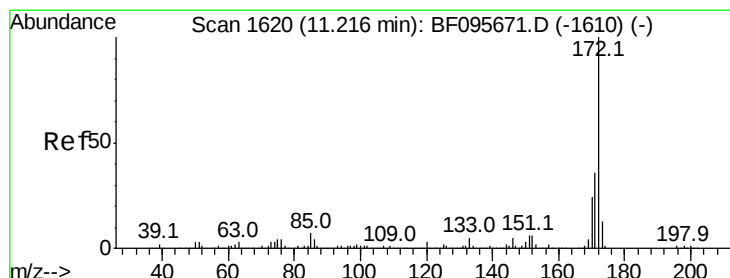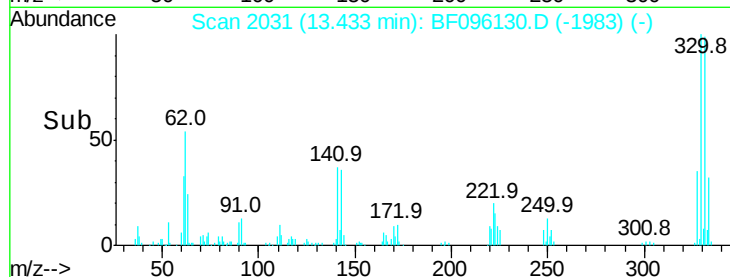
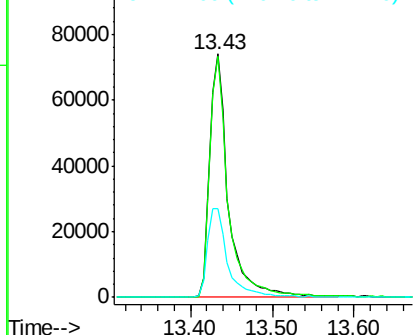


#44
 2-Fluorobiphenyl
 Concen: 75.94 ng
 RT: 11.09 min Scan# 1633
 Delta R.T. -0.02 min
 Lab File: BF096130.D
 Acq: 22 Jun 2017 19:32

Tgt Ion:172 Resp: 836383
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.6 44.4
 170 23.5 19.8 29.8

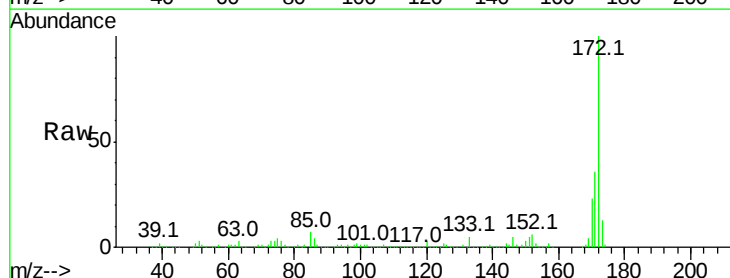

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

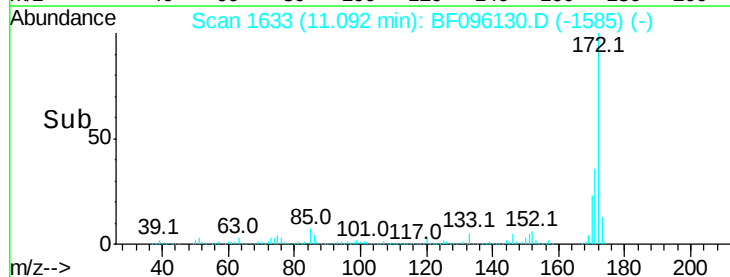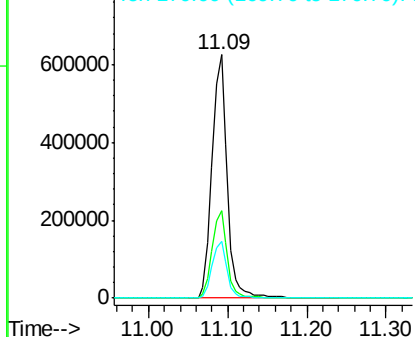



#49

Dimethylphthalate

Concen: 13.49 ng

RT: 11.79 min Scan# 1752

Delta R.T. -0.03 min

Lab File: BF096130.D

Acq: 22 Jun 2017 19:32

Instrument :

BNA_F

ClientSampleId :

FK-PS-01-008


Tot Ion:163 Resp: 156929

Ion Ratio Lower Upper

163 100

194 3.7 2.6 4.0




164 10.1 8.4 12.6

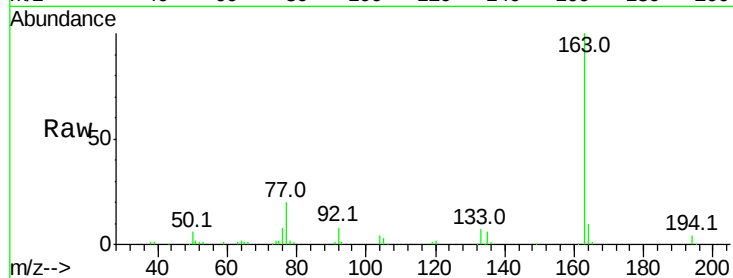

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

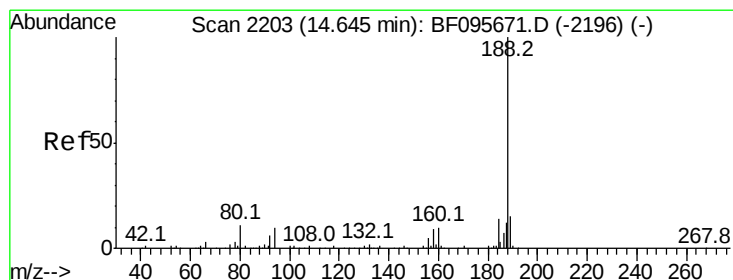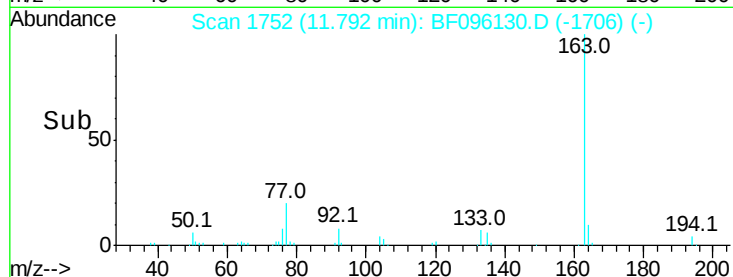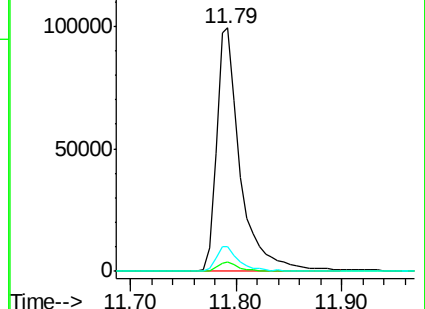

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.53 min Scan# 2217

Delta R.T. -0.01 min

Lab File: BF096130.D

Acq: 22 Jun 2017 19:32


Tgt Ion:188 Resp: 250866

Ion Ratio Lower Upper

188 100

94 11.1 9.4 14.2



80 12.0 10.2 15.2

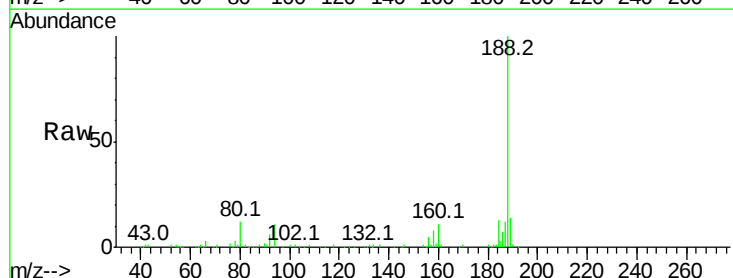

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

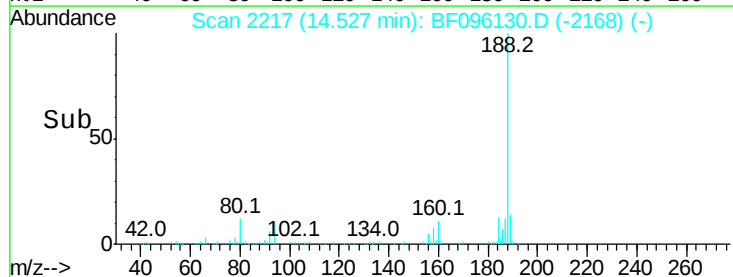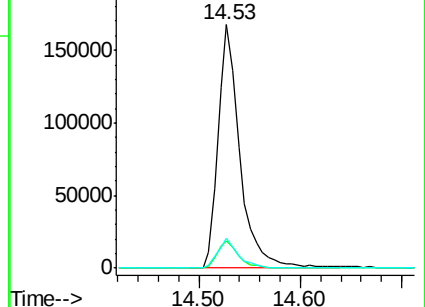







#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.27 min Scan# 2853
Delta R.T. -0.01 min
Lab File: BF096130.D
Acq: 22 Jun 2017 19:32

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-008

Tot Ion:240 Resp: 185701
Ion Ratio Lower Upper
240 100
120 14.3 5.8 8.8#
236 25.0 20.5 30.7

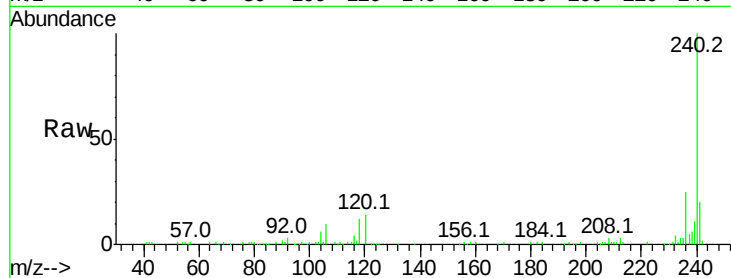


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

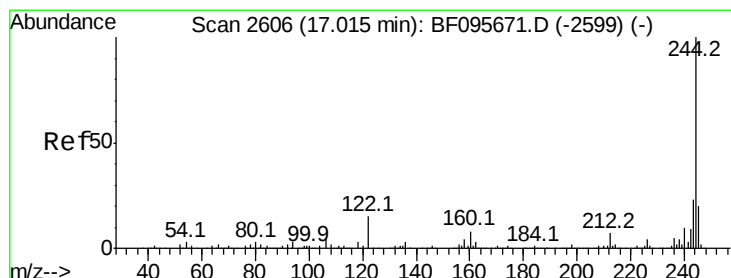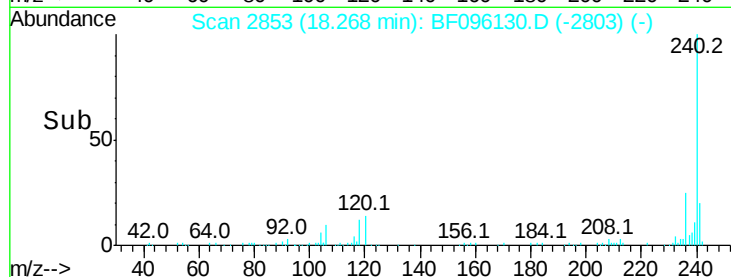
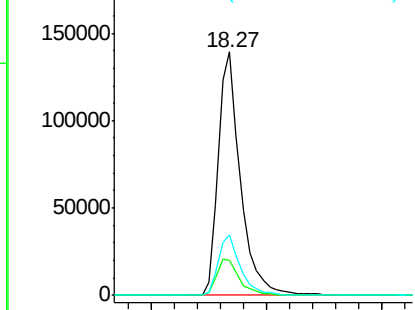





#78
Terphenyl-d14
Concen: 65.34 ng
RT: 16.92 min Scan# 2623
Delta R.T. -0.01 min
Lab File: BF096130.D
Acq: 22 Jun 2017 19:32

Tgt Ion:244 Resp: 488935
Ion Ratio Lower Upper
244 100
212 6.9 6.0 9.0
122 13.8 10.3 15.5

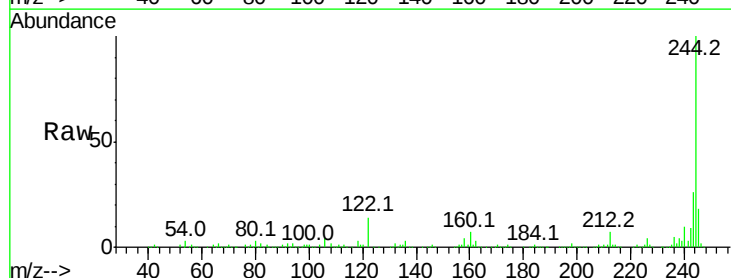

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

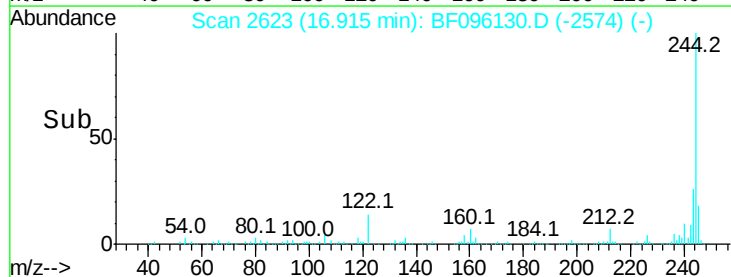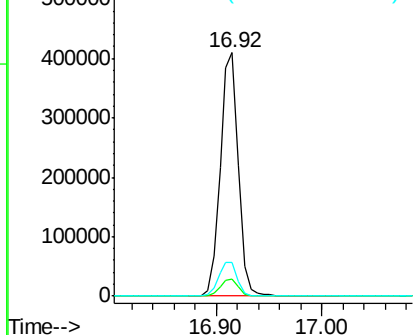

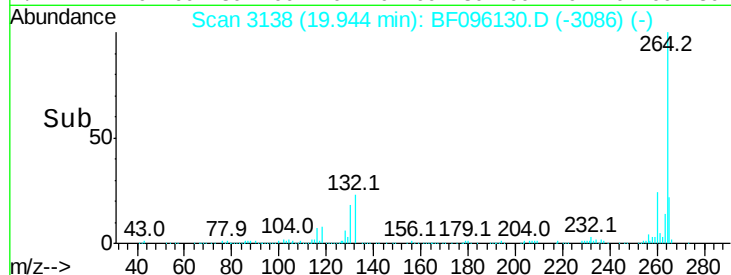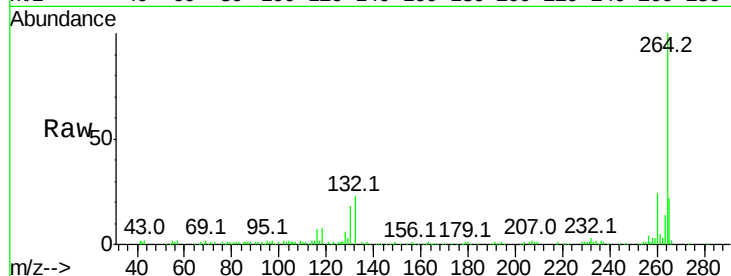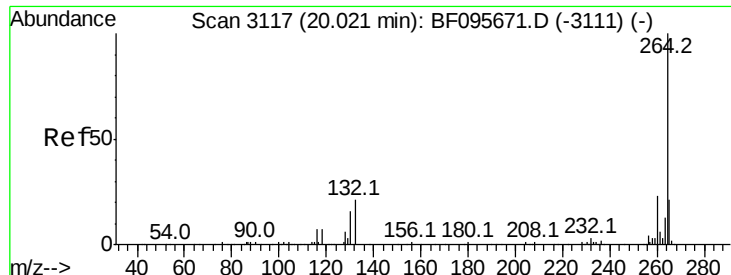

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 19.94 min Scan# 3138
 Delta R.T. 0.01 min
 Lab File: BF096130.D
 Acq: 22 Jun 2017 19:32

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-008

Tot Ion:	264	Resp:	155144
Ion Ratio	Lower	Upper	
264	100		
260	24.0	19.5	29.3
265	22.2	17.2	25.8

