

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062217\
 Data File : BF096123.D
 Acq On : 22 Jun 2017 15:44
 Operator : SJ/MA
 Sample : I3697-01RE 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-SF-02-001-ARE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.546	8	10	51	rVB	741751	1522046	100.00%	18.431%
2	4.428	497	500	508	rBV2	16257	40862	2.68%	0.495%
3	5.263	637	642	646	rBV2	15148	32045	2.11%	0.388%
4	6.922	921	924	930	rBV3	35612	90531	5.95%	1.096%
5	6.975	930	933	949	rVV	87810	279018	18.33%	3.379%
6	7.275	980	984	997	rBV	395924	580635	38.15%	7.031%
7	7.516	1021	1025	1042	rBV	125128	214650	14.10%	2.599%
8	8.234	1143	1147	1156	rBV2	38488	100201	6.58%	1.213%
9	8.322	1159	1162	1169	rVB4	16417	28530	1.87%	0.345%
10	9.310	1326	1330	1343	rBV	539328	820992	53.94%	9.942%
11	9.410	1345	1347	1354	rVB2	13551	20715	1.36%	0.251%
12	11.092	1628	1633	1645	rBV	193167	277281	18.22%	3.358%
13	11.316	1666	1671	1676	rVB2	14269	19031	1.25%	0.230%
14	11.798	1746	1753	1758	rBV	23221	41433	2.72%	0.502%
15	12.127	1804	1809	1815	rBV2	518445	698898	45.92%	8.463%
16	12.180	1815	1818	1825	rVB3	31572	47604	3.13%	0.576%
17	12.986	1950	1955	1960	rBV3	16021	20128	1.32%	0.244%
18	13.045	1960	1965	1972	rBV	14631	25141	1.65%	0.304%
19	13.351	2007	2017	2020	rBV3	7443	16779	1.10%	0.203%
20	13.757	2081	2086	2095	rBV3	17778	37287	2.45%	0.452%
21	14.486	2206	2210	2212	rBV2	13758	16228	1.07%	0.197%
22	14.521	2212	2216	2221	rVV2	439883	618336	40.63%	7.488%
23	14.563	2221	2223	2232	rVB	104511	161107	10.58%	1.951%
24	14.668	2237	2241	2251	rVB	32893	58583	3.85%	0.709%
25	15.215	2330	2334	2342	rBV2	51810	75134	4.94%	0.910%
26	15.345	2349	2356	2360	rBV3	15970	29381	1.93%	0.356%
27	15.392	2360	2364	2374	rVB3	15046	21784	1.43%	0.264%
28	15.492	2379	2381	2386	rVV3	12502	18115	1.19%	0.219%
29	15.786	2427	2431	2438	rBV4	12908	28321	1.86%	0.343%
30	16.162	2488	2495	2497	rBV5	11242	17236	1.13%	0.209%
31	16.304	2517	2519	2522	rBV3	19048	18884	1.24%	0.229%
32	16.357	2522	2528	2539	rVB	148374	237149	15.58%	2.872%
33	16.662	2576	2580	2589	rBV	150053	207686	13.65%	2.515%
34	16.845	2608	2611	2614	rBV	22280	26317	1.73%	0.319%

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF062217\
 Data File : BF096123.D
 Acq On : 22 Jun 2017 15:44
 Operator : SJ/MA
 Sample : I3697-01RE 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-SF-02-001-ARE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	16.909	2618	2622	2629	rVV	185553	217608	14.30%	2.635%
36	17.004	2632	2638	2644	rBV8	13138	30806	2.02%	0.373%
37	17.109	2652	2656	2659	rBV6	9191	15689	1.03%	0.190%
38	17.145	2659	2662	2666	rVB3	17035	23149	1.52%	0.280%
39	17.233	2673	2677	2681	rVB3	15030	22218	1.46%	0.269%
40	17.280	2681	2685	2689	rBV5	21132	37496	2.46%	0.454%
41	17.321	2689	2692	2695	rVB	24217	28060	1.84%	0.340%
42	17.468	2714	2717	2721	rBV6	12414	18351	1.21%	0.222%
43	17.762	2764	2767	2772	rBV2	26528	30930	2.03%	0.375%
44	18.186	2835	2839	2843	rVB2	33514	46874	3.08%	0.568%
45	18.262	2847	2852	2857	rBV2	445631	612755	40.26%	7.420%
46	18.592	2905	2908	2911	rVB2	26830	29036	1.91%	0.352%
47	18.974	2970	2973	2977	rVB2	35302	42873	2.82%	0.519%
48	19.345	3033	3036	3040	rBV2	35961	40998	2.69%	0.496%
49	19.545	3067	3070	3073	rBV	63733	88978	5.85%	1.077%
50	19.892	3127	3129	3134	rBV	55494	73561	4.83%	0.891%
51	19.939	3134	3137	3145	rVV	348409	450709	29.61%	5.458%


Sum of corrected areas: 8258159

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF062217\
Data File : BF096123.D
Acq On : 22 Jun 2017 15:44
Operator : SJ/MA
Sample : I3697-01RE 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-SF-02-001-ARE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

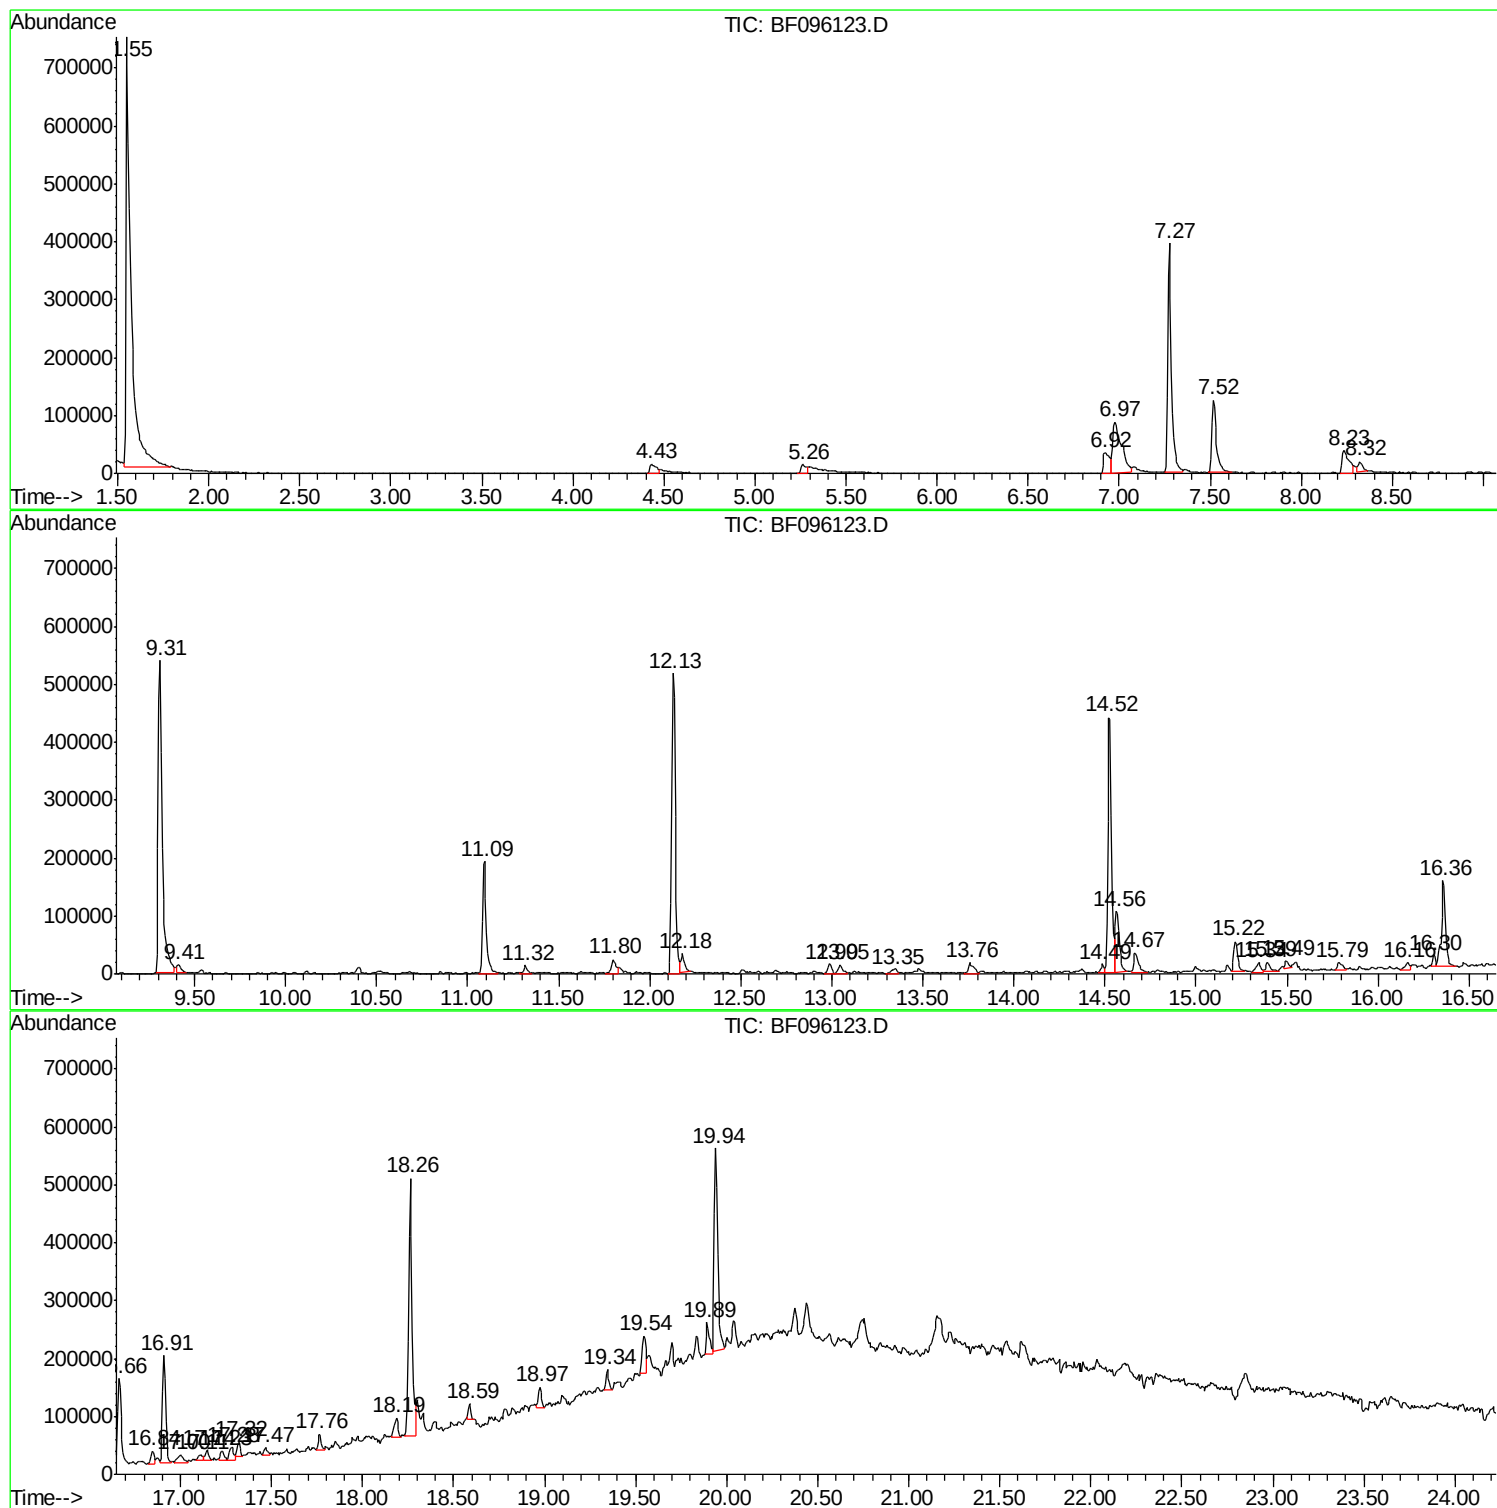

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF062217\
Data_File : BF096123.D
Acq_On : 22_Jun_2017. 15:444
Operator : SJ/MAA
Sample : I3697-01RE_5XX
Misc :
ALS_Vial : 9 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
FK-SF-02-001-ARE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
