


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF062217\
 Data File : BF096115.D
 Acq On : 22 Jun 2017 10:52
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 20 16:05:47 2017

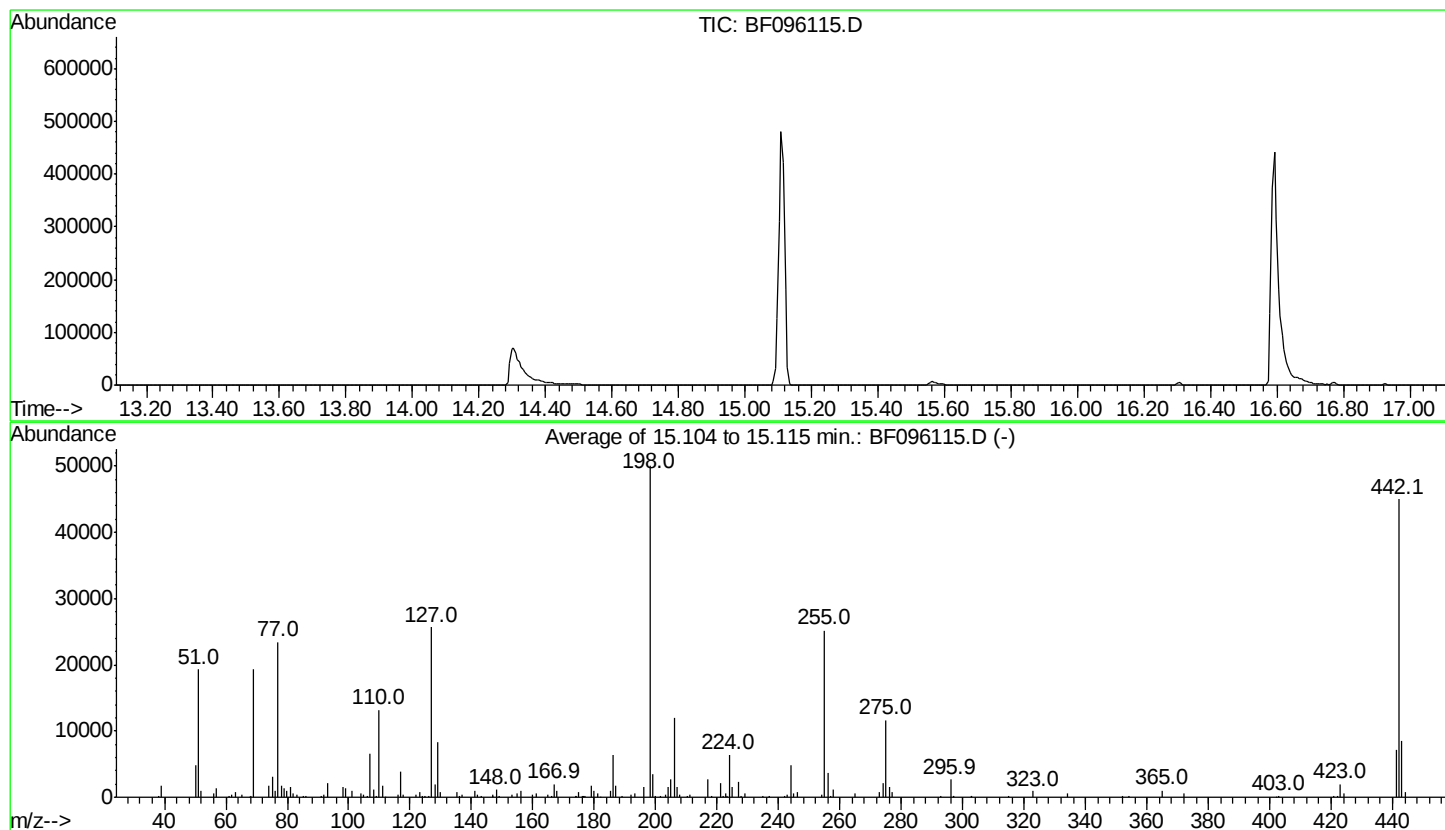

AutoFind: Scans 2315, 2316, 2317; Background Corrected with Scan 2308

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	19272	PASS
68	69	0.00	2	1.0	202	PASS
69	198	0.00	100	38.6	19309	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	25672	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50045	PASS
199	198	5	9	7.0	3511	PASS
275	198	10	60	23.4	11693	PASS
365	198	1	100	2.1	1068	PASS
441	442	0.01	24	15.9	7133	PASS
442	198	50	100	89.8	44960	PASS
443	442	15	24	18.7	8426	PASS