
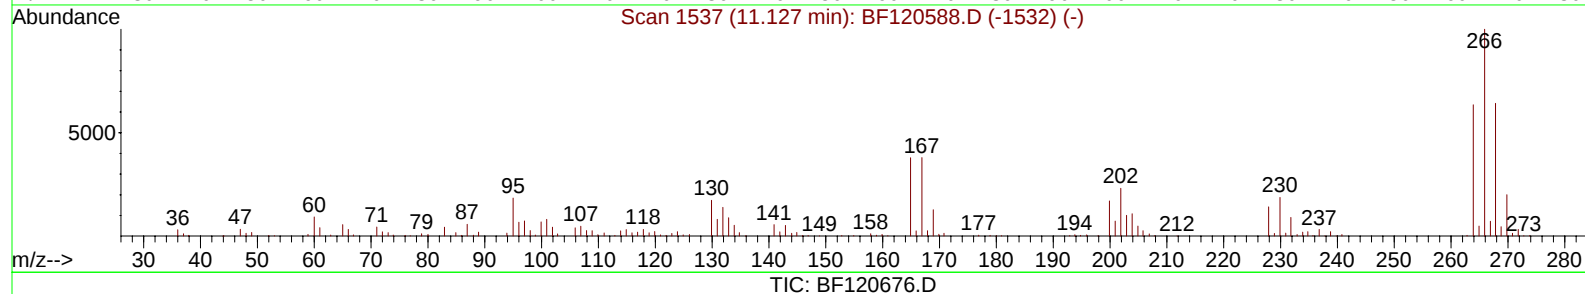
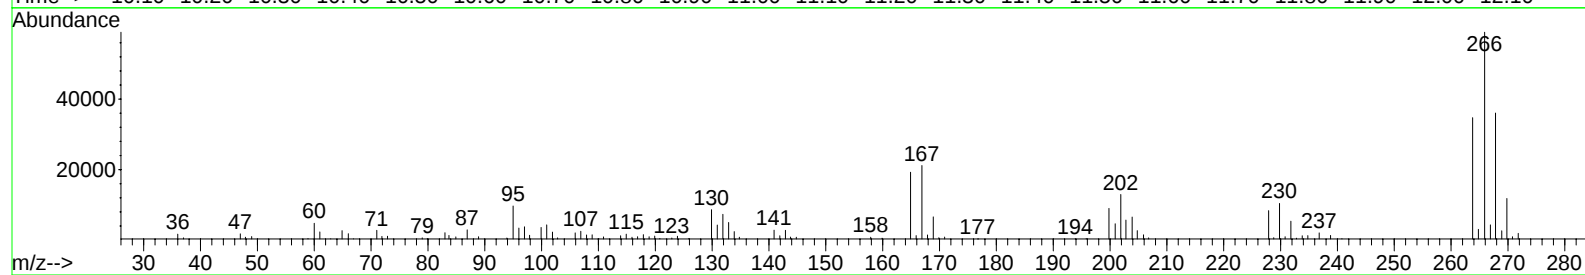


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062220\
 Data File : BF120676.D
 Acq On : 22 Jun 2020 14:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 18:32:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 11:28:22 2020
 Response via : Initial Calibration

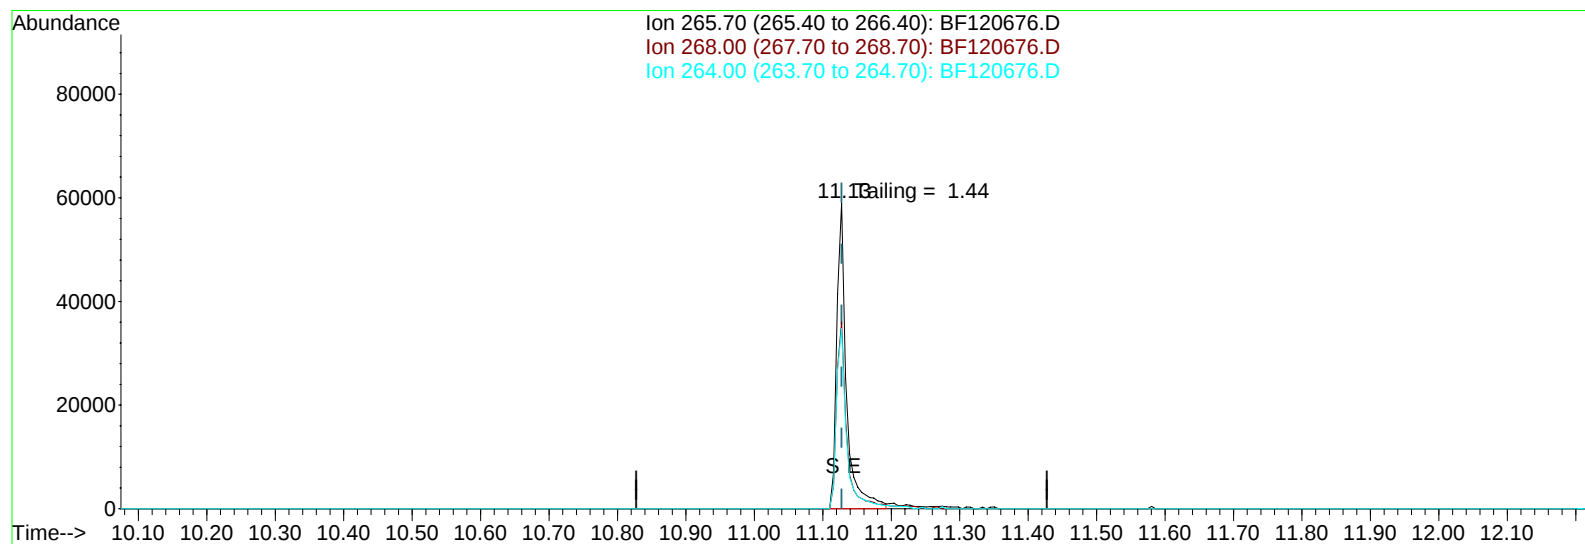

(70) Pentachlorophenol (C)




11.127min (+0.000) 27132.86ng

response 60190

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	61.10
264.00	63.50	58.85
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062220\
 Data File : BF120676.D
 Acq On : 22 Jun 2020 14:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 18:32:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 11 11:28:22 2020
 Response via : Initial Calibration

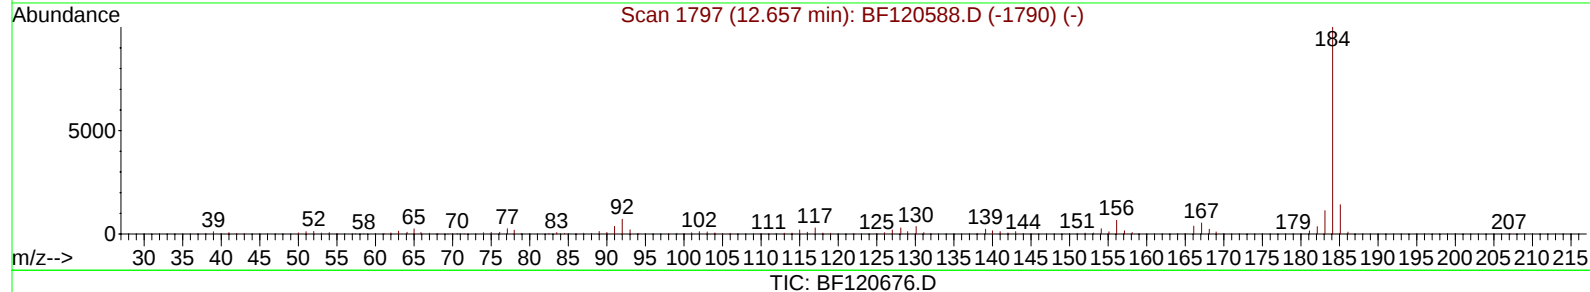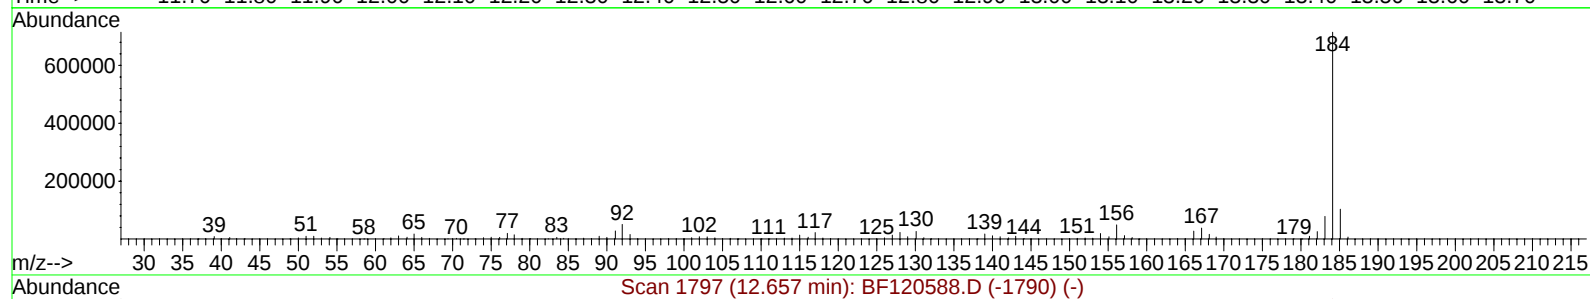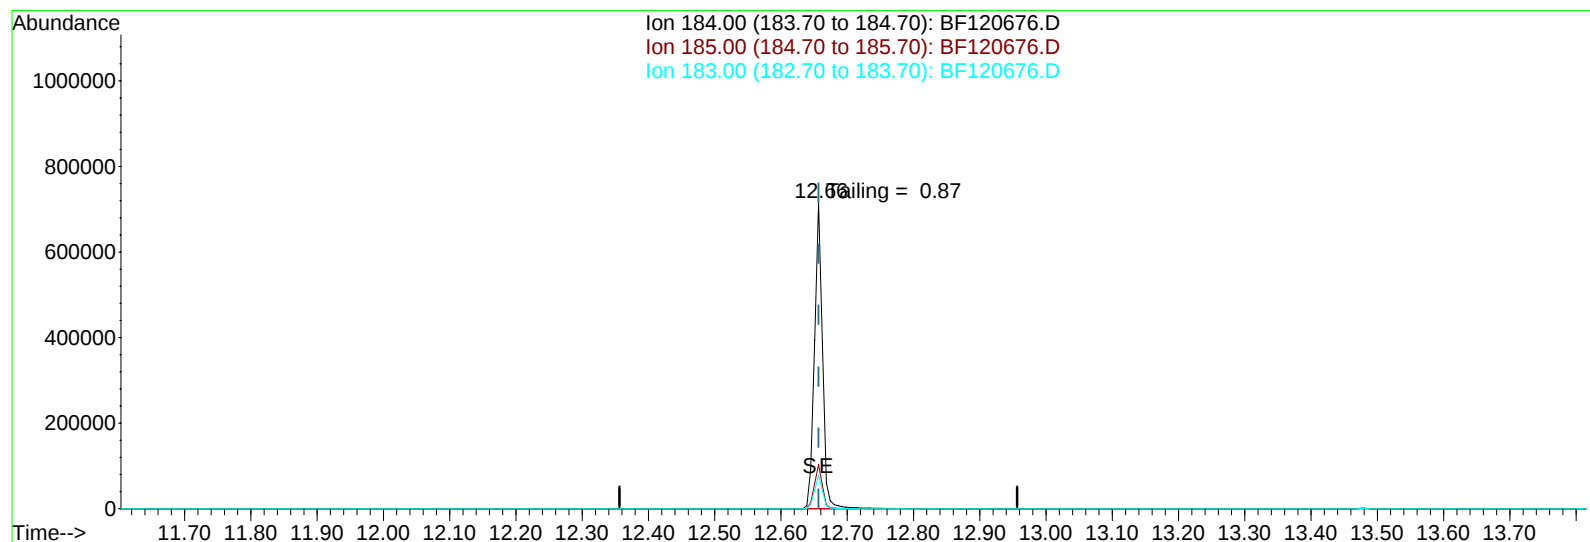

(77) Benzidine

12.657min (+0.000) 0.00ng

response 608223

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.45
183.00	11.30	10.96
0.00	0.00	0.00