

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062220\
 Data File : BF120685.D
 Acq On : 22 Jun 2020 19:35
 Operator : JU/CG
 Sample : L3082-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-10

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	560	564	583	rBV	2268595	2191378	59.83%	9.291%
2	6.434	734	739	742	rBV	1935943	2010717	54.90%	8.525%
3	6.798	797	801	804	rBV	806613	719835	19.65%	3.052%
4	6.951	823	827	830	rBV	2275183	1941972	53.02%	8.233%
5	7.357	891	896	899	rBV	1689846	1592309	43.48%	6.751%
6	8.081	1015	1019	1037	rBV	874028	792508	21.64%	3.360%
7	9.157	1197	1202	1205	rBV	3352827	3016707	82.37%	12.790%
8	9.551	1265	1269	1276	rBV	141137	134120	3.66%	0.569%
9	9.833	1313	1317	1332	rVB	1208205	1008409	27.53%	4.275%
10	10.622	1447	1451	1466	rBV	2027785	1923331	52.51%	8.154%
11	11.316	1566	1569	1572	rBV	1166020	1095987	29.92%	4.647%
12	11.339	1572	1573	1577	rVB	71822	48242	1.32%	0.205%
13	12.533	1772	1776	1780	rVB	75299	66757	1.82%	0.283%
14	12.757	1807	1814	1817	rBV	72827	78971	2.16%	0.335%
15	12.910	1835	1840	1843	rBV	3958941	3662497	100.00%	15.528%
16	13.810	1989	1993	2010	rBV2	164108	297413	8.12%	1.261%
17	13.957	2011	2018	2022	rBV	1232054	1270685	34.69%	5.387%
18	14.986	2189	2193	2203	rVB	35309	65196	1.78%	0.276%
19	15.339	2249	2253	2257	rVV	33633	44022	1.20%	0.187%
20	15.404	2259	2264	2267	rVV	997202	1253821	34.23%	5.316%
21	15.427	2267	2268	2272	rVB	69475	54916	1.50%	0.233%
22	15.851	2336	2340	2347	rBV2	54788	114135	3.12%	0.484%
23	15.933	2348	2354	2364	rVB2	27360	97918	2.67%	0.415%
24	16.339	2418	2423	2430	rBV2	26365	52458	1.43%	0.222%
25	17.603	2631	2638	2642	rBV7	21693	52563	1.44%	0.223%


Sum of corrected areas: 23586867

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062220\
Data File : BF120685.D
Acq On : 22 Jun 2020 19:35
Operator : JU/CG
Sample : L3082-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

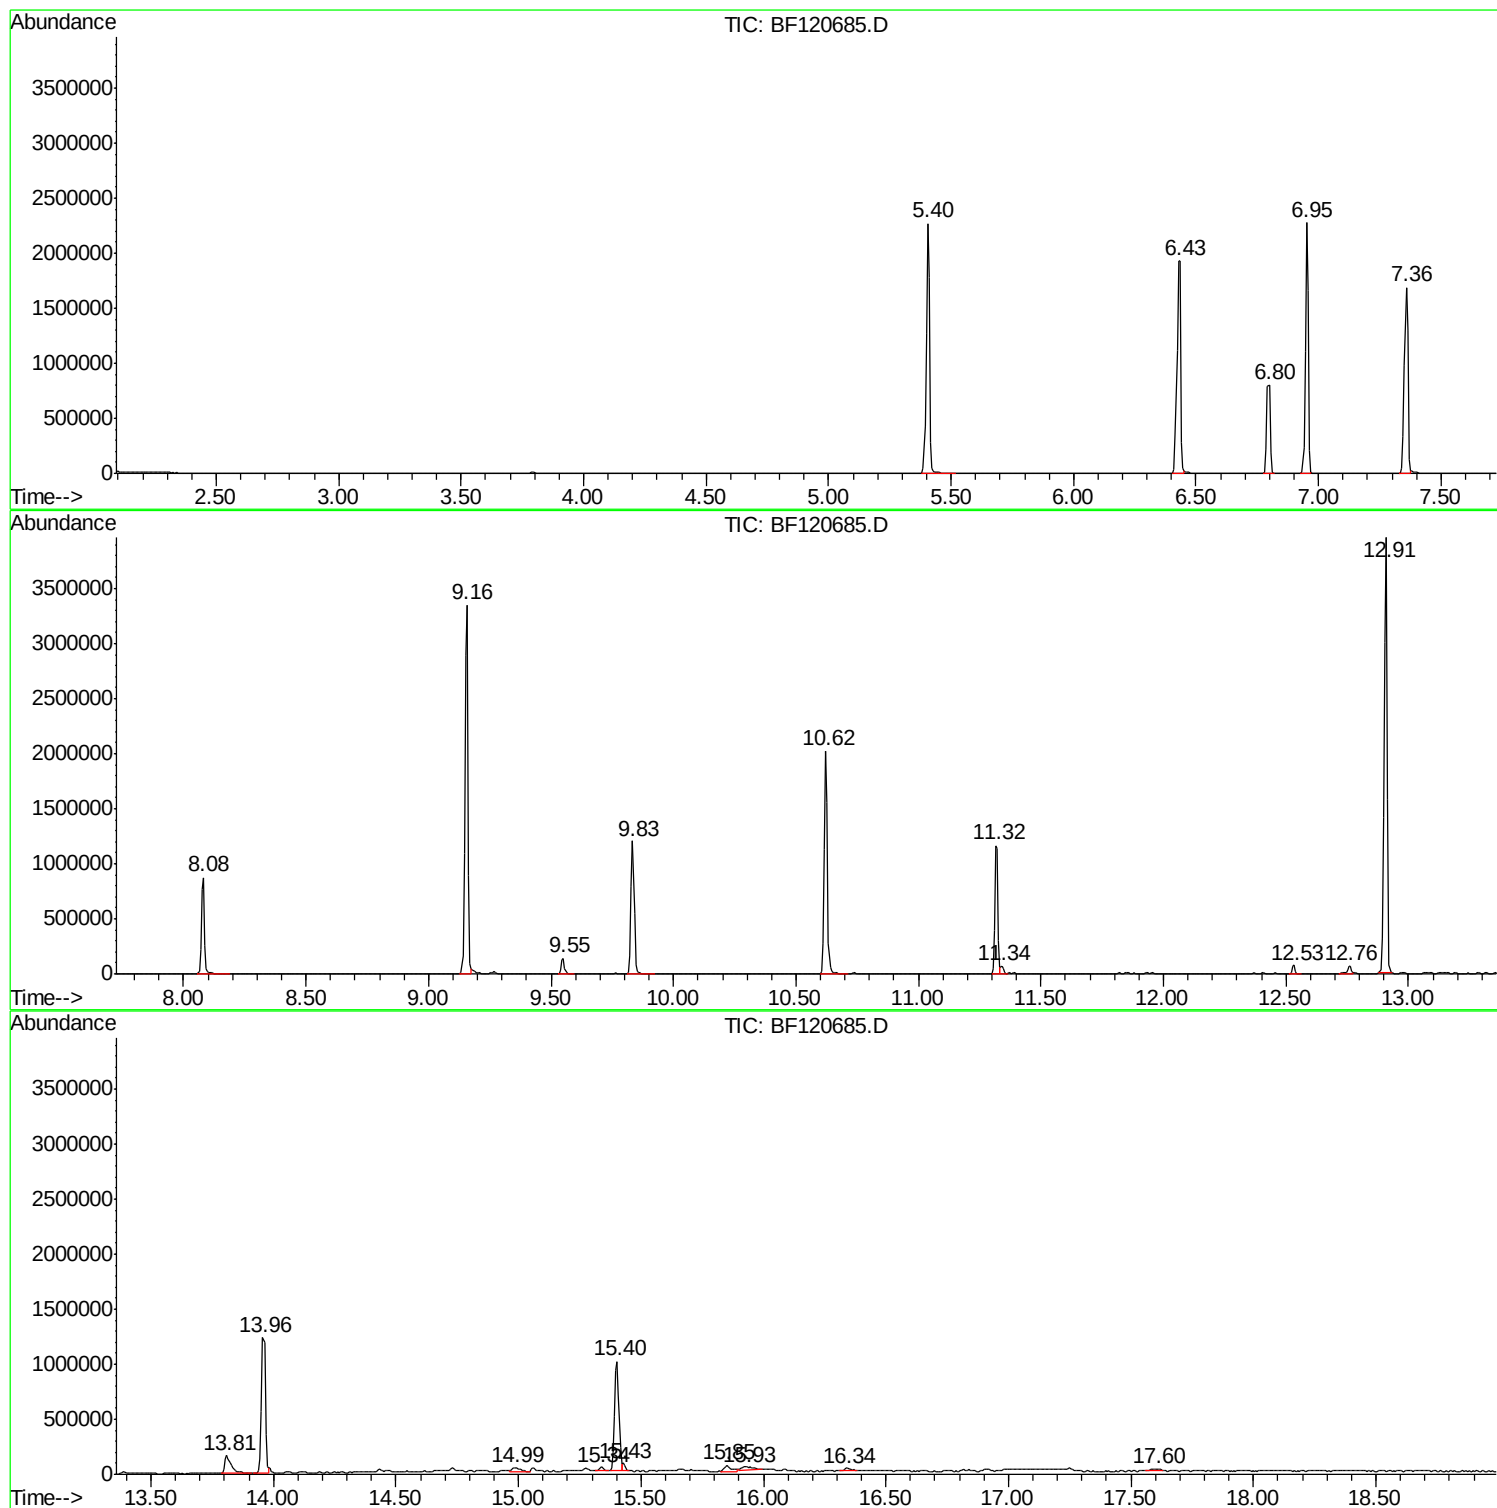

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062220\
Data File : BF120685.D
Acq On : 22 Jun 2020 19:35
Operator : JU/CG
Sample : L3082-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Dichloroacetic acid, heptad... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.81	4.68 ng	297413	Chrysene-d12	13.96

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	95
2		Carbonic acid, octadecyl 2,2,2-t...	444	C21H39Cl3O3	1000314-56-3	94
3		n-Tetracosanol-1	354	C24H50O	000506-51-4	94
4		Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
5		Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	93

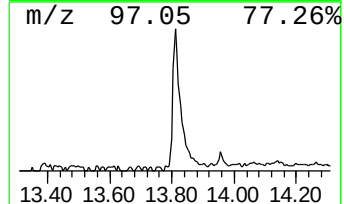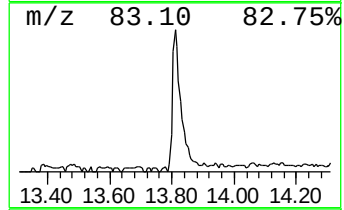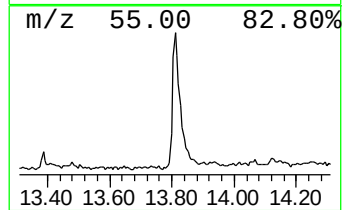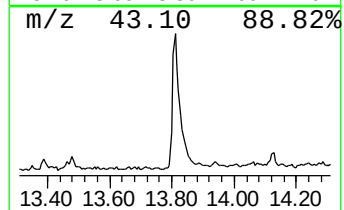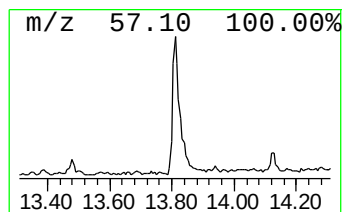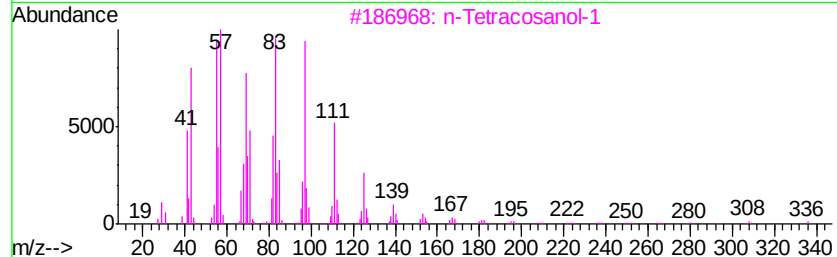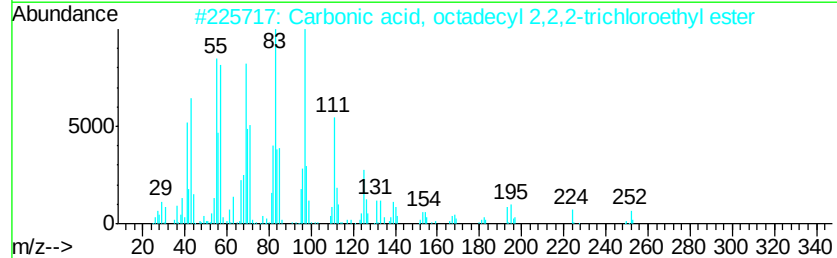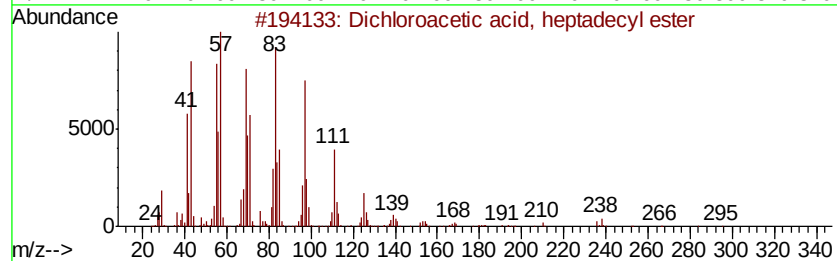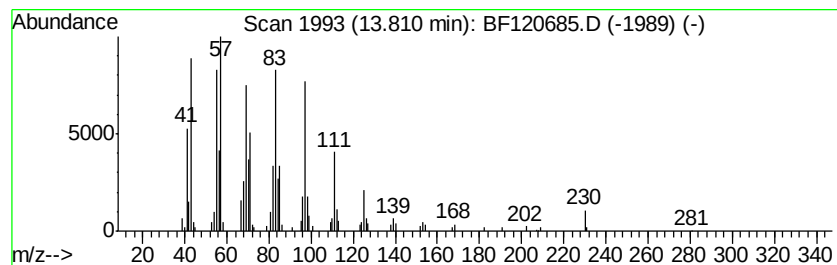

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062220\
Data File : BF120685.D
Acq On : 22 Jun 2020 19:35
Operator : JU/CG
Sample : L3082-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ac...	13.81	4.7	ng	297413	5	13.96	1270690	20.0