


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062220\
 Data File : BF120676.D
 Acq On : 22 Jun 2020 14:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 11 11:28:22 2020

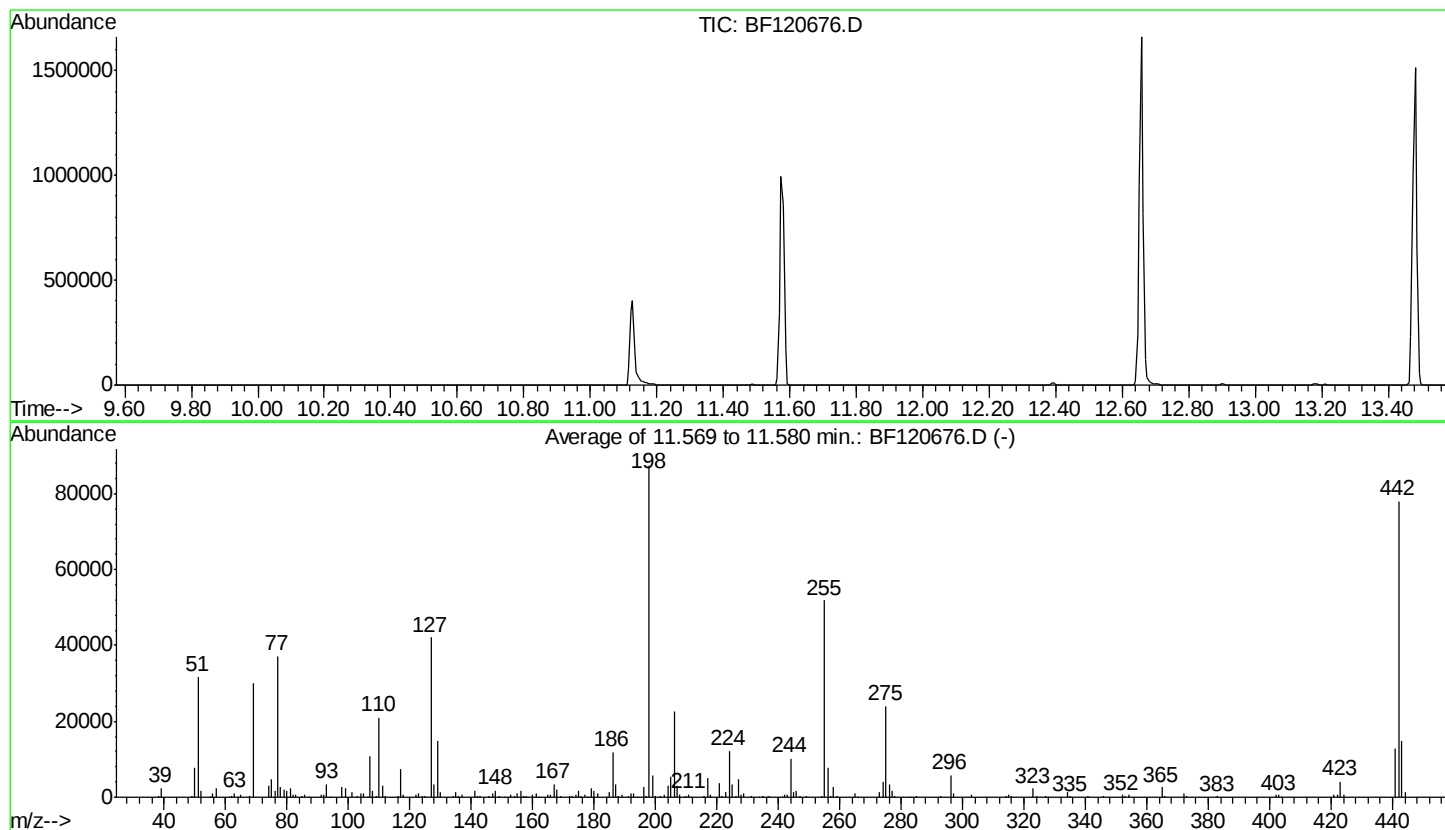

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	31725	PASS
68	69	0.00	2	1.5	448	PASS
69	198	0.00	100	34.5	30186	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	42109	PASS
197	198	0.00	2	0.6	495	PASS
198	198	100	100	100.0	87402	PASS
199	198	5	9	6.6	5727	PASS
275	198	10	60	27.6	24103	PASS
365	198	1	100	3.1	2666	PASS
441	198	0.01	100	14.7	12858	PASS
442	198	50	100	89.3	78058	PASS
443	442	15	24	19.0	14839	PASS