
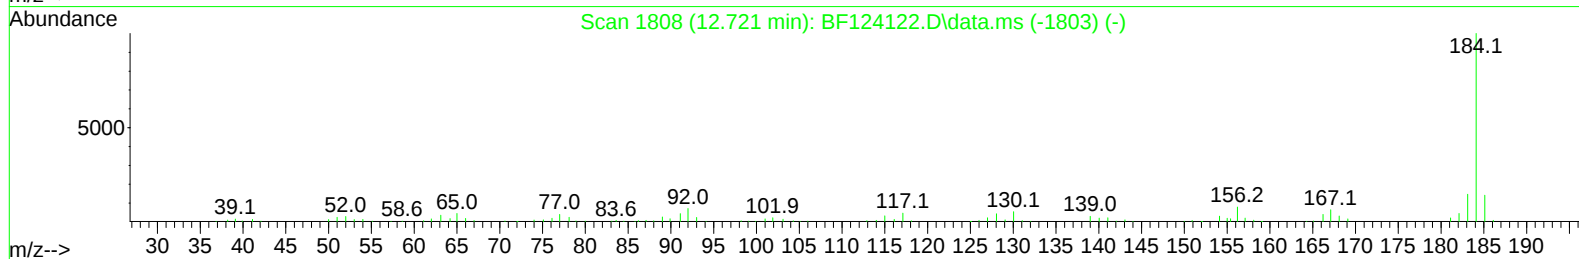
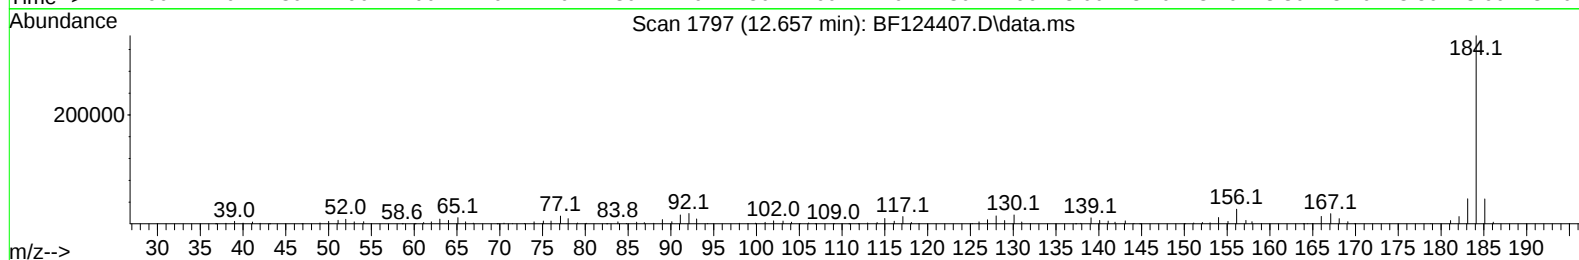


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062221\
 Data File : BF124407.D
 Acq On : 22 Jun 2021 12:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 13:39:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 15 20:09:26 2021
 Response via : Initial Calibration

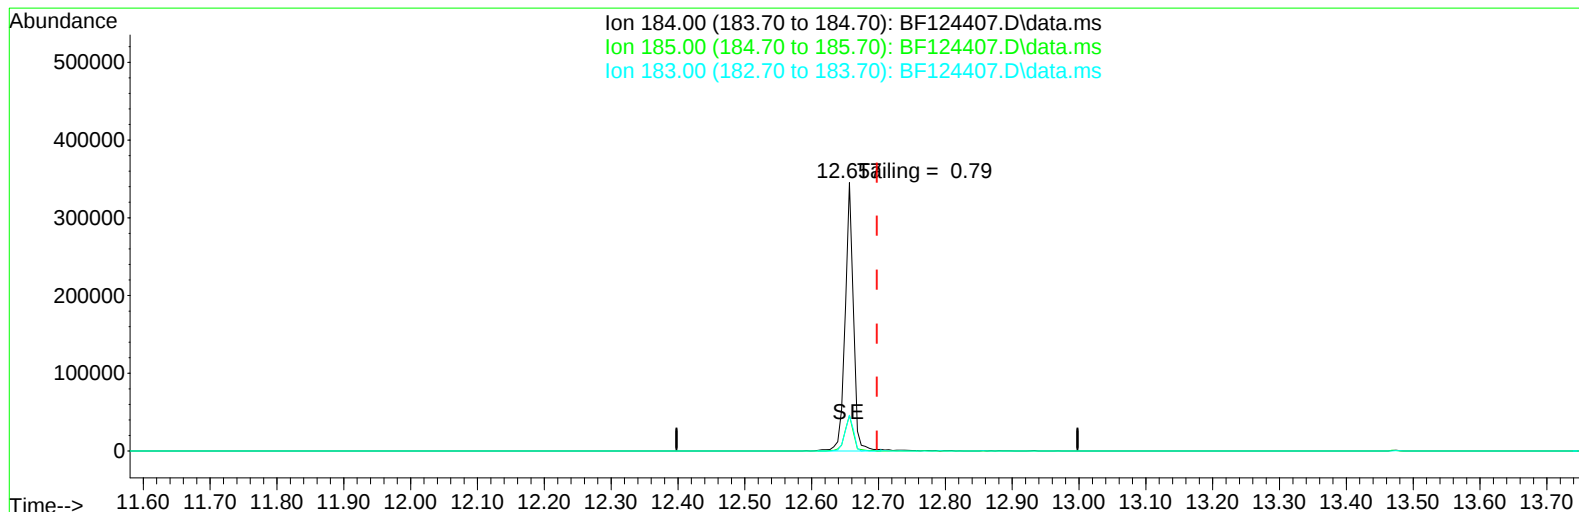

TIC: BF124407.D\data.ms

(77) Benzidine




12.657min (-0.041) 0.00 ng

response 298429

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.27
183.00	9.80	13.40#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062221\
Data File : BF124407.D
Acq On : 22 Jun 2021 12:17
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 13:39:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

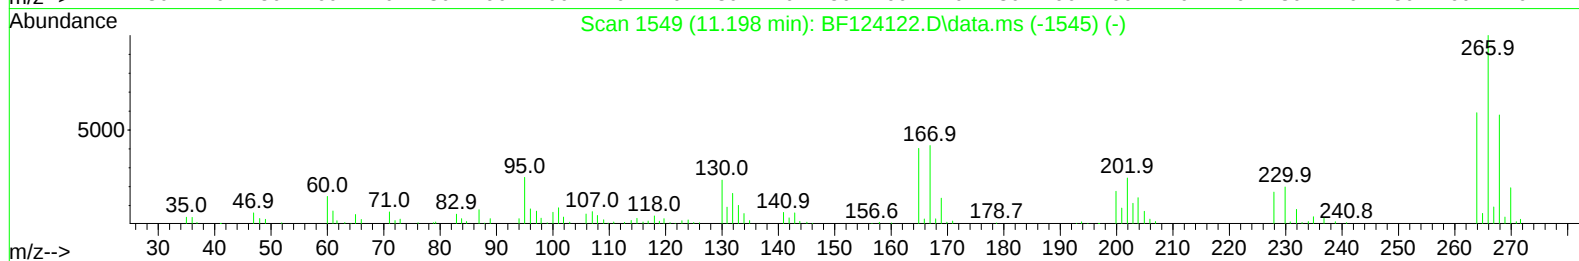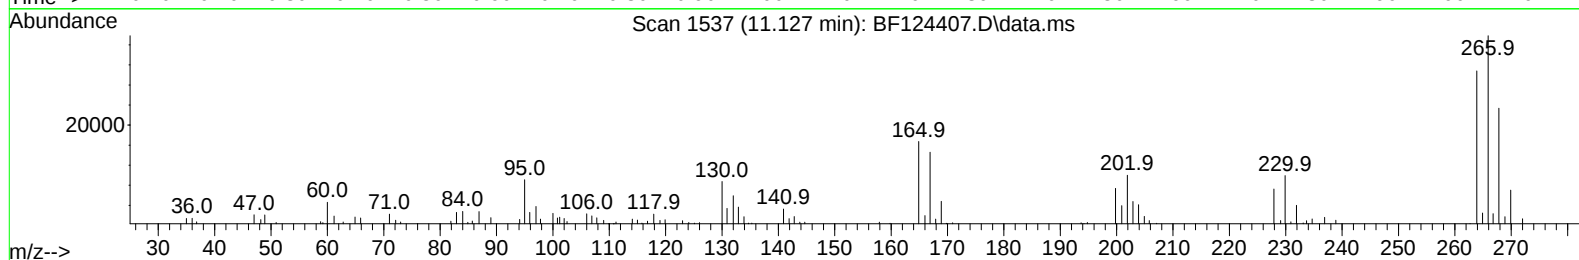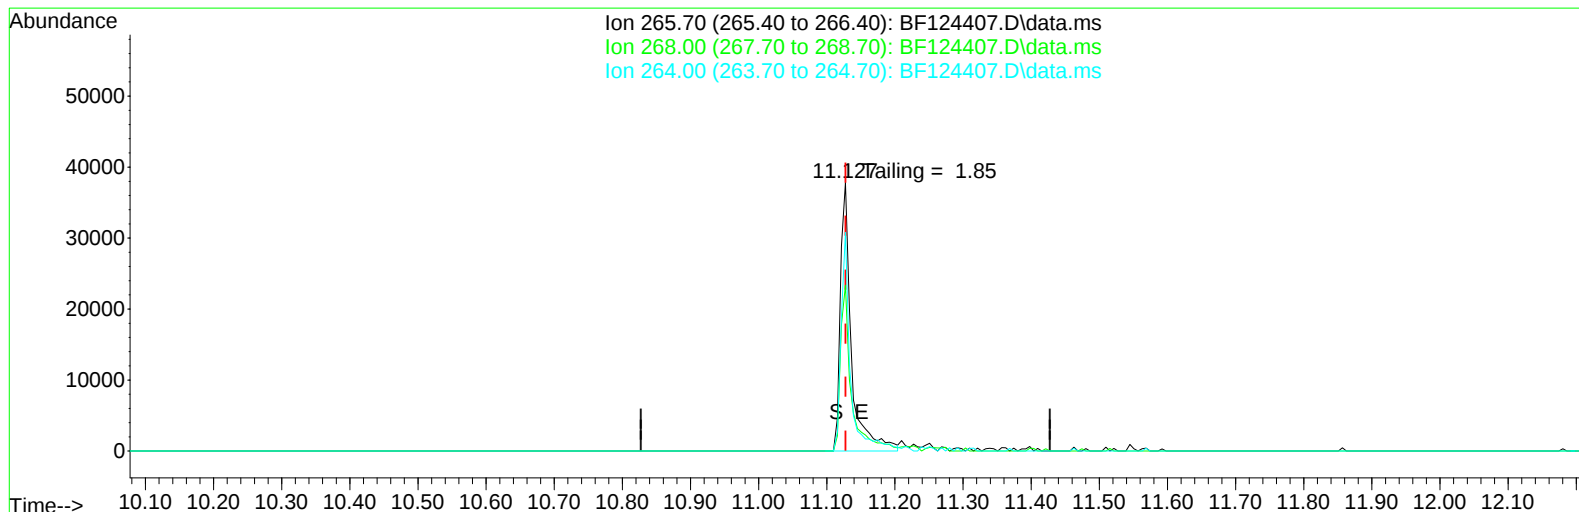

TIC: BF124407.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 23103.76 ng

response 43004

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	61.75
264.00	65.70	81.43#
0.00	0.00	0.00