

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062221\
 Data File : BF124412.D
 Acq On : 22 Jun 2021 15:10
 Operator : JU/CG
 Sample : M2773-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-9-AOC-2

Quant Time: Jun 22 15:47:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 15 20:09:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.781	152	42178	20.000	ng	0.00
21) Naphthalene-d8	8.063	136	168017	20.000	ng	#-0.01
39) Acenaphthene-d10	9.822	164	104619	20.000	ng	0.00
64) Phenanthrene-d10	11.310	188	191927	20.000	ng	0.00
76) Chrysene-d12	13.963	240	90959	20.000	ng	# 0.00
86) Perylene-d12	15.427	264	78134	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.410	112	223744	79.855	ng	0.00
7) Phenol-d6	6.428	99	282706	75.065	ng	-0.02
23) Nitrobenzene-d5	7.351	82	221585	52.306	ng	0.00
42) 2,4,6-Tribromophenol	10.616	330	107264	72.368	ng	0.00
45) 2-Fluorobiphenyl	9.145	172	460498	55.389	ng	0.00
79) Terphenyl-d14	12.898	244	440665	66.515	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062221\
Data File : BF124412.D
Acq On : 22 Jun 2021 15:10
Operator : JU/CG
Sample : M2773-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-9-AOC-2

Quant Time: Jun 22 15:47:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration




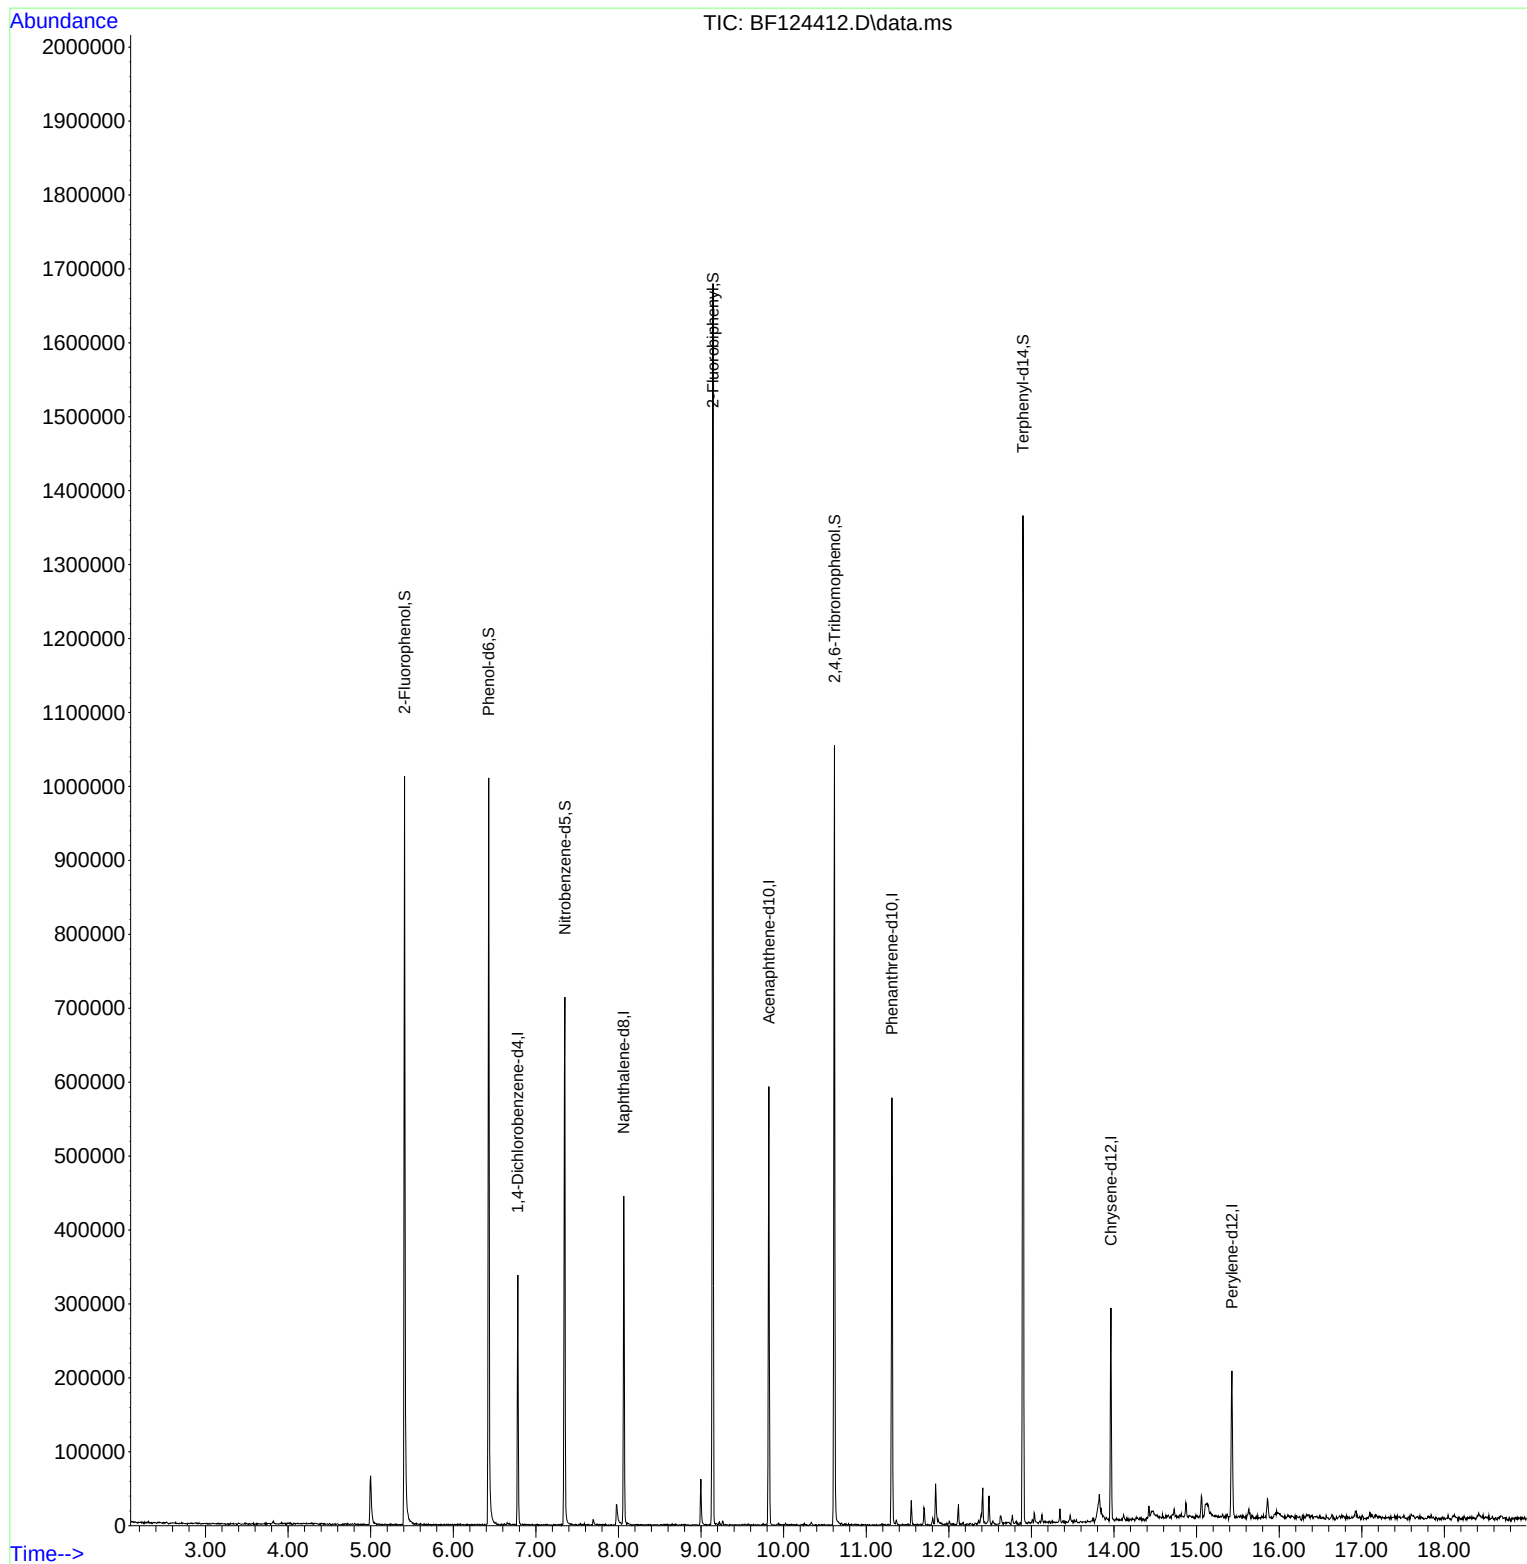


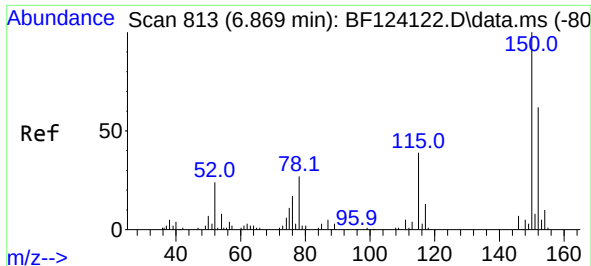

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.781 min Scan# 798
Delta R.T. -0.005 min
Lab File: BF124412.D
Acq: 22 Jun 2021 15:10




Instrument :
BNA_F
ClientSampleId :
SB-9-AOC-2


Tgt Ion:152 Resp: 42178
Ion Ratio Lower Upper
152 100
150 168.4 127.0 190.6
115 67.6 54.3 81.5

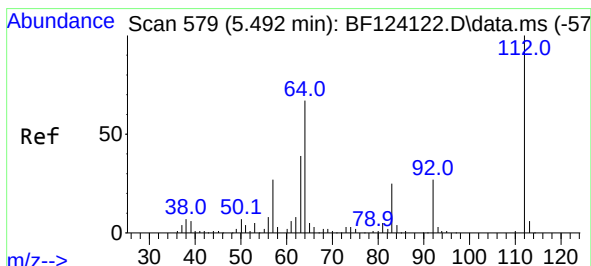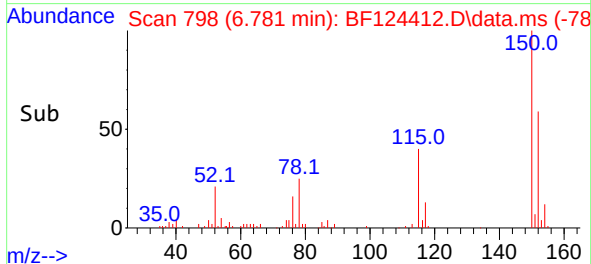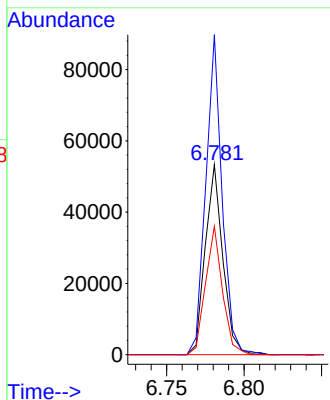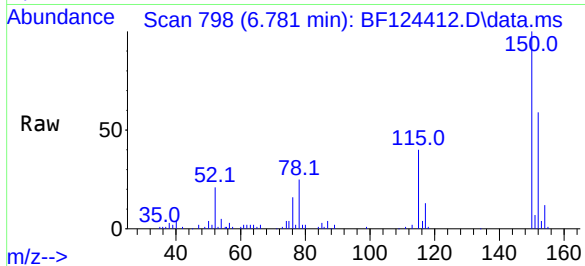

#5
2-Fluorophenol
Concen: 79.855 ng
RT: 5.410 min Scan# 565
Delta R.T. -0.006 min
Lab File: BF124412.D
Acq: 22 Jun 2021 15:10

Tgt Ion:112 Resp: 223744
Ion Ratio Lower Upper
112 100
64 69.5 61.4 92.0
63 39.4 33.0 49.4


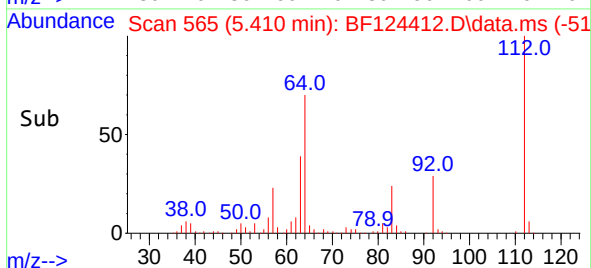
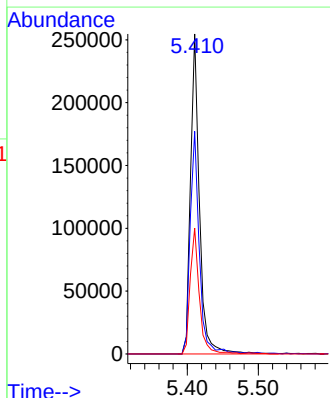
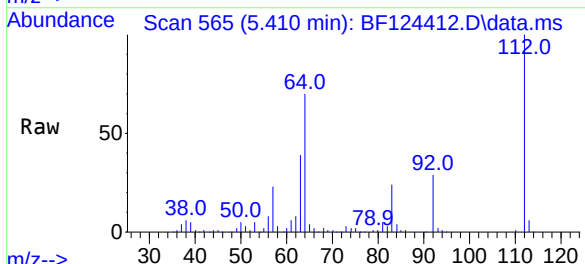


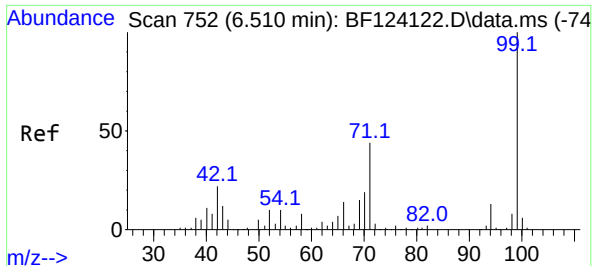

#7
Phenol-d6
Concen: 75.065 ng
RT: 6.428 min Scan# 738
Delta R.T. -0.017 min
Lab File: BF124412.D
Acq: 22 Jun 2021 15:10




Instrument :
BNA_F
ClientSampleId :
SB-9-AOC-2


Tgt Ion: 99 Resp: 282706
Ion Ratio Lower Upper
99 100
42 19.4 19.8 29.8#
71 45.0 31.1 46.7

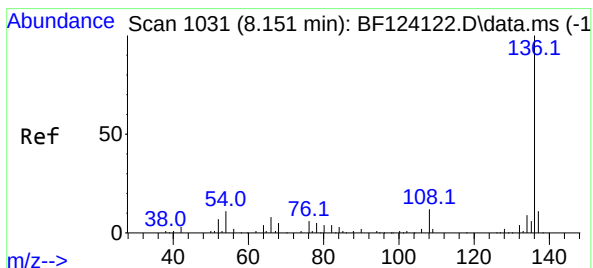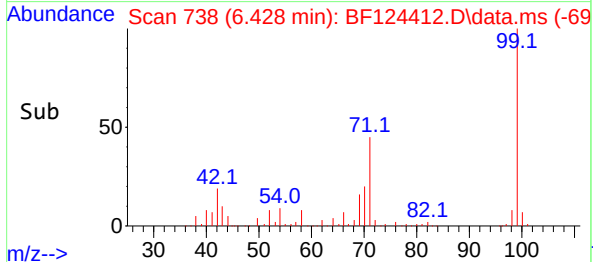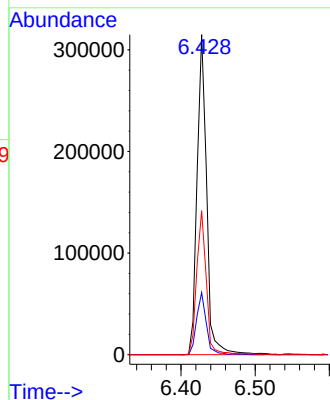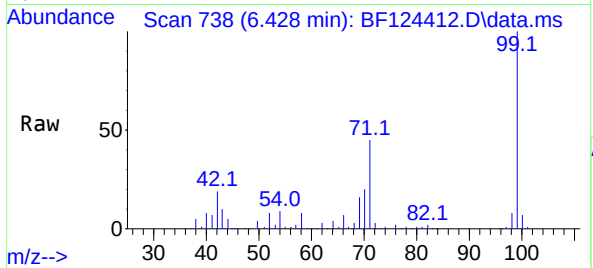

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.063 min Scan# 1016
Delta R.T. -0.012 min
Lab File: BF124412.D
Acq: 22 Jun 2021 15:10

Tgt Ion: 136 Resp: 168017
Ion Ratio Lower Upper
136 100
137 10.5 8.7 13.1
54 8.9 9.8 14.6#
68 5.2 4.1 6.1

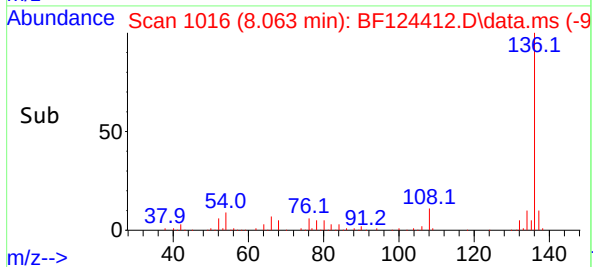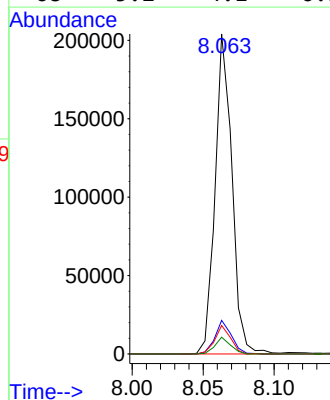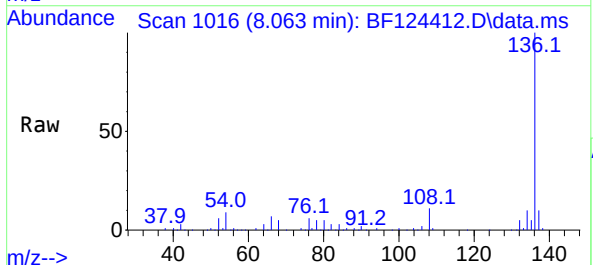

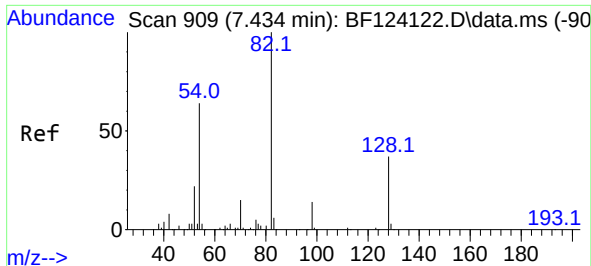

#23

Nitrobenzene-d5

Concen: 52.306 ng

RT: 7.351 min Scan# 895

Delta R.T. -0.006 min

Lab File: BF124412.D

Acq: 22 Jun 2021 15:10

Instrument :

BNA_F

ClientSampleId :

SB-9-AOC-2





Tgt Ion: 82 Resp: 221585

Ion Ratio Lower Upper

82 100

128 38.7 29.4 44.2

54 52.8 54.1 81.1#

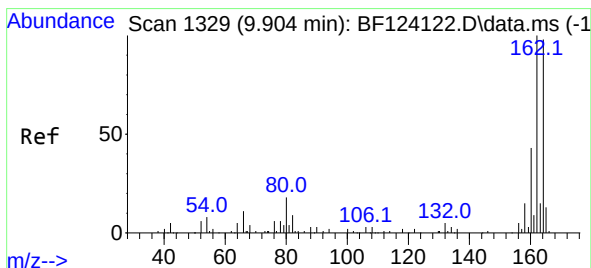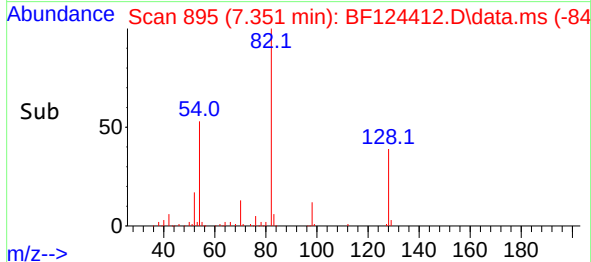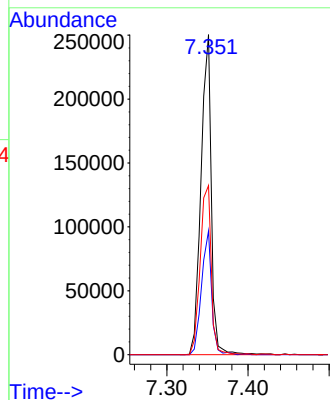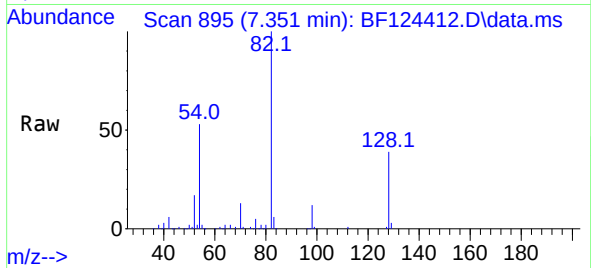

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.822 min Scan# 1315

Delta R.T. -0.006 min

Lab File: BF124412.D

Acq: 22 Jun 2021 15:10




Tgt Ion:164 Resp: 104619


Ion Ratio Lower Upper

164 100

162 107.8 80.7 121.1

160 43.9 37.3 55.9


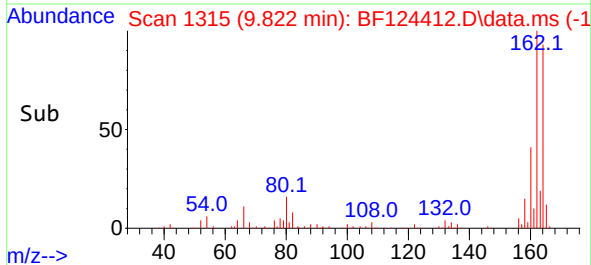
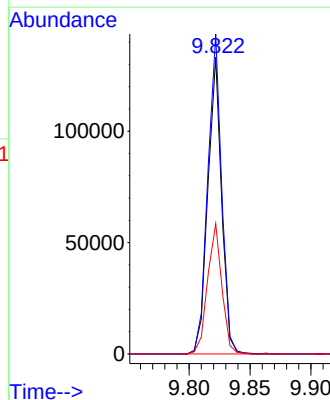
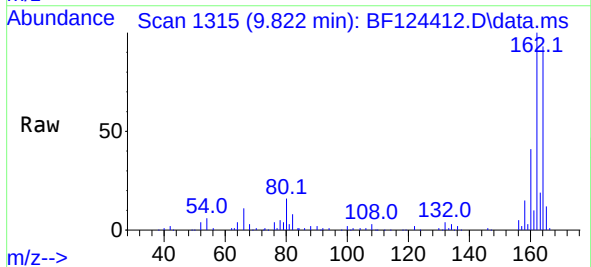


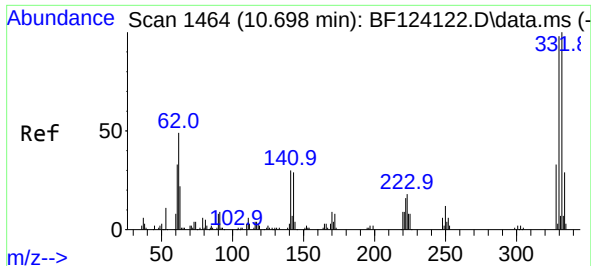

#42
2,4,6-Tribromophenol
Concen: 72.368 ng
RT: 10.616 min Scan# 1450
Delta R.T. -0.006 min
Lab File: BF124412.D
Acq: 22 Jun 2021 15:10




Instrument :
BNA_F
ClientSampleID :
SB-9-AOC-2


Tgt Ion: 330 Resp: 107264
Ion Ratio Lower Upper
330 100
332 96.1 77.1 115.7
141 39.2 27.9 41.9

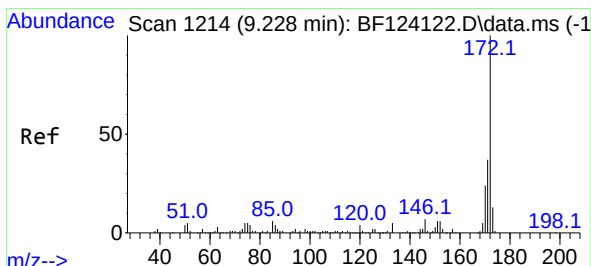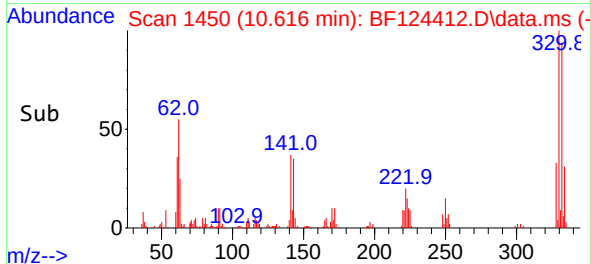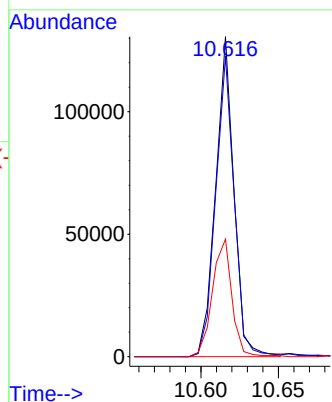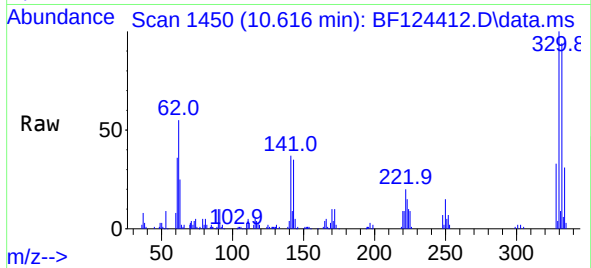

#45
2-Fluorobiphenyl
Concen: 55.389 ng
RT: 9.145 min Scan# 1200
Delta R.T. -0.006 min
Lab File: BF124412.D
Acq: 22 Jun 2021 15:10

Tgt Ion: 172 Resp: 460498
Ion Ratio Lower Upper
172 100
171 37.0 28.1 42.1
170 22.7 19.2 28.8


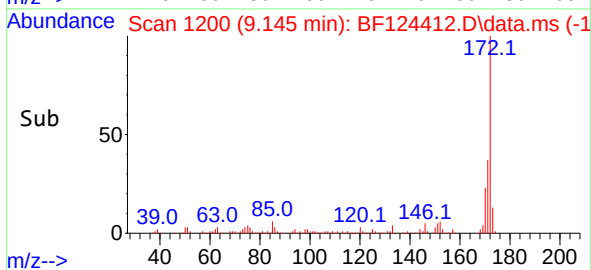
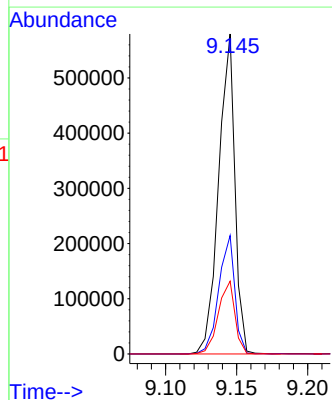
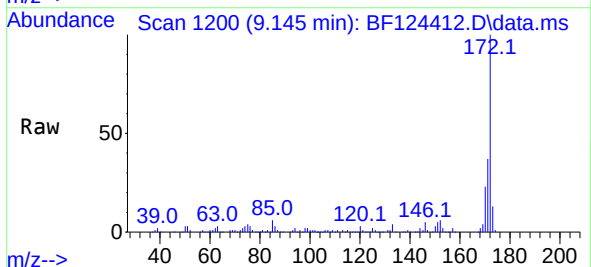


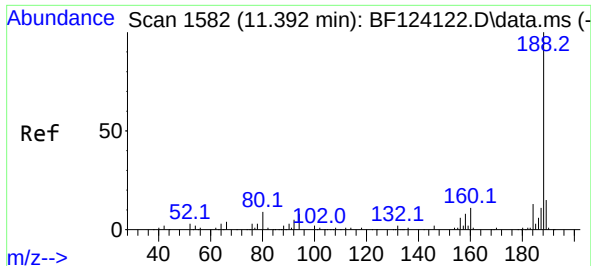

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.310 min Scan# 1568
Delta R.T. -0.006 min
Lab File: BF124412.D
Acq: 22 Jun 2021 15:10




Instrument :
BNA_F
ClientSampleId :
SB-9-AOC-2


Tgt Ion:188 Resp: 191927
Ion Ratio Lower Upper
188 100
94 8.0 6.9 10.3
80 10.7 8.2 12.2

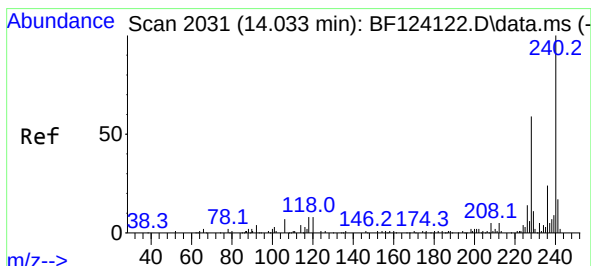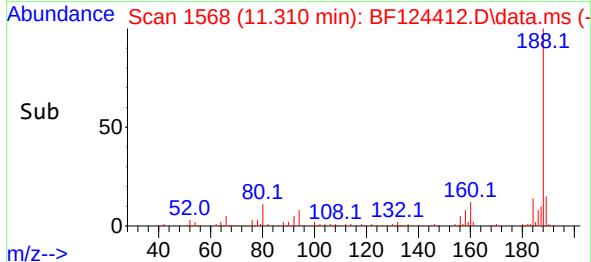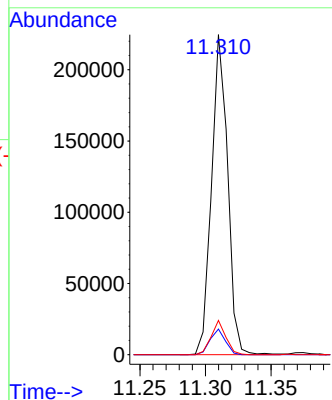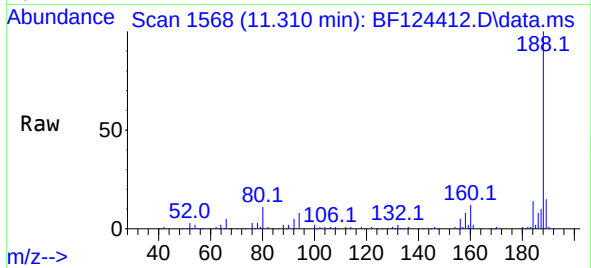

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.963 min Scan# 2019
Delta R.T. 0.000 min
Lab File: BF124412.D
Acq: 22 Jun 2021 15:10

Tgt Ion:240 Resp: 90959
Ion Ratio Lower Upper
240 100
120 6.7 7.2 10.8#
236 25.5 19.0 28.4


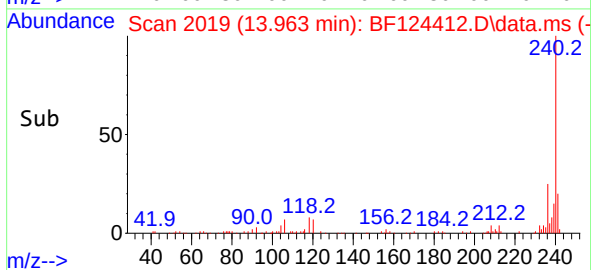
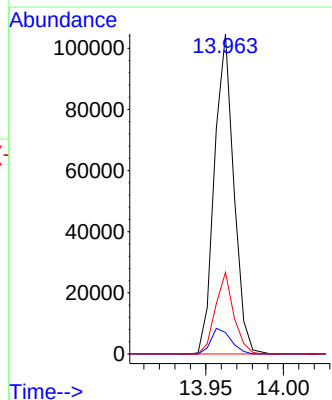
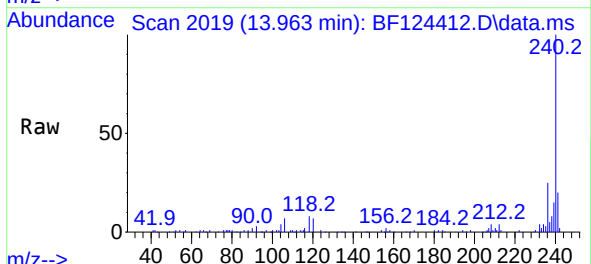


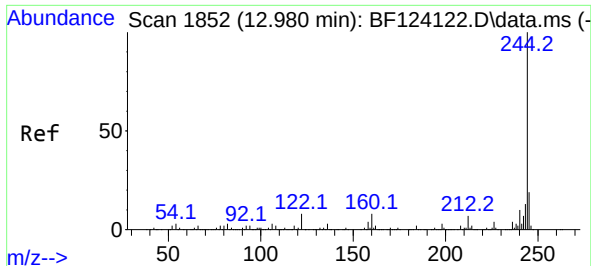

#79
Terphenyl-d14
Concen: 66.515 ng
RT: 12.898 min Scan# 1838
Delta R.T. -0.006 min
Lab File: BF124412.D
Acq: 22 Jun 2021 15:10

Instrument :
BNA_F
ClientSampleId :
SB-9-AOC-2

Tgt Ion:244 Resp: 440665
Ion Ratio Lower Upper
244 100
212 7.3 5.7 8.5
122 9.4 9.7 14.5#

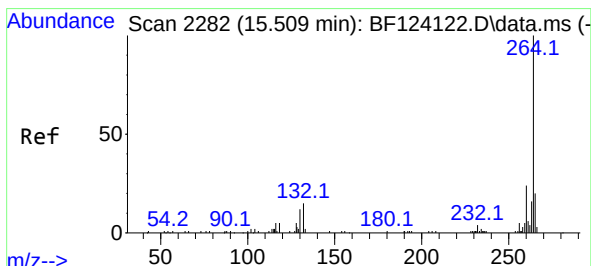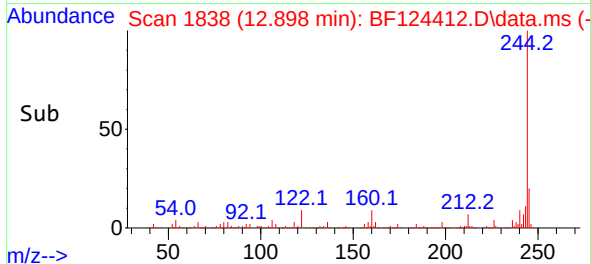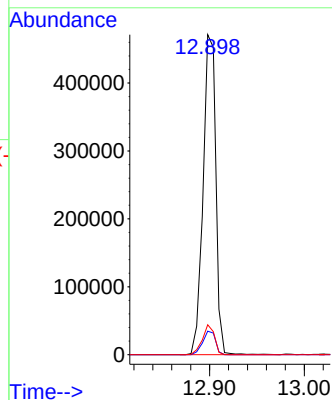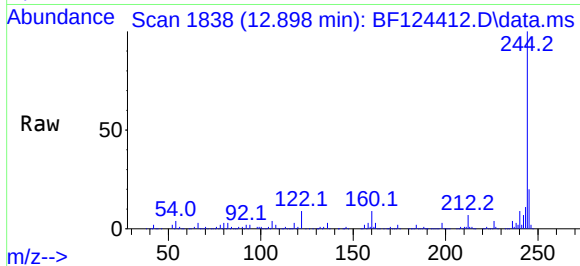

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.427 min Scan# 2268
Delta R.T. 0.012 min
Lab File: BF124412.D
Acq: 22 Jun 2021 15:10

Tgt Ion:264 Resp: 78134
Ion Ratio Lower Upper
264 100
260 24.4 18.7 28.1
265 19.8 17.8 26.8

