


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062221\
 Data File : BF124407.D
 Acq On : 22 Jun 2021 12:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 15 20:09:26 2021

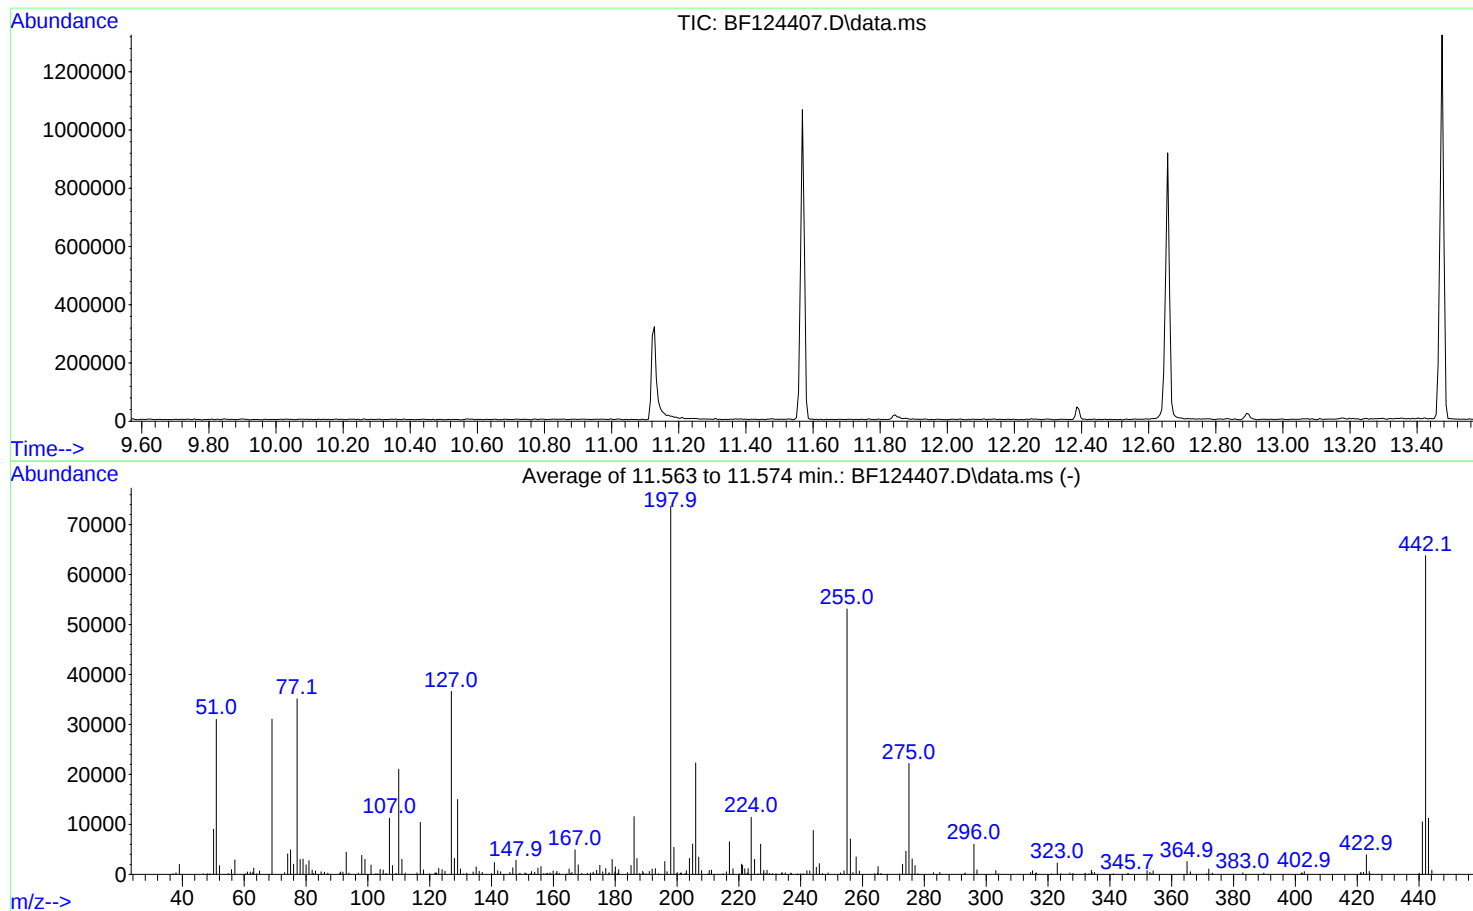




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	31035	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.2	31059	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	36624	PASS
197	198	0.00	2	0.8	559	PASS
198	198	100	100	100.0	73616	PASS
199	198	5	9	7.4	5417	PASS
275	198	10	60	30.2	22206	PASS
365	198	1	100	3.5	2576	PASS
441	198	0.01	100	14.2	10488	PASS
442	442	50	100	100.0	63797	PASS
443	442	15	24	17.6	11236	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062221\
 Data File : BF124407.D
 Acq On : 22 Jun 2021 12:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 22 13:39:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 15 20:09:26 2021
 Response via : Initial Calibration

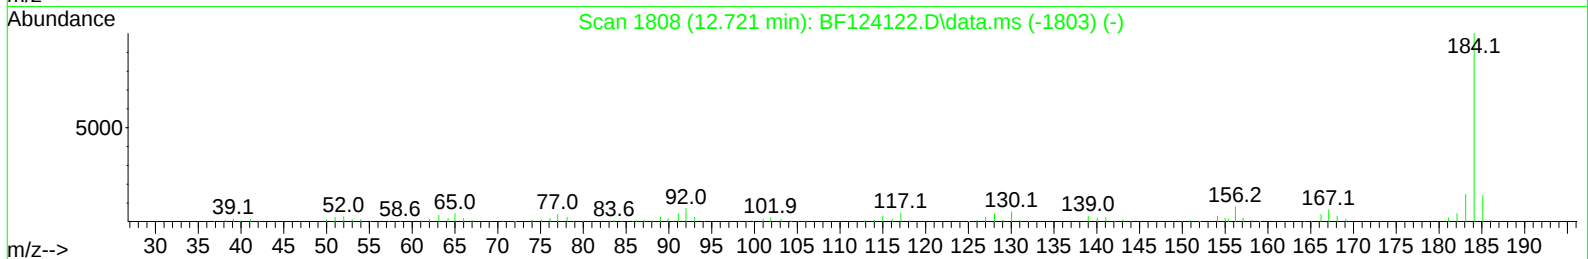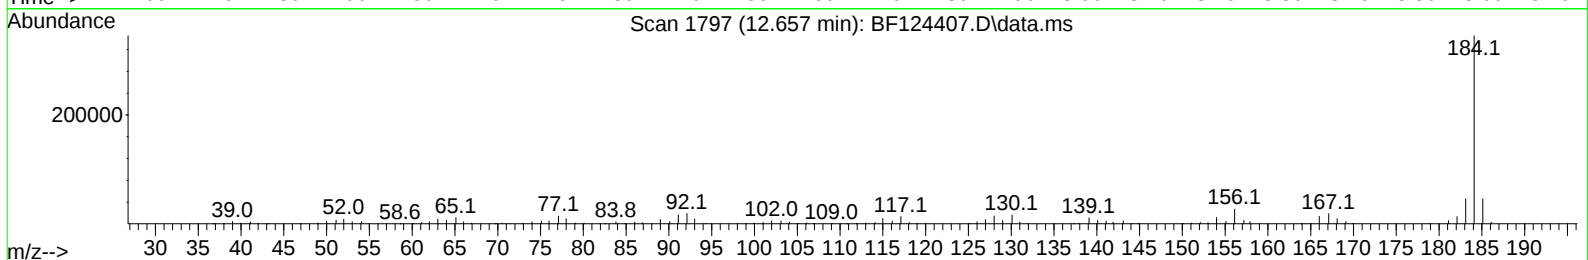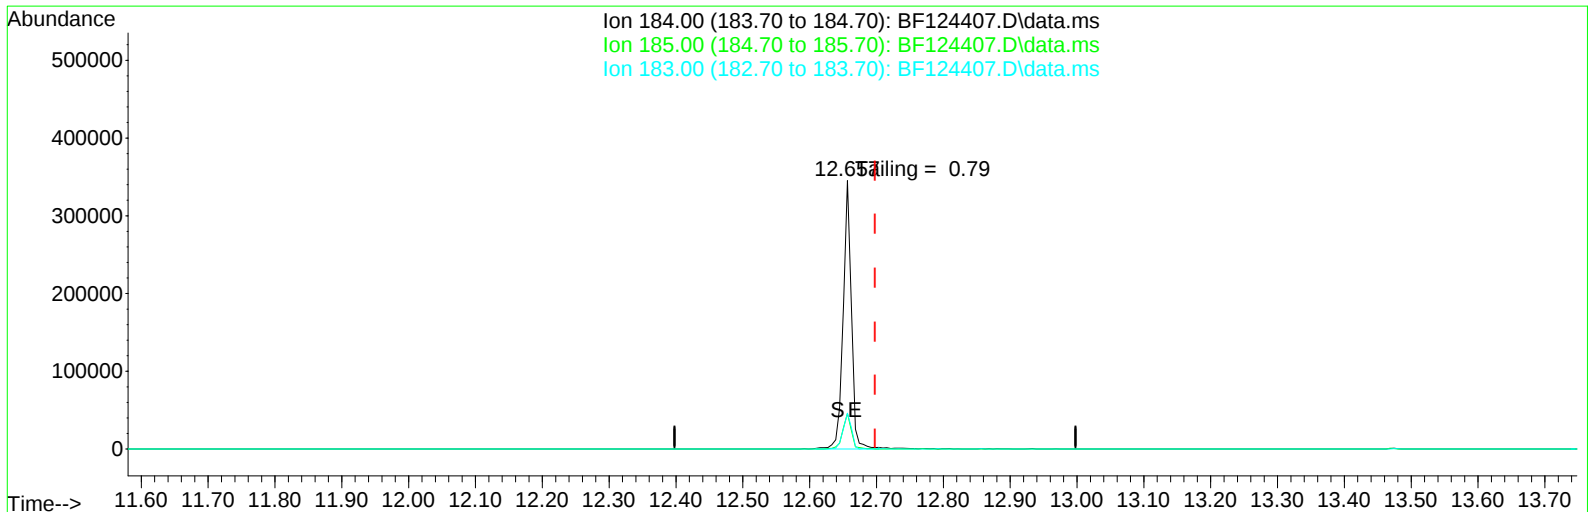

TIC: BF124407.D\data.ms

(77) Benzidine

12.657min (-0.041) 0.00 ng




response 298429

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.27
183.00	9.80	13.40#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062221\
Data File : BF124407.D
Acq On : 22 Jun 2021 12:17
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 22 13:39:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:09:26 2021
Response via : Initial Calibration

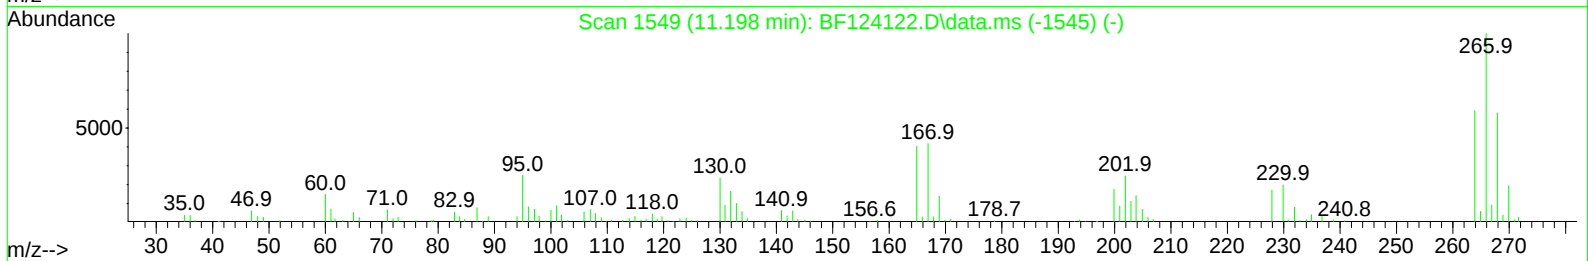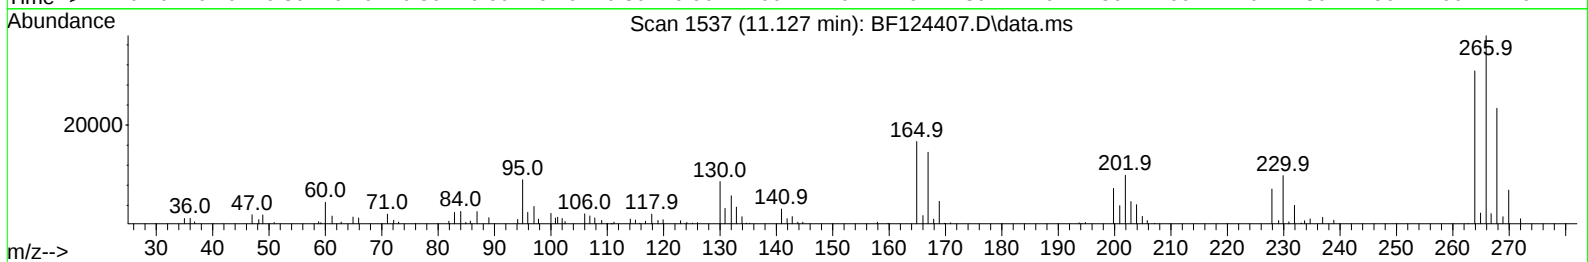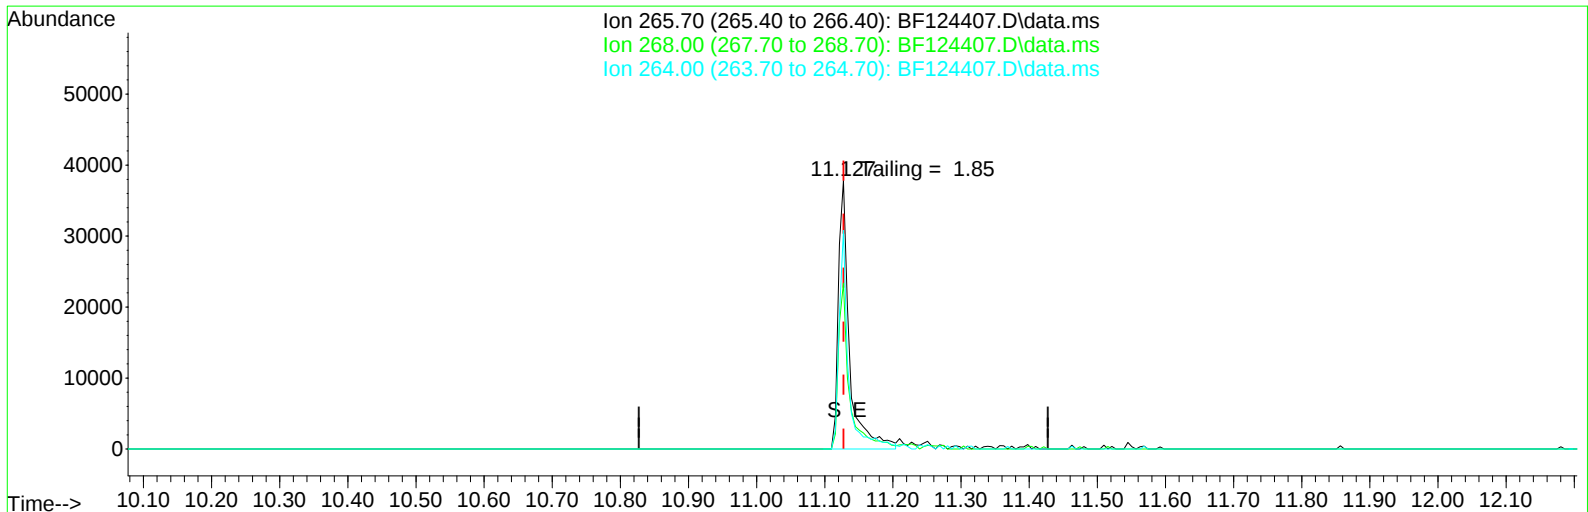

TIC: BF124407.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.000) 23103.76 ng

response 43004

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	61.75
264.00	65.70	81.43#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/22/2021	BNA_F	<u>BF124407.D</u>
Compound Name	Response	Retention Time
DDT	188006	13.47
DDD	1443	13.17
DDE	388	12.83
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1831	189837	0.96