
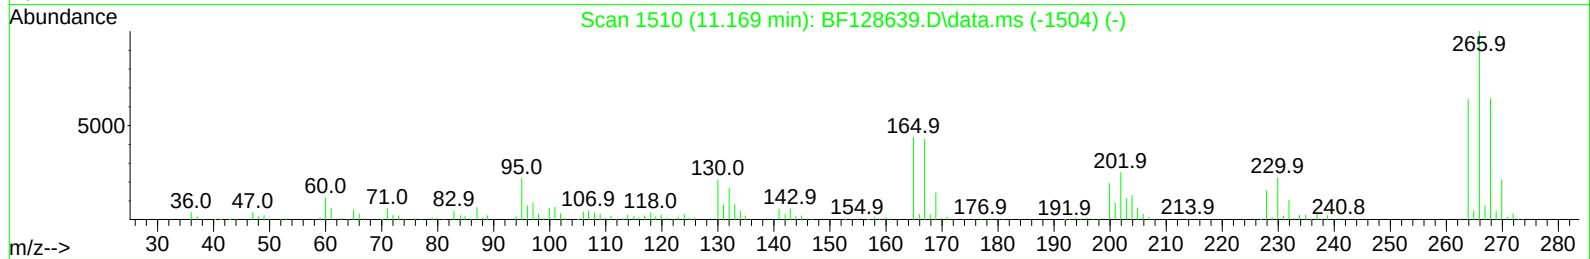
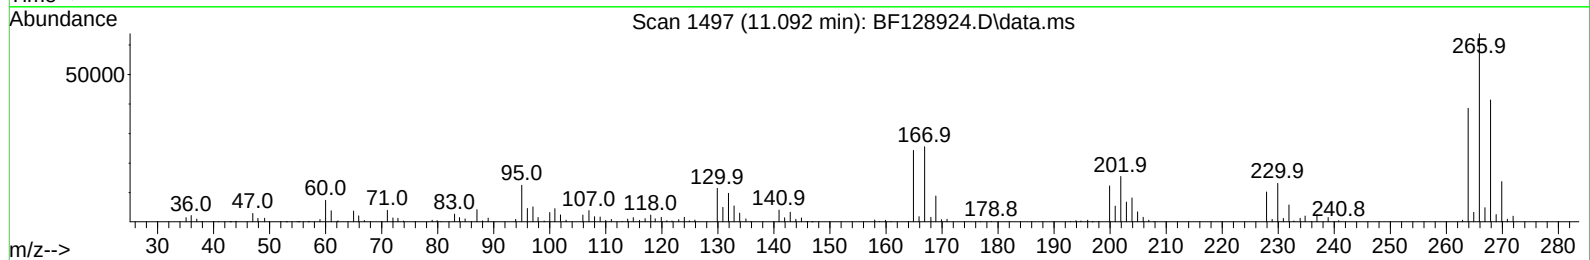


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
Data File : BF128924.D
Acq On : 22 Jun 2022 10:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 01:23:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:02:29 2022
Response via : Initial Calibration

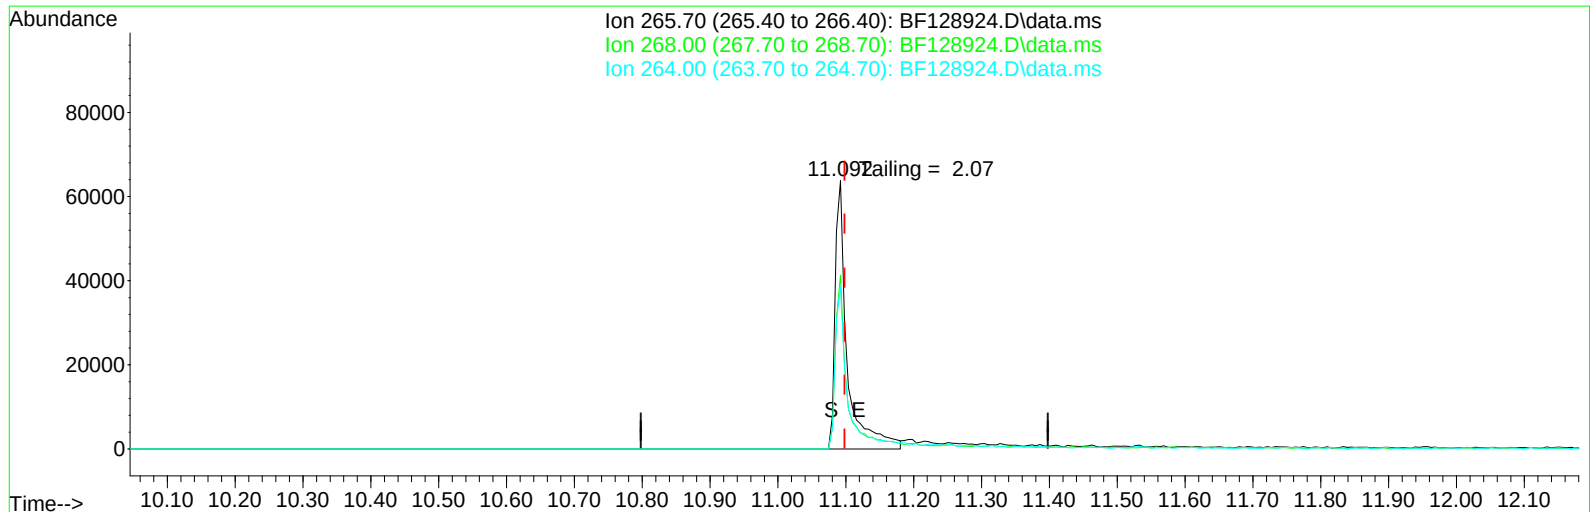

TIC: BF128924.D\data.ms

(70) Pentachlorophenol (C)




11.092min (-0.006) 23289.34 ng

response 79477

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.82
264.00	61.80	60.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
 Data File : BF128924.D
 Acq On : 22 Jun 2022 10:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 01:23:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 22 01:02:29 2022
 Response via : Initial Calibration

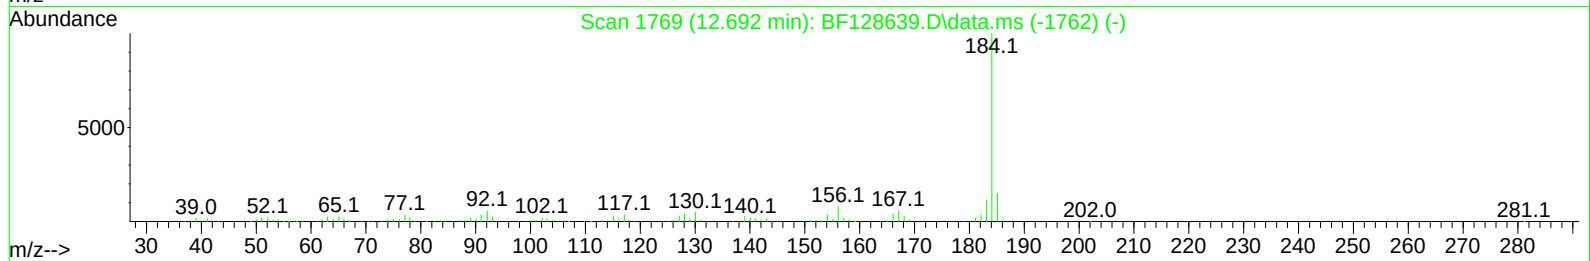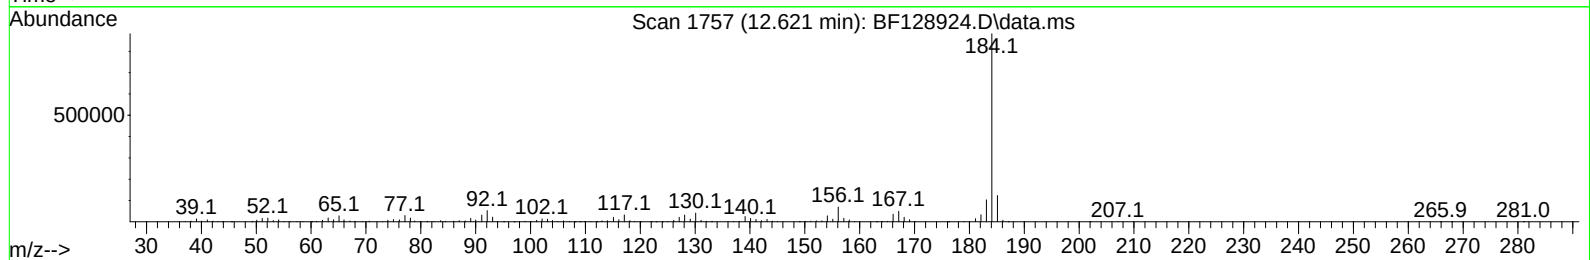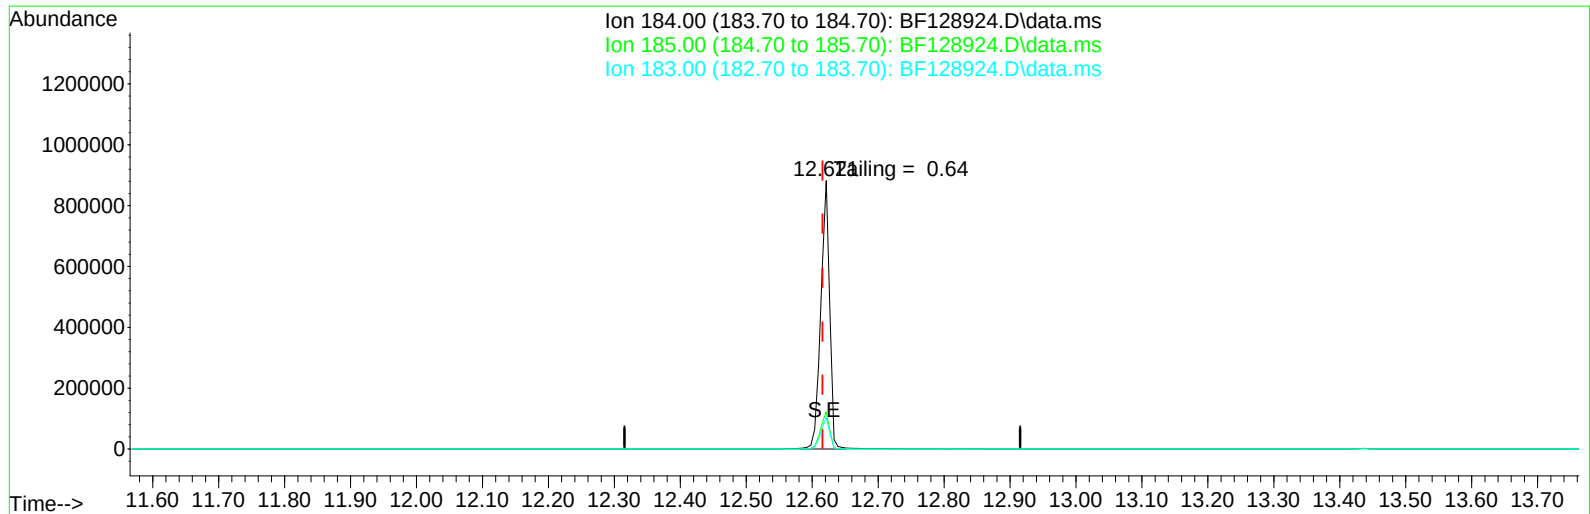

TIC: BF128924.D\data.ms

(77) Benzidine**12.621min (+ 0.006) 685908.27 ng****response 820393**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.94
183.00	11.60	11.71
0.00	0.00	0.00