

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
 Data File : BF128931.D
 Acq On : 22 Jun 2022 14:57
 Operator : CG\JU
 Sample : PB145737BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145737BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	525	529	546	rBV	3461724	3577096	72.52%	13.069%
2	6.410	696	701	722	rBV	3071023	3495088	70.86%	12.769%
3	6.745	754	758	762	rBV	868353	709960	14.39%	2.594%
4	7.316	849	855	858	rBV	2141816	2525462	51.20%	9.227%
5	8.028	970	976	980	rBV	945371	902750	18.30%	3.298%
6	9.110	1153	1160	1163	rBV	4752165	4685871	95.00%	17.120%
7	9.786	1268	1275	1278	rBV	1117208	1094216	22.18%	3.998%
8	10.580	1403	1410	1413	rBV	2835745	2577920	52.26%	9.419%
9	11.275	1521	1528	1531	rBV	1230977	1147269	23.26%	4.192%
10	12.869	1793	1799	1802	rVB	4911126	4932480	100.00%	18.021%
11	13.916	1973	1977	1981	rBV	1088408	956608	19.39%	3.495%
12	14.010	1987	1993	1997	rBV	60616	64165	1.30%	0.234%
13	15.363	2218	2223	2231	rVB	556983	701797	14.23%	2.564%




Sum of corrected areas: 27370682

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
Data File : BF128931.D
Acq On : 22 Jun 2022 14:57
Operator : CG\JU
Sample : PB145737BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

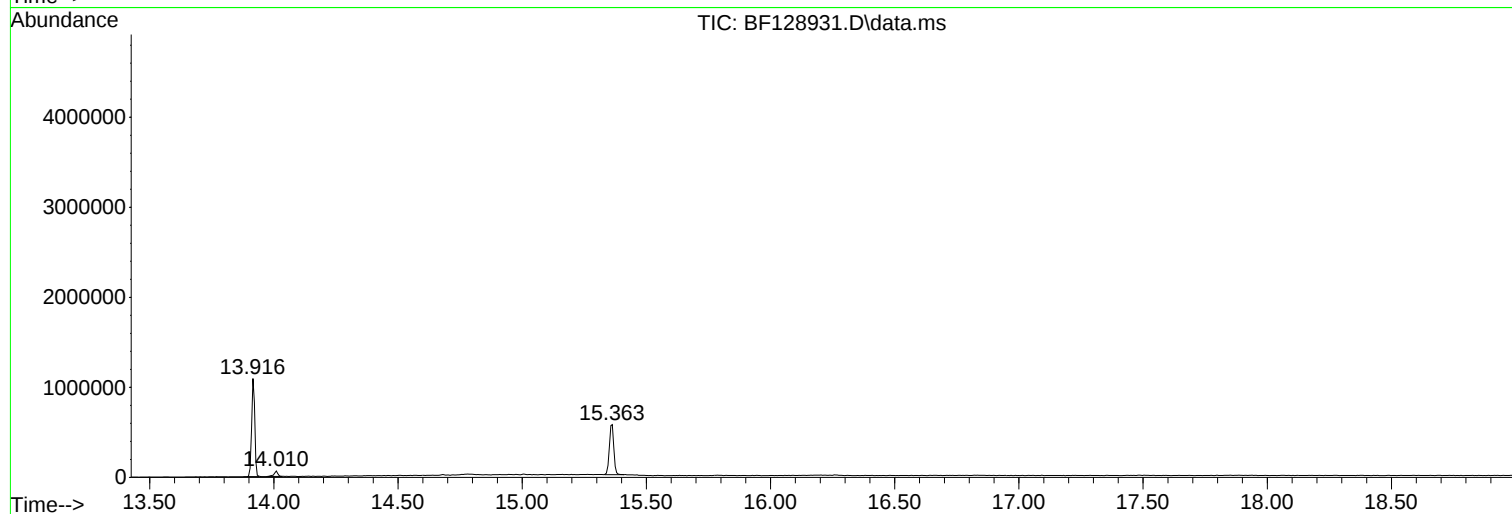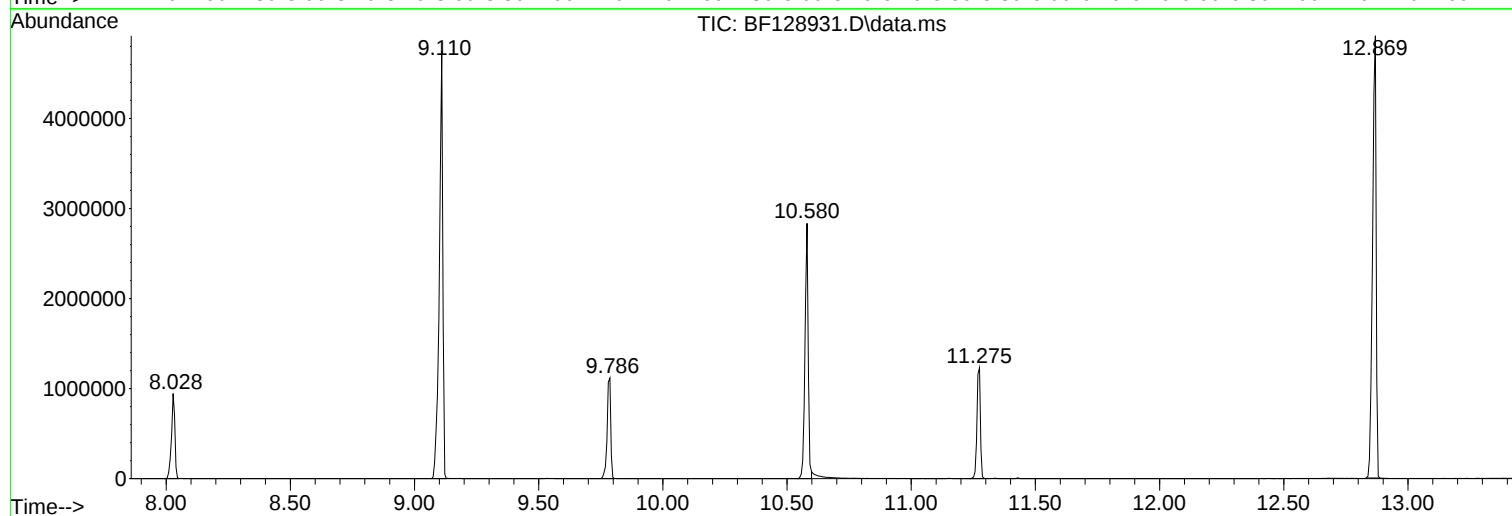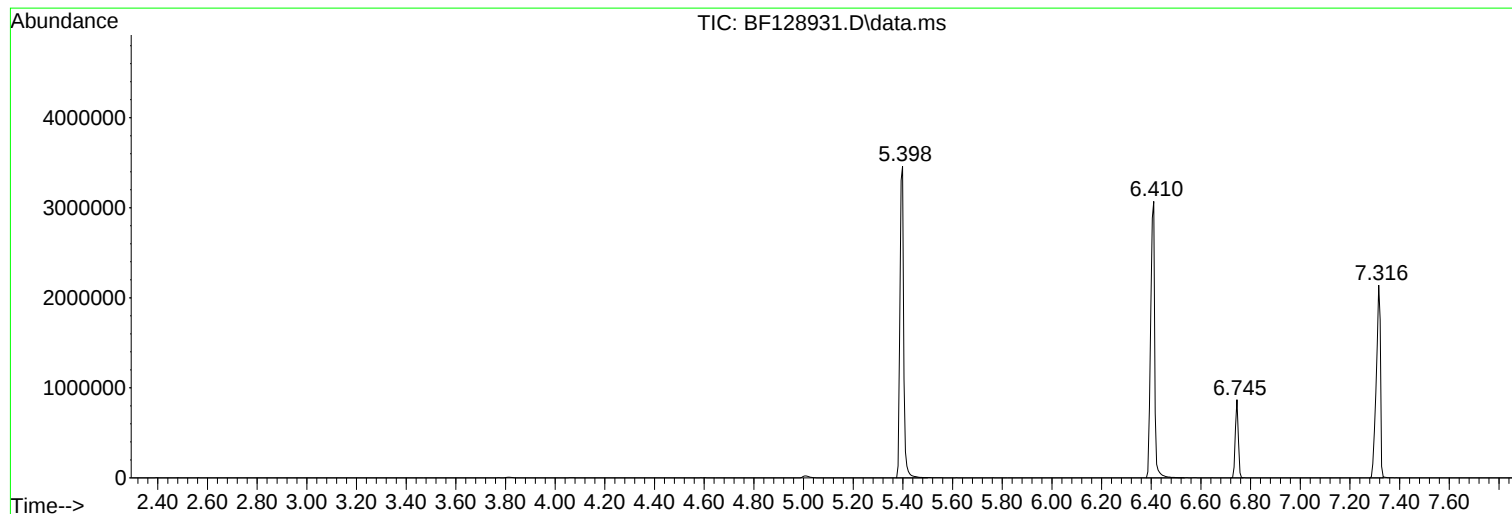

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
Data File : BF128931.D
Acq On : 22 Jun 2022 14:57
Operator : CG\JU
Sample : PB145737BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
Data File : BF128931.D
Acq On : 22 Jun 2022 14:57
Operator : CG\JU
Sample : PB145737BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------