

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
 Data File : BF128934.D
 Acq On : 22 Jun 2022 16:26
 Operator : CG\JU
 Sample : N3387-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-303-20220616

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	523	526	545	rBV	1446677	1469339	28.16%	5.998%
2	6.398	696	699	717	rBV	849091	886645	16.99%	3.619%
3	6.745	754	758	769	rVB	915205	776809	14.89%	3.171%
4	7.322	849	856	858	rBV	2217916	2751255	52.73%	11.230%
5	8.028	971	976	980	rBV	1103079	1003579	19.23%	4.097%
6	9.110	1153	1160	1163	rBV	4897474	4776265	91.54%	19.496%
7	9.780	1268	1274	1278	rBV	1176307	1107841	21.23%	4.522%
8	10.580	1403	1410	1413	rBV	3254095	3095023	59.32%	12.634%
9	11.269	1522	1527	1531	rBV	1311795	1200857	23.02%	4.902%
10	12.868	1791	1799	1802	rBV	5165467	5217669	100.00%	21.298%
11	13.915	1973	1977	1981	rVB	1221341	1079502	20.69%	4.406%
12	14.010	1987	1993	1999	rBV	85669	88652	1.70%	0.362%
13	14.680	2101	2107	2111	rBV	44412	59056	1.13%	0.241%
14	15.362	2217	2223	2230	rBV	776909	985728	18.89%	4.024%




Sum of corrected areas: 24498220

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
Data File : BF128934.D
Acq On : 22 Jun 2022 16:26
Operator : CG\JU
Sample : N3387-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20220616

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

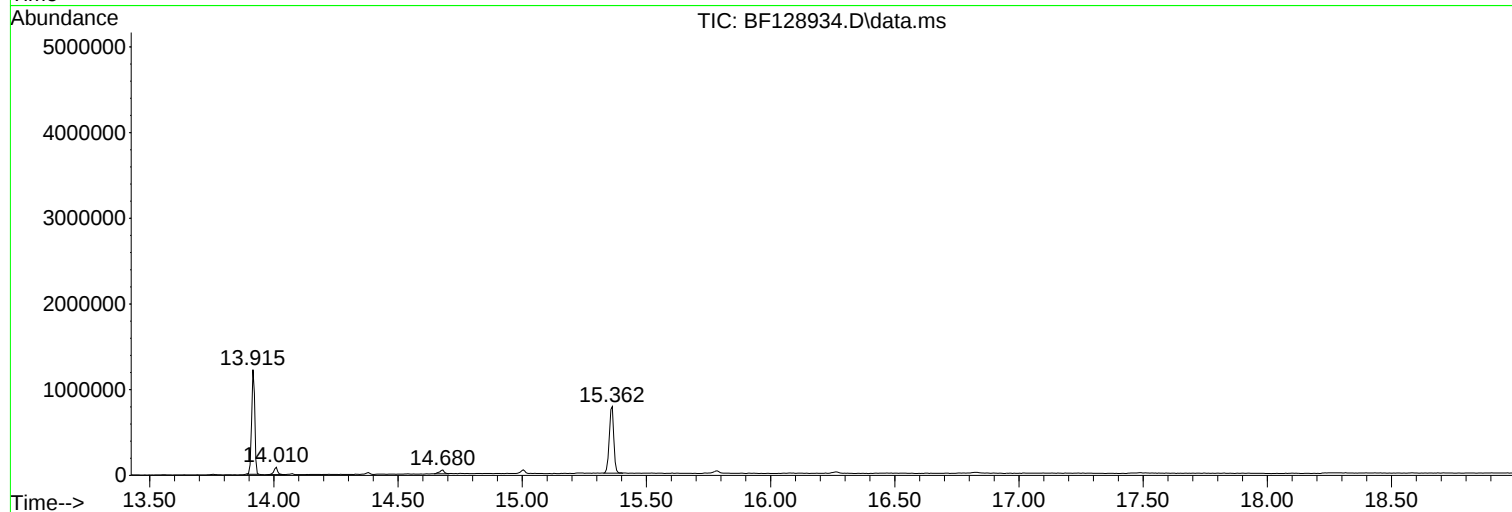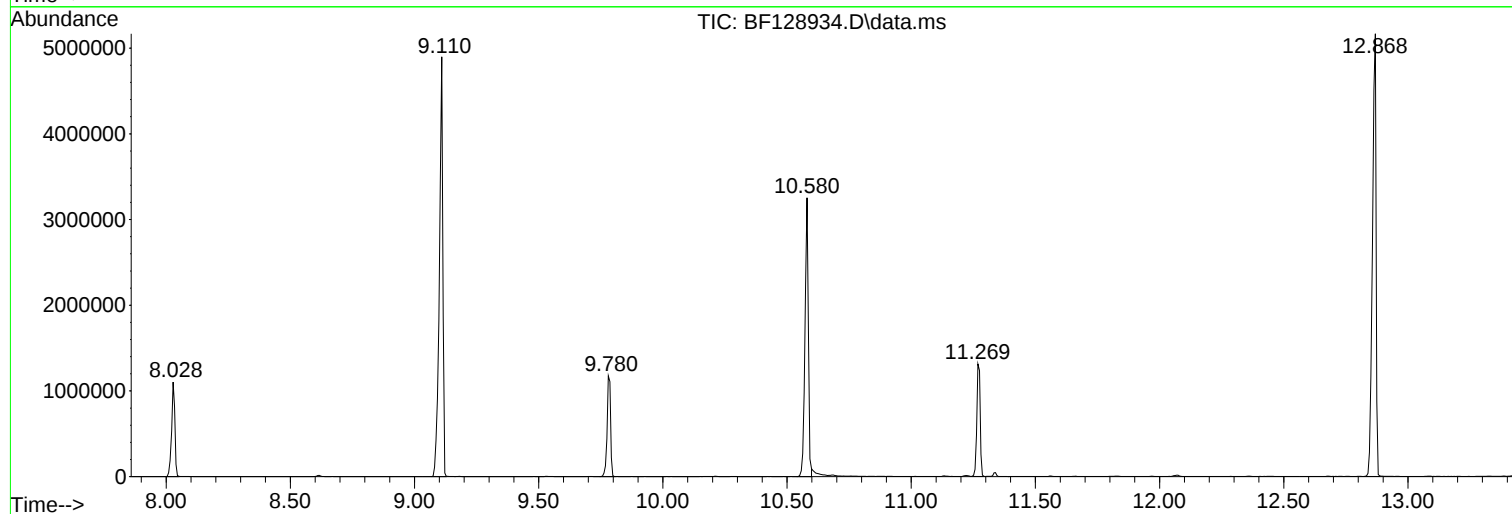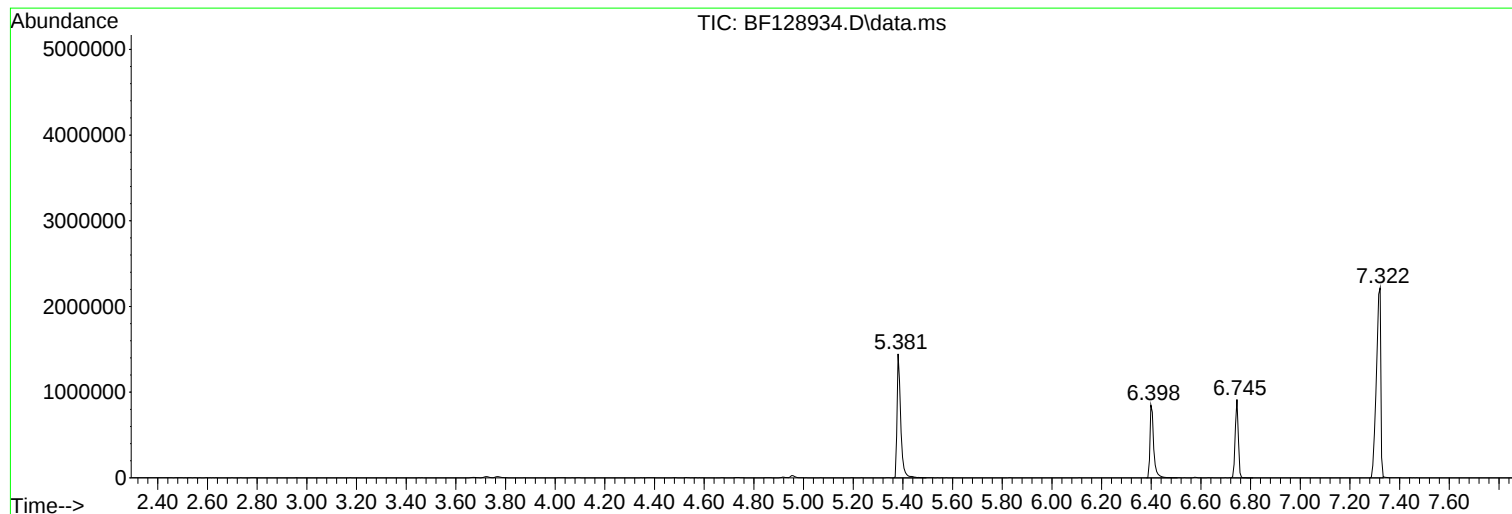

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
Data File : BF128934.D
Acq On : 22 Jun 2022 16:26
Operator : CG\JU
Sample : N3387-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20220616

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
Data File : BF128934.D
Acq On : 22 Jun 2022 16:26
Operator : CG\JU
Sample : N3387-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20220616

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------