
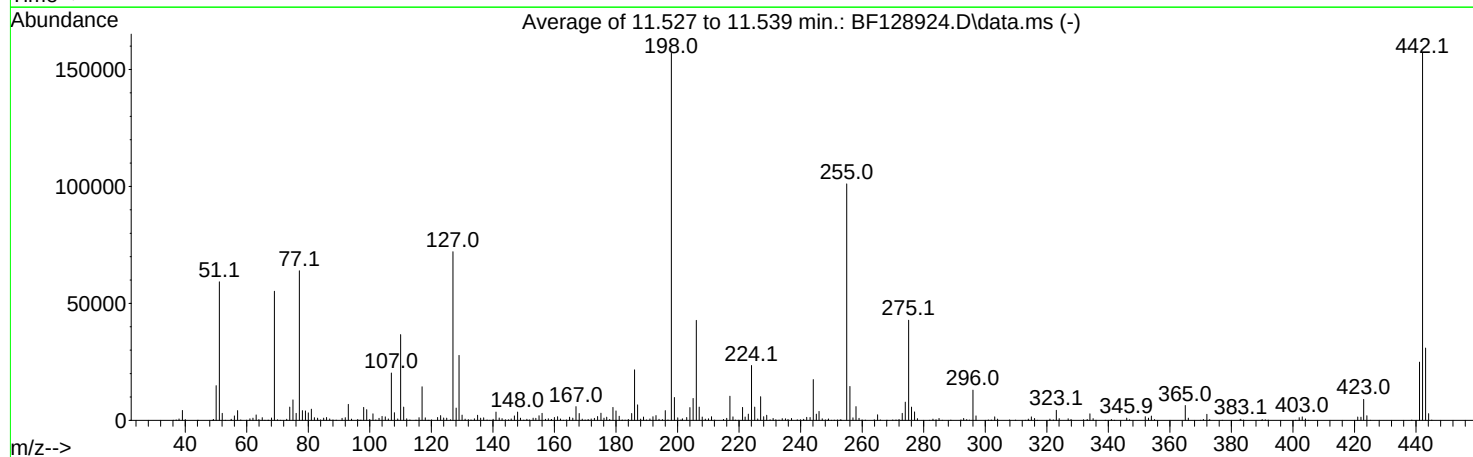


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
 Data File : BF128924.D
 Acq On : 22 Jun 2022 10:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 23 14:30:33 2022

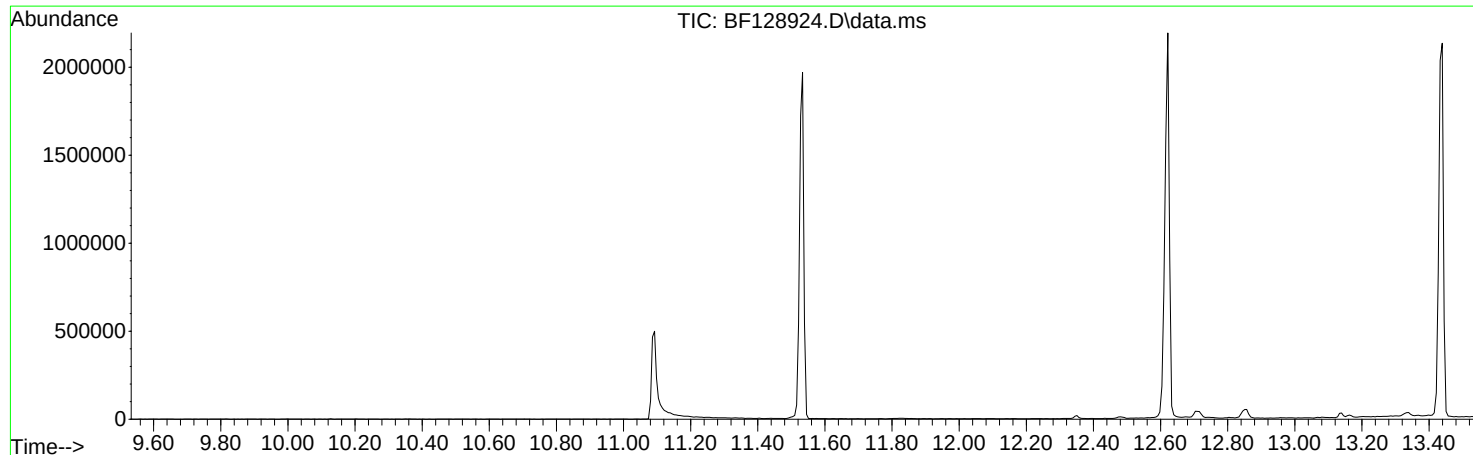




AutoFind: Scans 1571, 1572, 1573; Background Corrected with Scan 1564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	59234	PASS
68	69	0.00	2	1.9	1021	PASS
69	198	0.00	100	35.2	55184	PASS
70	69	0.00	2	0.5	252	PASS
127	198	10	80	46.0	72112	PASS
197	198	0.00	2	0.1	179	PASS
198	198	100	100	100.0	156931	PASS
199	198	5	9	6.3	9811	PASS
275	198	10	60	27.3	42792	PASS
365	198	1	100	4.1	6388	PASS
441	198	0.01	100	15.9	24912	PASS
442	442	50	100	100.0	157275	PASS
443	442	15	24	19.7	30923	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
Data File : BF128924.D
Acq On : 22 Jun 2022 10:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 23 01:23:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:02:29 2022
Response via : Initial Calibration

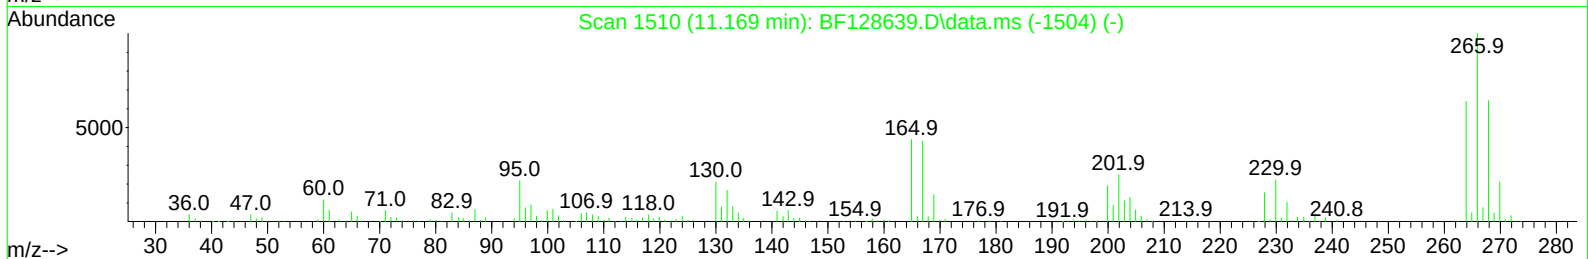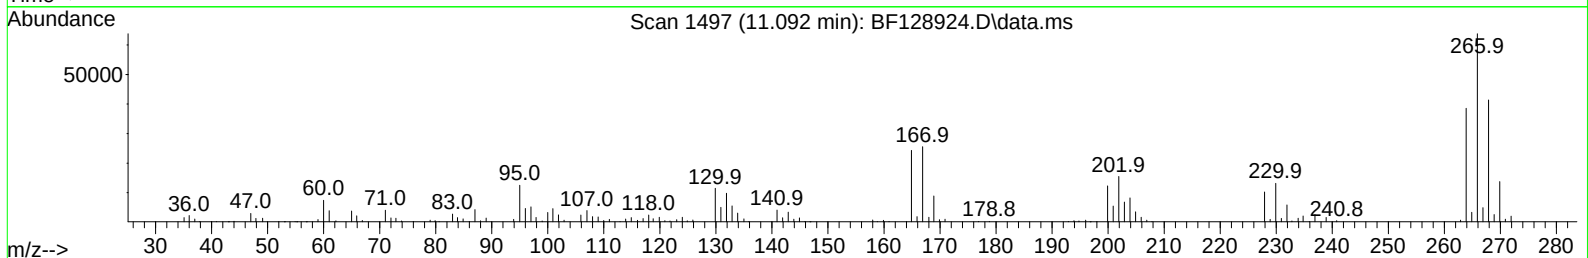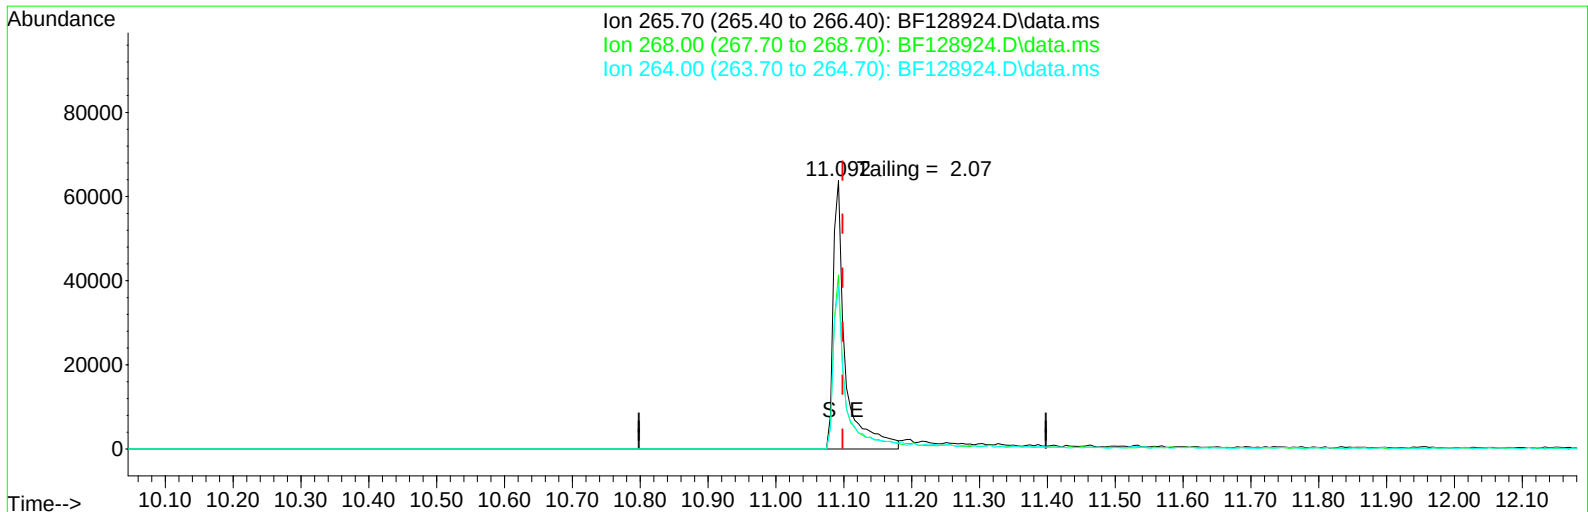

TIC: BF128924.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.006) 23289.34 ng




response 79477

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.82
264.00	61.80	60.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062222\
Data File : BF128924.D
Acq On : 22 Jun 2022 10:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 23 01:23:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:02:29 2022
Response via : Initial Calibration

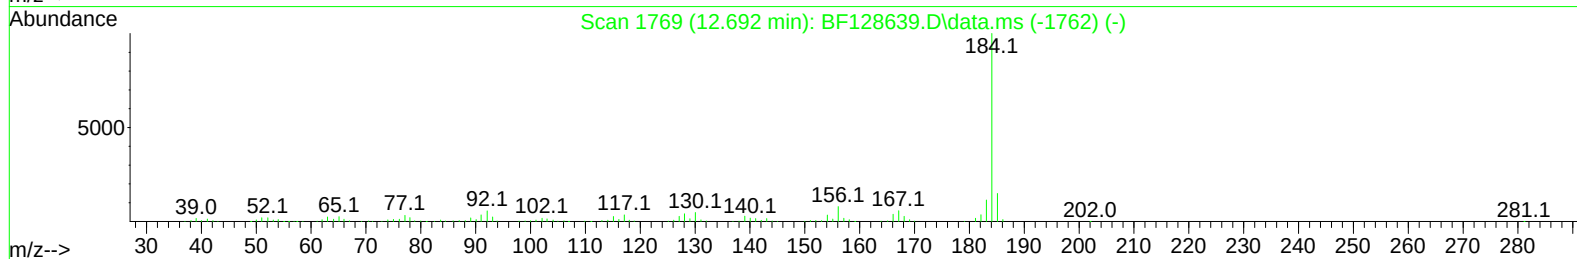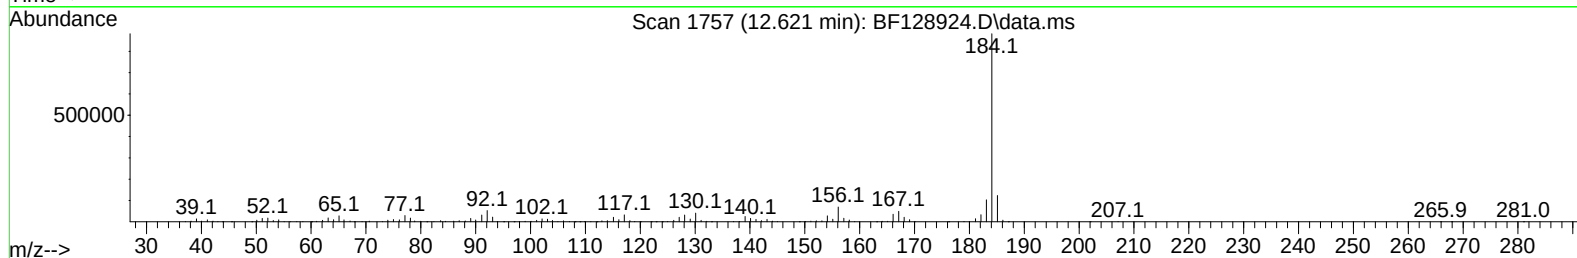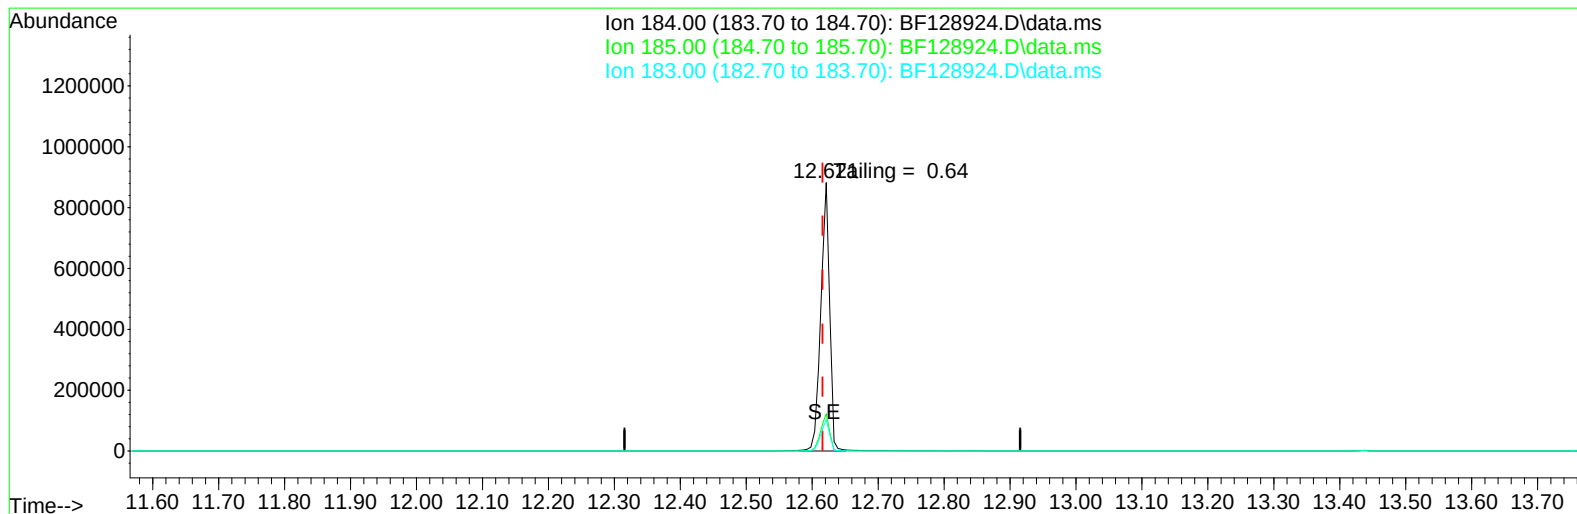

TIC: BF128924.D\data.ms

(77) Benzidine

12.621min (+ 0.006) 685908.27 ng

response 820393

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.94
183.00	11.60	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/22/2022	BNA_F	<u>BF128924.D</u>
Compound Name	Response	Retention Time
DDT	385301	13.439
DDD	7299	13.139
DDE	2223	12.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9522	394823	2.41

Instrument :
BNA_F
ClientSampleId :
DFTPP