

Data Path : Z:\HPCHEM1\BNA_F\Data\BF062316\
 Data File : BF088325.D
 Acq On : 24 Jun 2016 9:59
 Operator : UM/SJ
 Sample : H3084-02DL 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 0.25

Instrument :
 BNA_F
 ClientSampleId :
 LF001MW001-160512DL

Quant Time: Jun 24 11:55:42 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 22 14:55:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.54	152	585	5.00	ng	-0.07
21) Naphthalene-d8	7.88	136	81951	5.00	ng	-0.01
38) Acenaphthene-d10	9.62	164	40584	5.00	ng	-0.02
63) Phenanthrene-d10	11.10	188	61675	5.00	ng	-0.02
75) Chrysene-d12	13.73	240	45947	5.00	ng	-0.02
86) Perylene-d12	15.09	264	40536	5.00	ng	-0.02

System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	1666	12.17	ng	0.05
7) Phenol-d6	6.28	99	3325	20.04	ng	0.02
23) Nitrobenzene-d5	7.18	82	3933	0.70	ng	0.00
41) 2,4,6-Tribromophenol	10.42	330	752	0.44	ng	-0.01
44) 2-Fluorobiphenyl	8.96	172	6223	-0.84	ng	-0.01
78) Terphenyl-d14	12.67	244	4925	0.61	ng	-0.02


Target Compounds						Qvalue
3) Pyridine	2.62	79	1233	7.85	ng	# 1
4) n-Nitrosodimethylamine	2.62	42	84733	1274.05	ng	# 1
8) 2-Chlorophenol	6.20	128	820	5.06	ng	# 1
9) Benzaldehyde	6.10	77	5405	Below Cal		# 1
10) Phenol	6.30	94	21845	134.35	ng	98
12) 1,3-Dichlorobenzene	6.54	146	17840	102.63	ng	95
13) 1,4-Dichlorobenzene	6.54	146	17840	101.88	ng	97
14) 1,2-Dichlorobenzene	6.76	146	340928	2140.85	ng	96
15) Benzyl Alcohol	6.65	79	7255	55.90	ng	# 6
16) 2,2'-oxybis(1-Chloropropan	6.98	45	100931	513.59	ng	90
17) 2-Methylphenol	6.89	107	25363	193.04	ng	95
18) Hexachloroethane	7.06	117	344	5.54	ng	# 1
19) n-Nitroso-di-n-propylamine	6.99	70	23710	223.42	ng	# 1
20) 3+4-Methylphenols	7.05	107	101733	663.61	ng	# 75
22) Acetophenone	7.03	105	21456	2.93	ng	# 64
24) Nitrobenzene	7.05	77	38074	7.00	ng	# 36
27) 2,4-Dimethylphenol	7.59	122	21733	4.05	ng	# 93
31) Naphthalene	7.90	128	168393	10.38	ng	98
32) Benzoic acid	7.70	122	183521	62.14	ng	# 15
33) 4-Chloroaniline	7.90	127	21304	2.94	ng	# 31
45) 1,1'-Biphenyl	9.06	154	6079	Below Cal		87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\Data\BF062316\
Data File : BF088325.D
Acq On : 24 Jun 2016 9:59
Operator : UM/SJ
Sample : H3084-02DL 10X
Misc :
ALS Vial : 29 Sample Multiplier: 0.25

Instrument :
BNA_F
ClientSampleId :
LF001MW001-160512DL

Quant Time: Jun 24 11:55:42 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

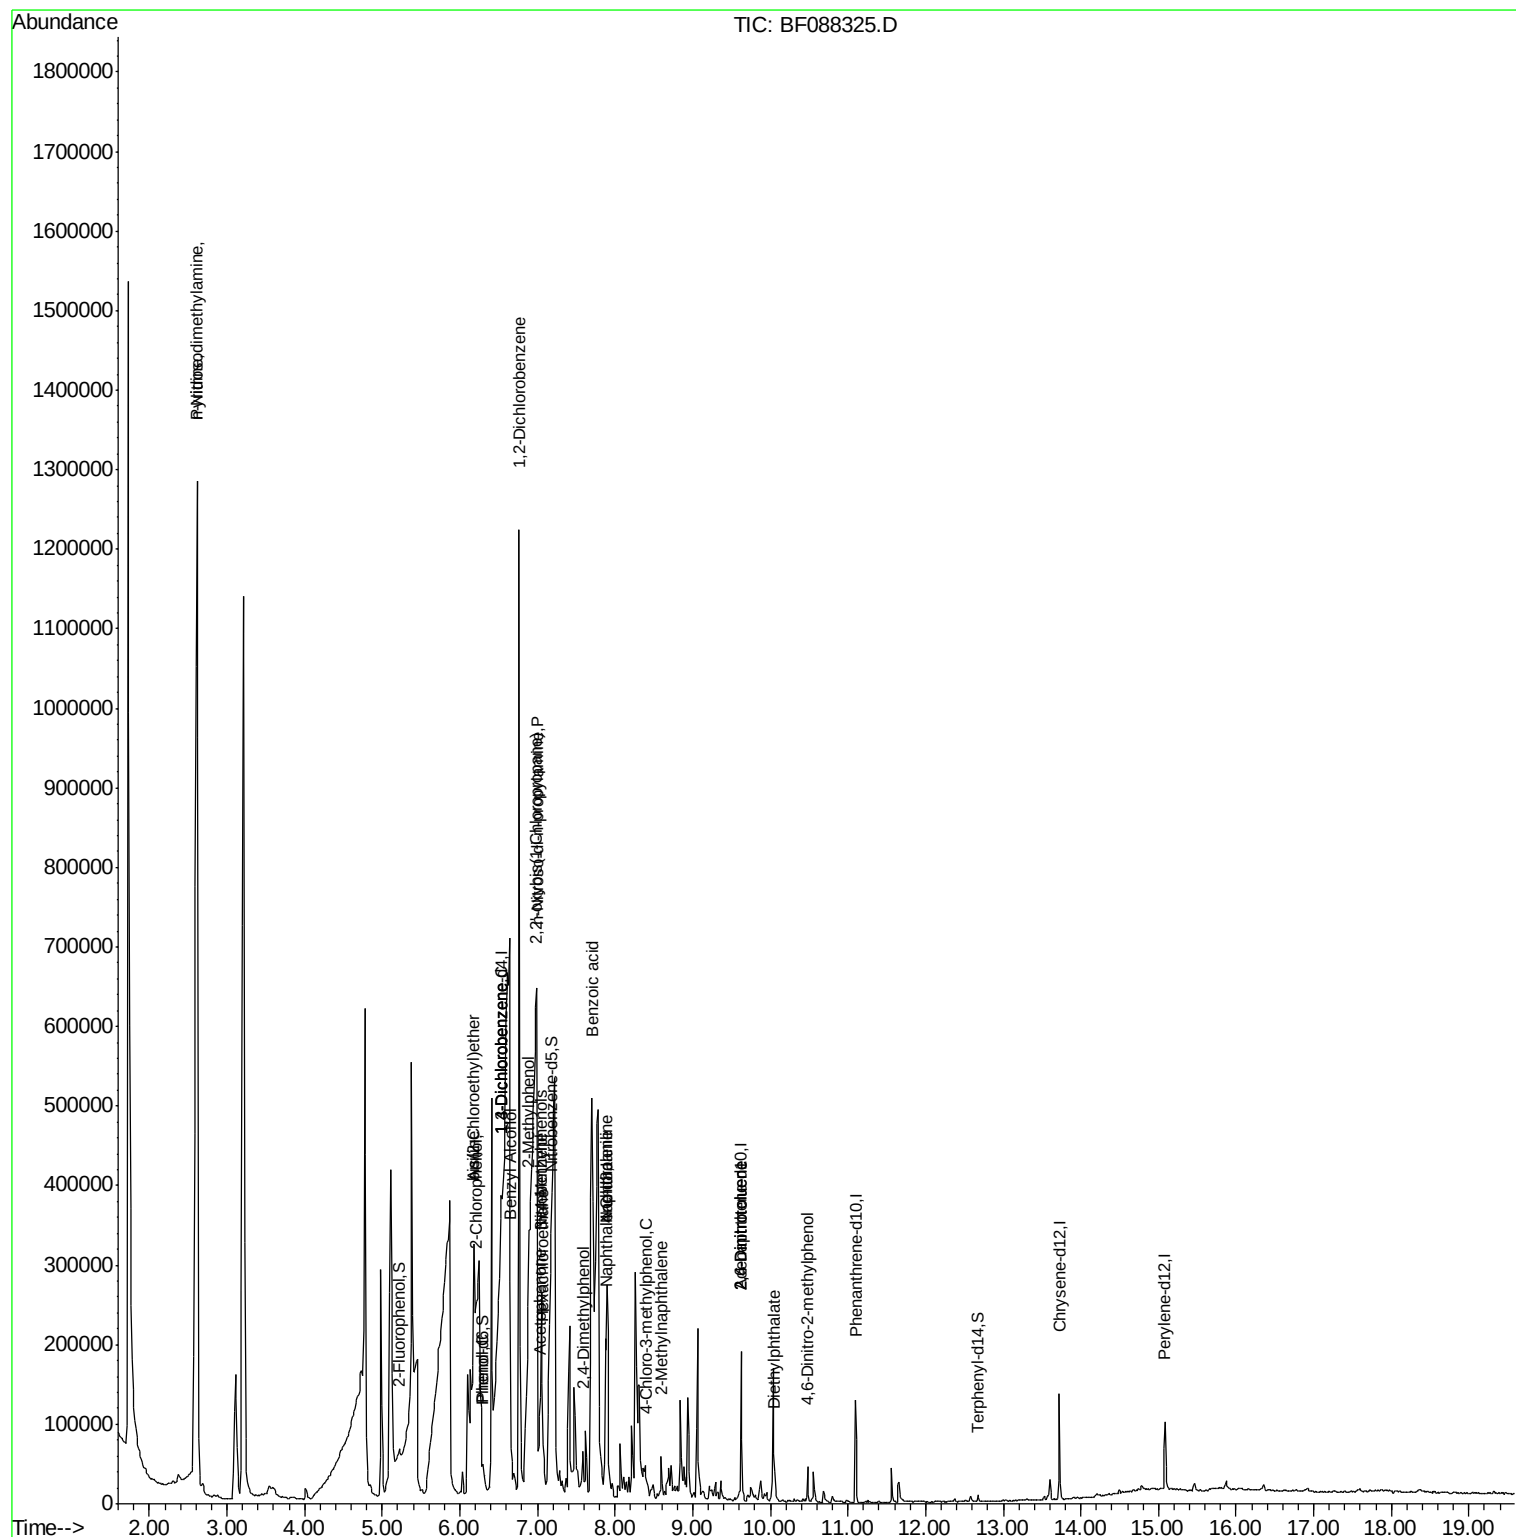

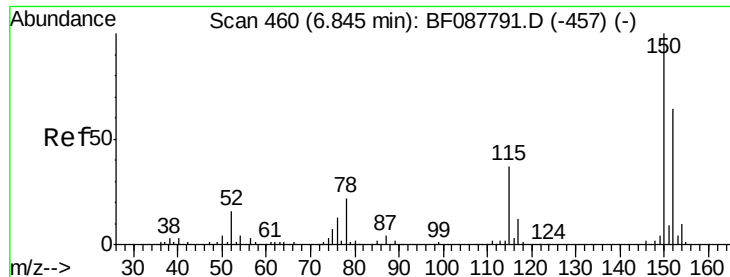

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 6.54 min Scan# 433

Delta R.T. -0.07 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59

Instrument :

BNA_F

ClientSampleId :

LF001MW001-160512DL


Tgt Ion:152 Resp: 585

Ion Ratio Lower Upper

152 100

150 159.6 123.8 185.6




115 46.0 39.6 59.4

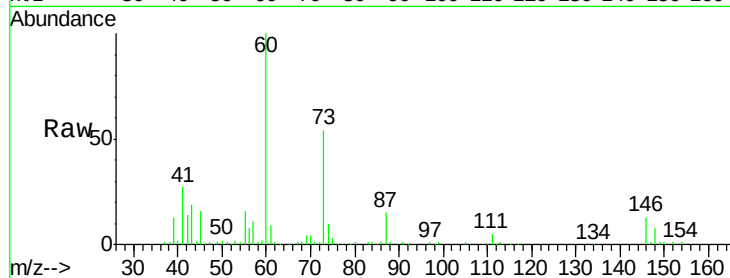

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

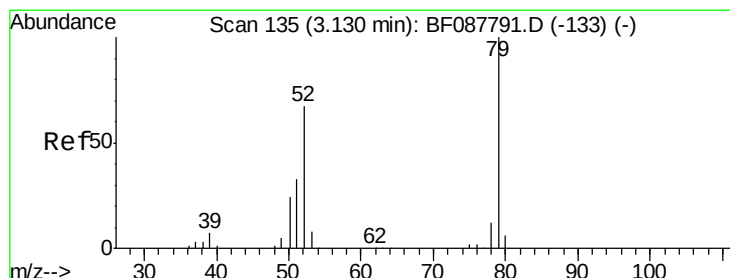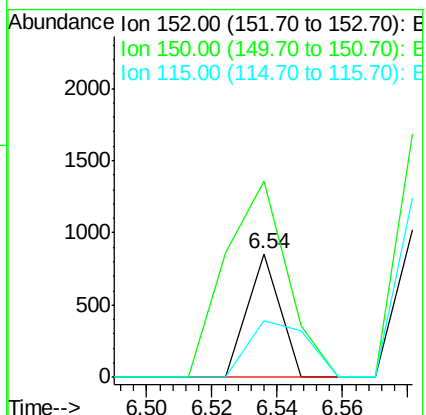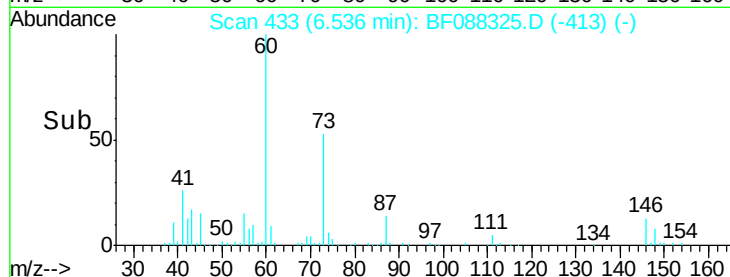

#3

Pyridine

Concen: 7.85 ng

RT: 2.62 min Scan# 90

Delta R.T. -0.06 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59


Tgt Ion: 79 Resp: 1233

Ion Ratio Lower Upper

79 100

52 209.7 56.3 84.5#



51 775.3 27.4 41.2#

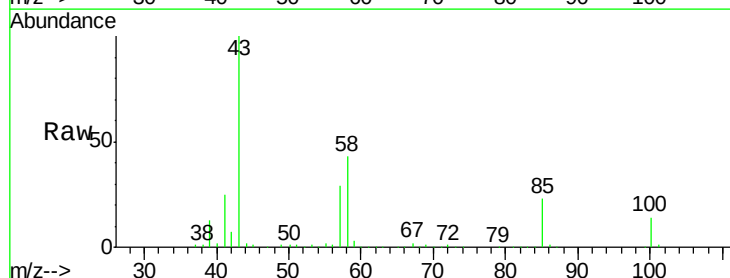


Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 52.00 (51.70 to 52.70): BF0

Ion 51.00 (50.70 to 51.70): BF0

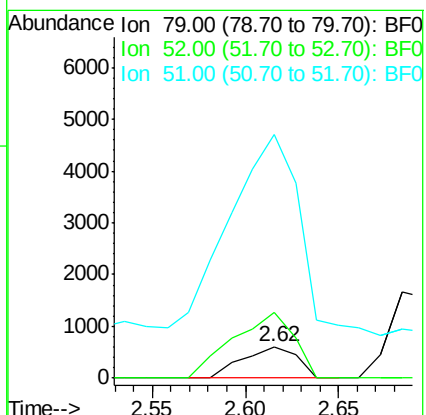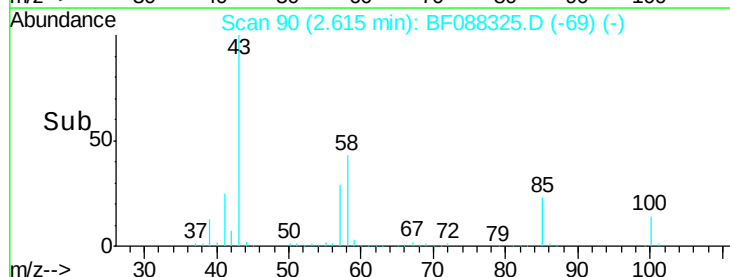



#4

n-Nitrosodimethylamine

Concen: 1274.05 ng

RT: 2.62 min Scan# 90

Delta R.T. -0.01 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59

Instrument :





BNA_F

ClientSampleId :

LF001MW001-160512DL

Tgt Ion: 42 Resp: 84733

Ion	Ratio	Lower	Upper
42	100		
74	1.7	108.6	163.0#
44	34.4	5.5	8.3#

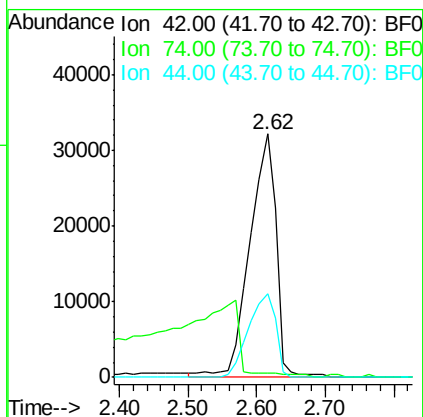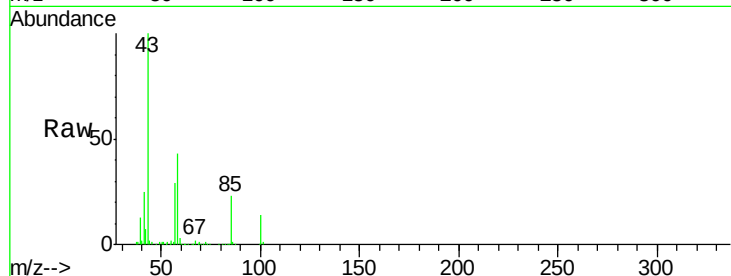

#5

2-Fluorophenol

Concen: 12.17 ng

RT: 5.22 min Scan# 318




Delta R.T. 0.05 min


Lab File: BF088325.D

Acq: 24 Jun 2016 9:59

Tgt Ion: 112 Resp: 1666

Ion	Ratio	Lower	Upper
112	100		
64	47.9	42.2	63.2
63	0.0	21.8	32.8#

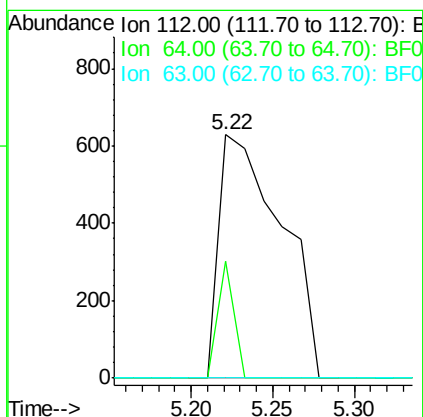

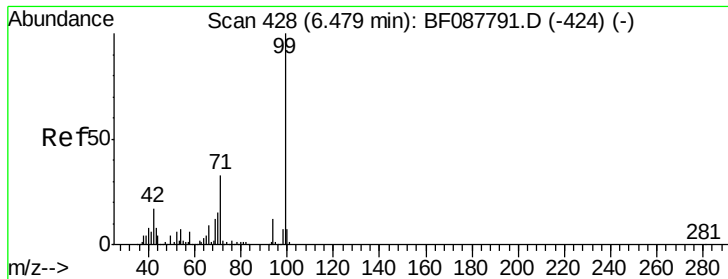

#7

Phenol-d6

Concen: 20.04 ng

RT: 6.28 min Scan# 411

Delta R.T. 0.02 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59

Instrument :

BNA_F

ClientSampleId :

LF001MW001-160512DL


Tgt Ion: 99 Resp: 3325

Ion Ratio Lower Upper

99 100

42 62.8 12.2 18.2#




71 64.7 23.4 35.0#

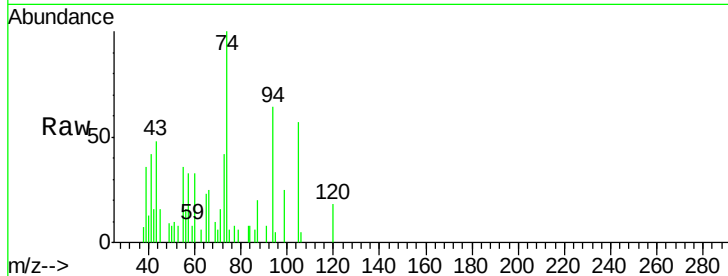

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

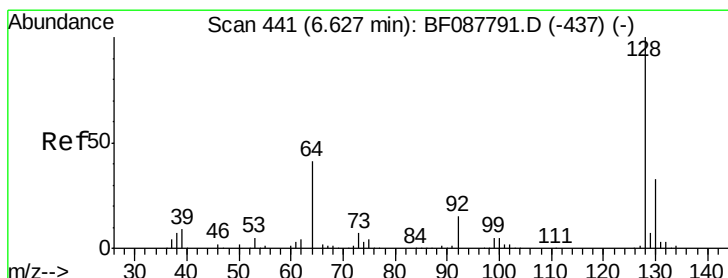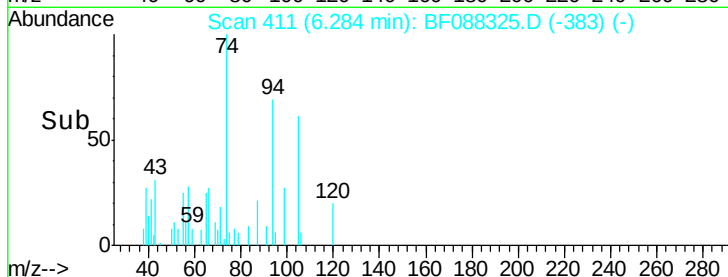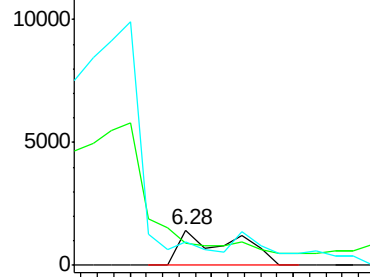

#8

2-Chlorophenol

Concen: 5.06 ng

RT: 6.20 min Scan# 404

Delta R.T. -0.18 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59


Tgt Ion: 128 Resp: 820

Ion Ratio Lower Upper

128 100

130 0.0 12.0 52.0#



64 144.7 30.8 70.8#

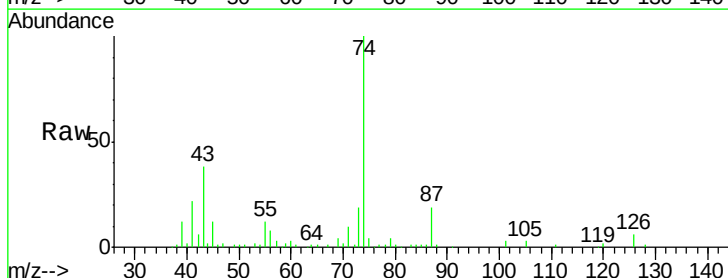


Abundance Ion 128.00 (127.70 to 128.70): E

Ion 130.00 (129.70 to 130.70): E

Ion 64.00 (63.70 to 64.70): BF0

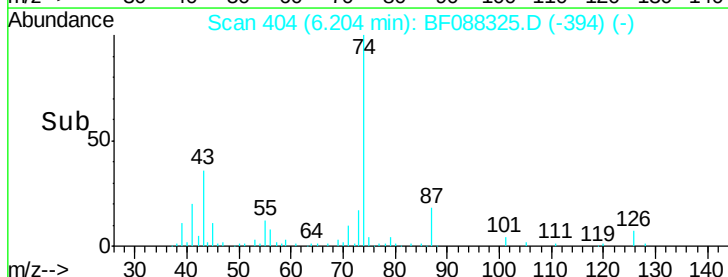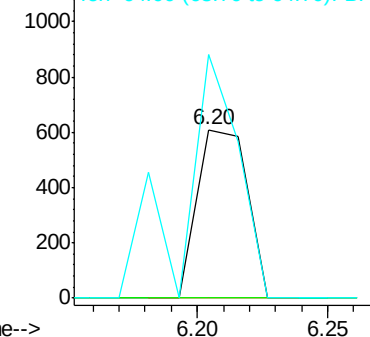



#9

Benzaldehyde

Concen: Below Cal

RT: 6.10 min Scan# 395

Delta R.T. -0.05 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59

Instrument :

BNA_F

ClientSampleId :

LF001MW001-160512DL





Tgt Ion: 77 Resp: 5405

Ion Ratio Lower Upper

77 100

105 840.4 90.6 130.6#

106 76.5 85.3 125.3#

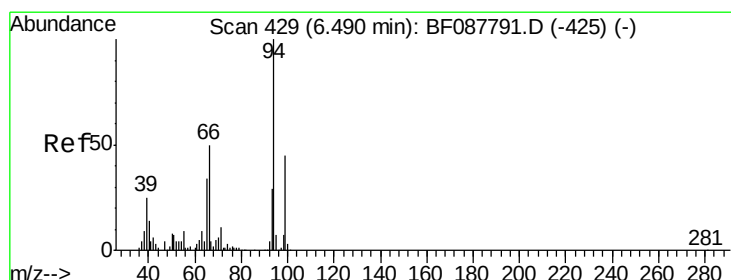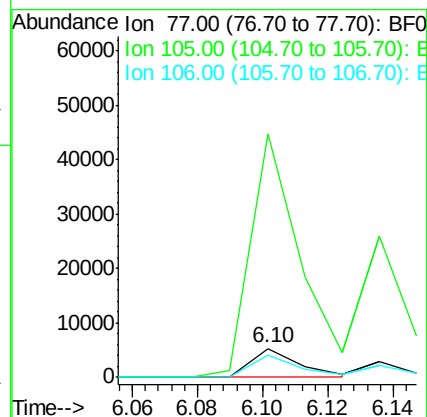

#10

Phenol

Concen: 134.35 ng

RT: 6.30 min Scan# 412

Delta R.T. 0.02 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59




Tgt Ion: 94 Resp: 21845


Ion Ratio Lower Upper

94 100

65 25.8 5.9 45.9

66 32.4 14.0 54.0

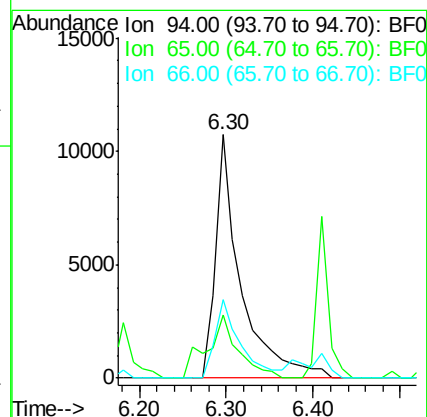

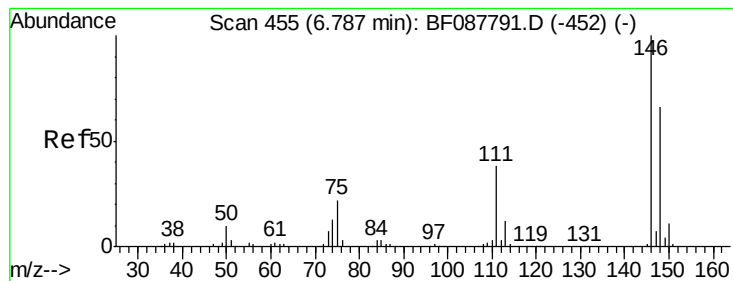

#12

1,3-Dichlorobenzene

Concen: 102.63 ng

RT: 6.54 min Scan# 433

Delta R.T. -0.00 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59

Instrument :

BNA_F

ClientSampleId :

LF001MW001-160512DL





Tgt Ion:146 Resp: 17840

Ion Ratio Lower Upper

146 100

148 66.0 50.9 76.3

75 27.5 25.6 38.4

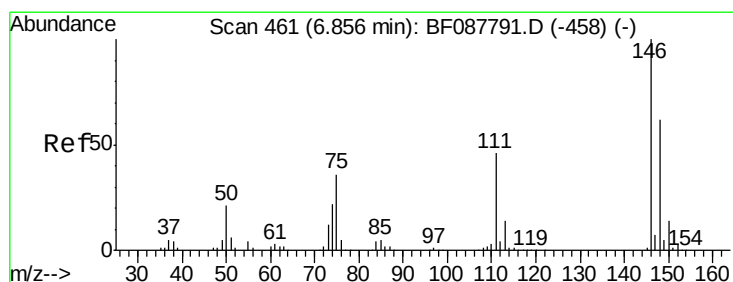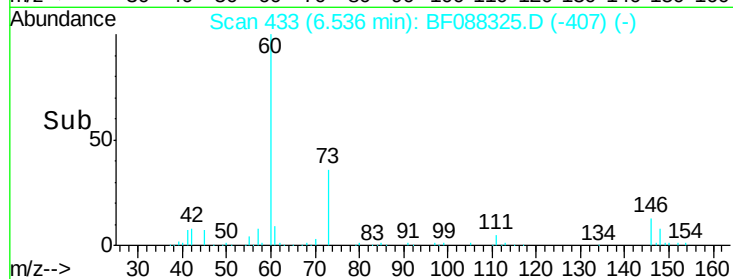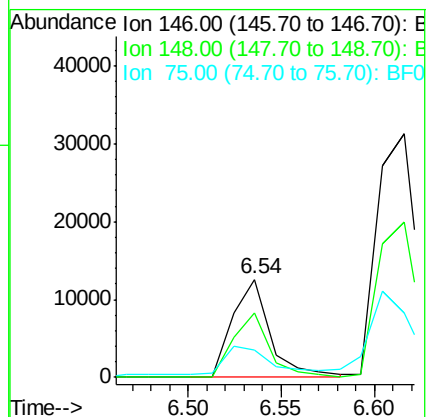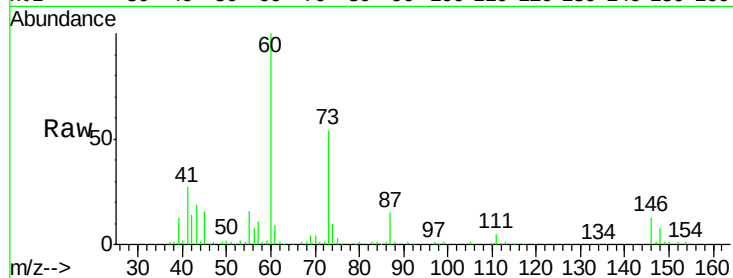

#13

1,4-Dichlorobenzene

Concen: 101.88 ng

RT: 6.54 min Scan# 433

Delta R.T. -0.08 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59




Tgt Ion:146 Resp: 17840


Ion Ratio Lower Upper

146 100

148 66.0 52.0 78.0

111 39.5 33.8 50.8

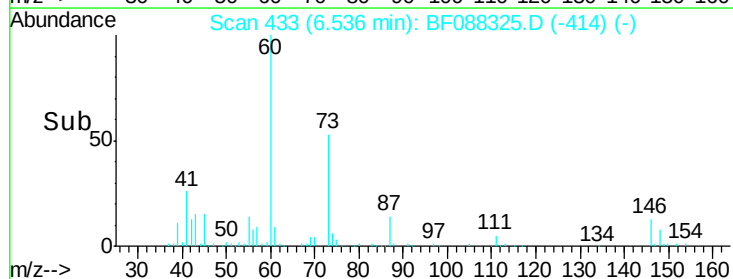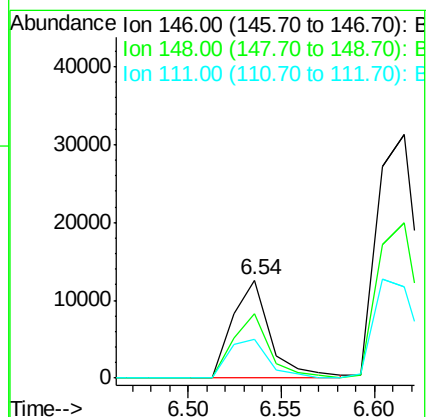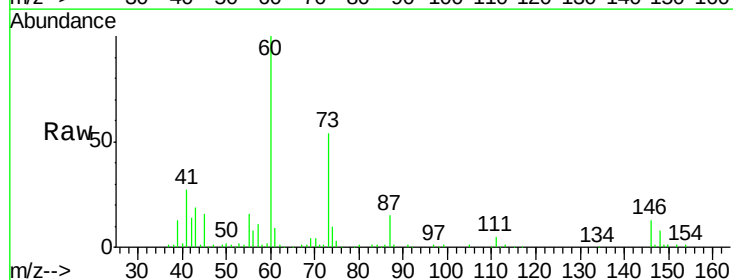

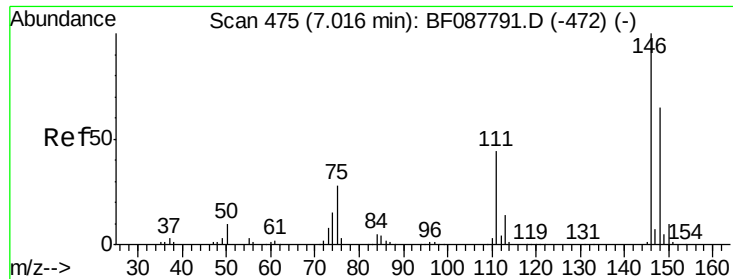

#14

1,2-Dichlorobenzene

Concen: 2140.85 ng

RT: 6.76 min Scan# 453

Delta R.T. -0.01 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59

Instrument :

BNA_F

ClientSampleId :

LF001MW001-160512DL


Tgt Ion:146 Resp: 340928

Ion Ratio Lower Upper

146 100

148 64.7 52.3 78.5




111 42.2 28.7 43.1

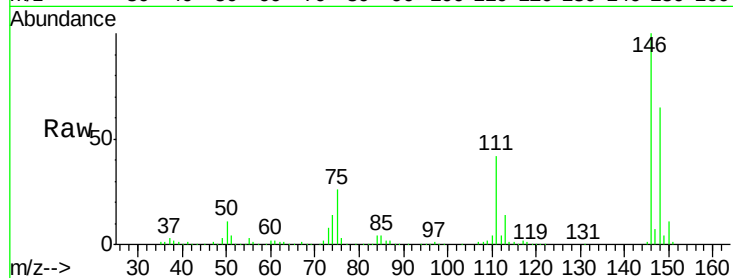

Abundance Ion 146.00 (145.70 to 146.70): E

Ion 148.00 (147.70 to 148.70): E

Ion 111.00 (110.70 to 111.70): E

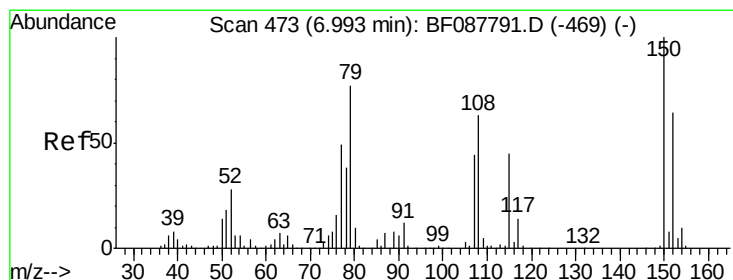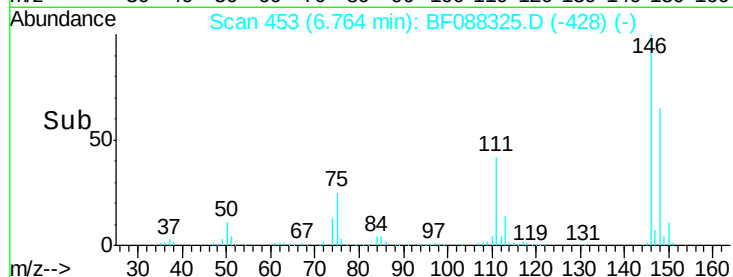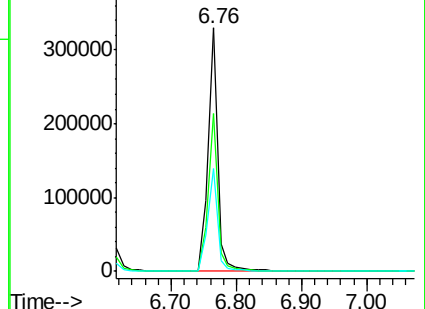

#15

Benzyl Alcohol

Concen: 55.90 ng

RT: 6.65 min Scan# 443

Delta R.T. -0.11 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59


Tgt Ion: 79 Resp: 7255

Ion Ratio Lower Upper

79 100

108 0.0 65.0 97.6#



77 138.1 50.3 75.5#

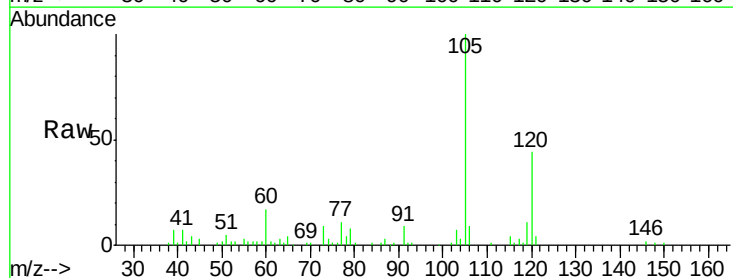


Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BF0



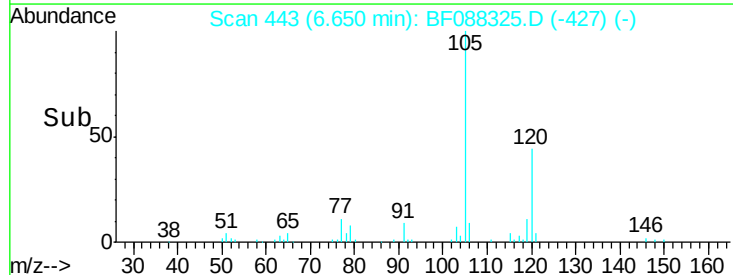
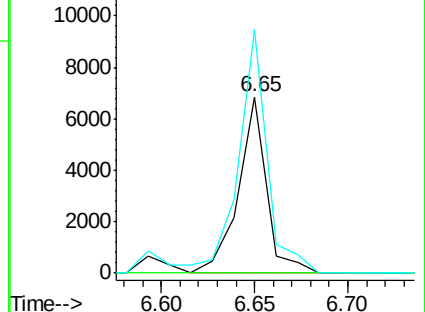




#16
2,2'-oxybis(1-Chloropropane)
Concen: 513.59 ng
RT: 6.98 min Scan# 472
Delta R.T. 0.08 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59




Instrument :
BNA_F
ClientSampleId :
LF001MW001-160512DL


Tgt Ion	Ratio	Lower	Upper
45	100		
77	6.2	0.0	32.5
79	9.0	0.0	29.5

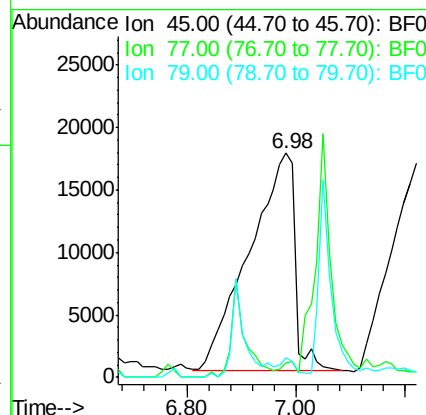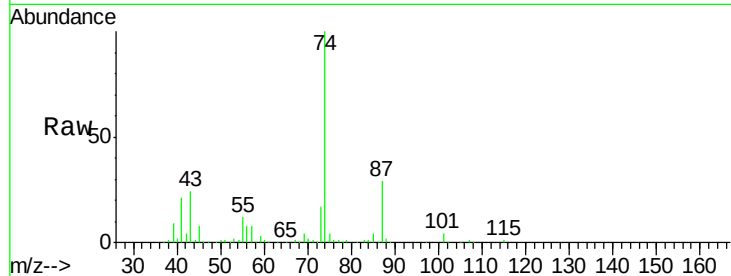

#17
2-Methylphenol
Concen: 193.04 ng
RT: 6.89 min Scan# 464
Delta R.T. -0.00 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59

Tgt Ion	Ratio	Lower	Upper
107	100		
108	110.9	90.9	136.3
77	40.4	36.6	55.0
79	41.2	36.5	54.7



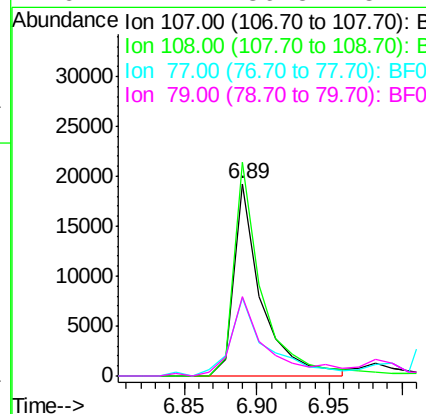



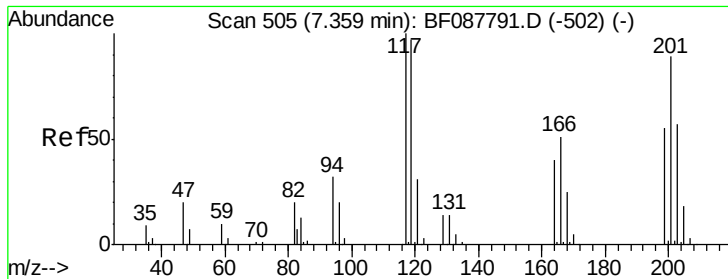

#18
Hexachloroethane
Concen: 5.54 ng
RT: 7.06 min Scan# 479
Delta R.T. -0.05 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59




Instrument :
BNA_F
ClientSampleId :
LF001MW001-160512DL


Tgt Ion: 117 Resp: 344
Ion Ratio Lower Upper
117 100
119 1095.0 77.4 116.2#
201 0.0 80.4 120.6#

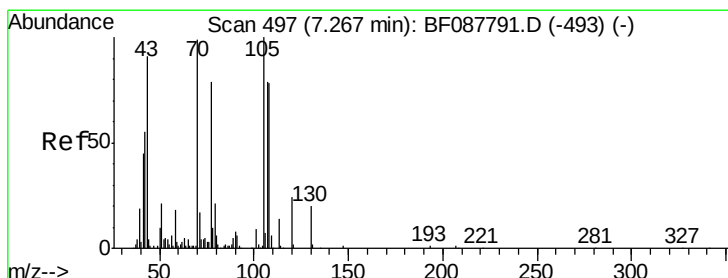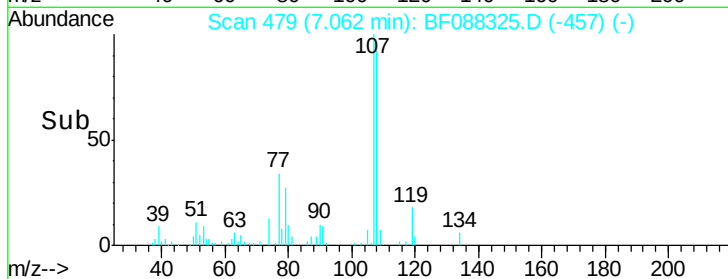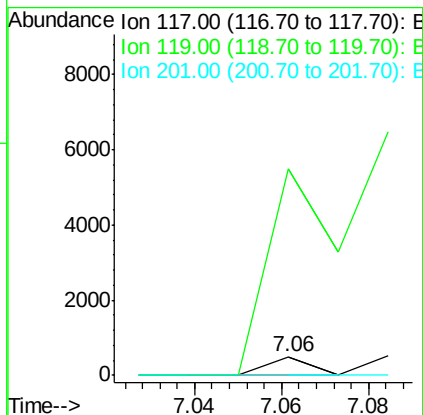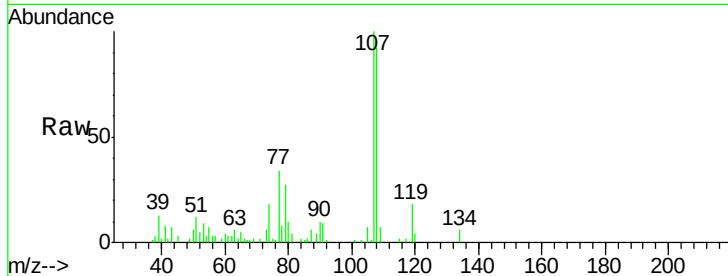

#19
n-Nitroso-di-n-propylamine
Concen: 223.42 ng
RT: 6.99 min Scan# 473
Delta R.T. -0.05 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59

Tgt Ion: 70 Resp: 23710
Ion Ratio Lower Upper
70 100
42 208.6 49.6 74.4#
101 254.7 7.1 10.7#
130 0.0 15.4 23.2#

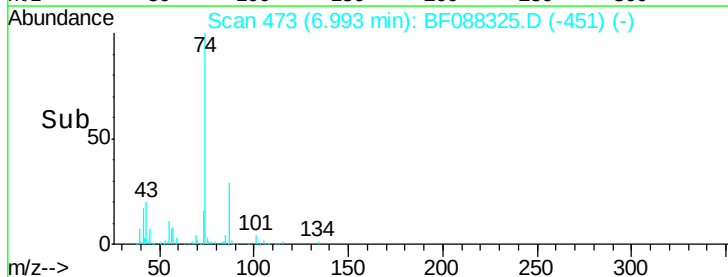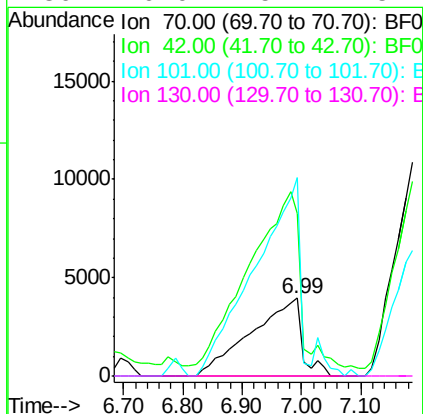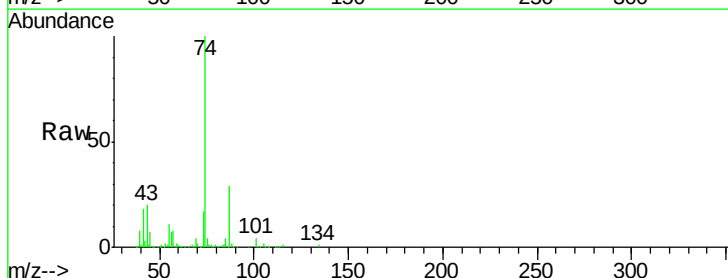




#20
3+4-Methylphenols
Concen: 663.61 ng
RT: 7.05 min Scan# 478
Delta R.T. -0.00 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59

Instrument :
BNA_F
ClientSampleId :
LF001MW001-160512DL

Tgt Ion	Ratio	Lower	Upper
107	100		
108	86.4	67.8	107.8
77	29.5	59.3	99.3#
79	23.9	7.0	47.0

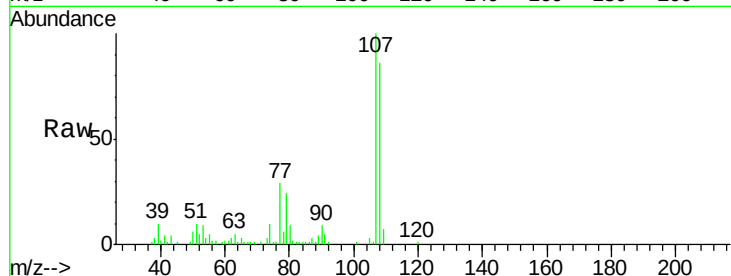




Abundance

Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BF0

Ion 79.00 (78.70 to 79.70): BF0

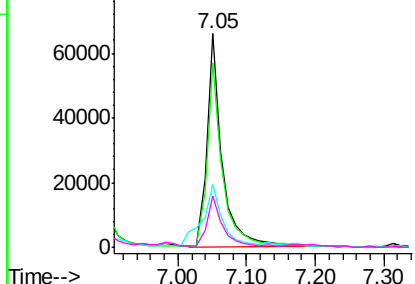

#21
Naphthalene-d8
Concen: 5.00 ng
RT: 7.88 min Scan# 551
Delta R.T. -0.01 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59

Tgt Ion	Ratio	Lower	Upper
136	100		
137	10.4	9.1	13.7
54	5.5	6.6	10.0#
68	4.6	5.1	7.7#




Abundance


Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

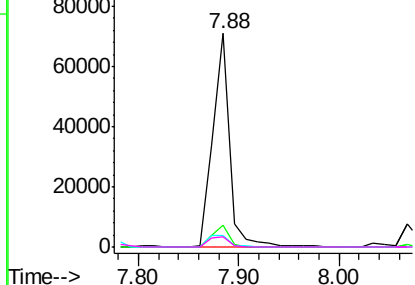



#22

Acetophenone

Concen: 2.93 ng

RT: 7.03 min Scan# 476

Delta R.T. -0.00 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59

Instrument :

BNA_F

ClientSampleId :

LF001MW001-160512DL

Tgt Ion: 105 Resp: 21456


Ion Ratio Lower Upper

105 100

71 98.4 5.3 7.9#

51 24.1 18.2 27.4

120 21.5 18.0 27.0






Abundance Ion 105.00 (104.70 to 105.70): E

Ion 71.00 (70.70 to 71.70): BF0

Ion 51.00 (50.70 to 51.70): BF0

Ion 120.00 (119.70 to 120.70): E

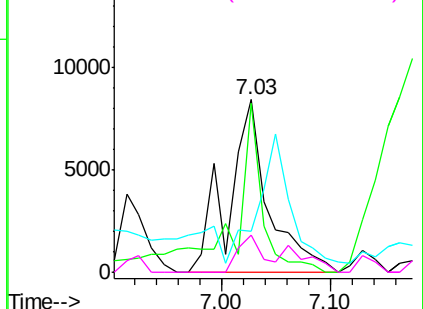

#23

Nitrobenzene-d5

Concen: 0.70 ng

RT: 7.18 min Scan# 489

Delta R.T. -0.00 min

Lab File: BF088325.D

Acq: 24 Jun 2016 9:59


Tgt Ion: 82 Resp: 3933

Ion Ratio Lower Upper

82 100

128 45.8 35.9 53.9



54 83.6 40.9 61.3#




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0




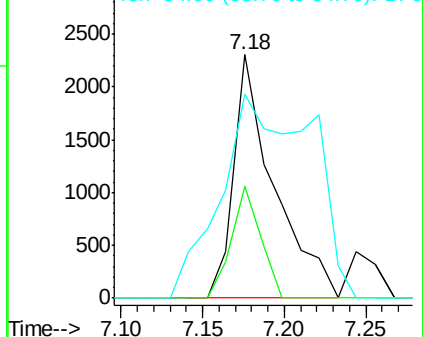


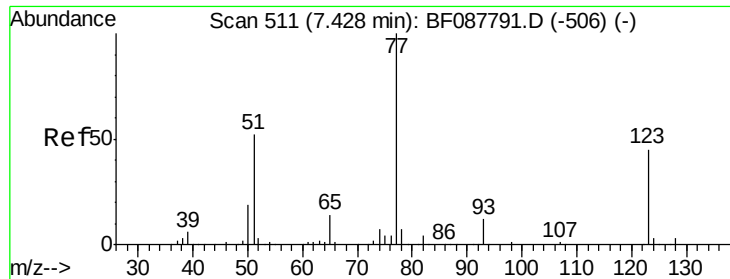

#24
 Nitrobenzene
 Concen: 7.00 ng
 RT: 7.05 min Scan# 478
 Delta R.T. -0.15 min
 Lab File: BF088325.D
 Acq: 24 Jun 2016 9:59




Instrument :
 BNA_F
 ClientSampleId :
 LF001MW001-160512DL


Tgt Ion: 77 Resp: 38074
 Ion Ratio Lower Upper
 77 100
 123 0.0 45.0 67.4#
 65 9.9 10.2 15.2#

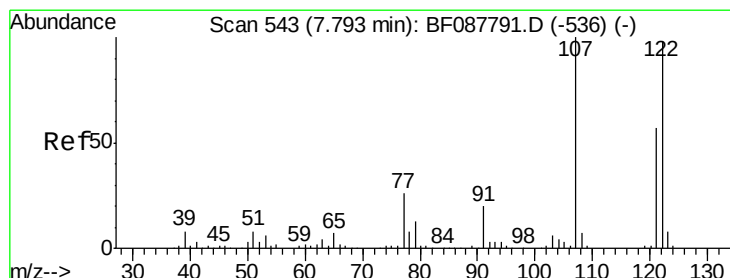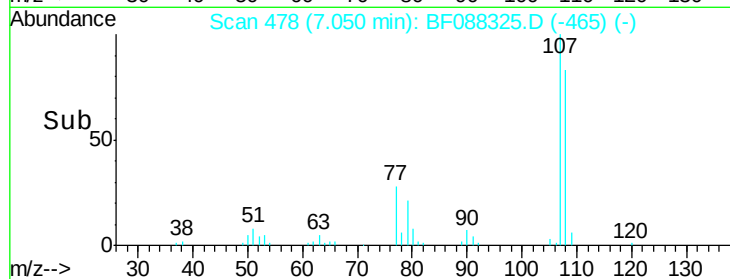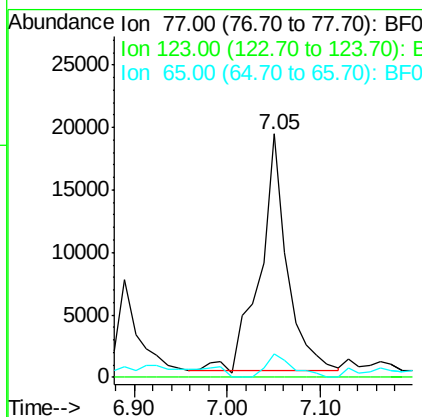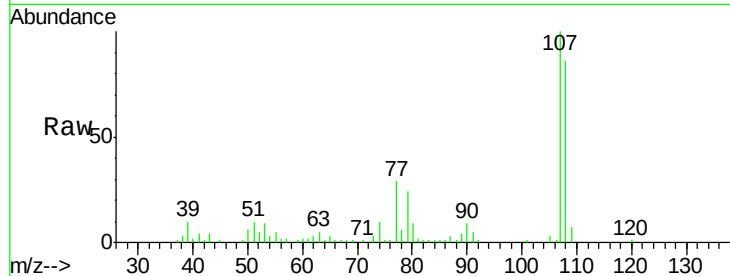

#27
 2,4-Dimethylphenol
 Concen: 4.05 ng
 RT: 7.59 min Scan# 525
 Delta R.T. 0.01 min
 Lab File: BF088325.D
 Acq: 24 Jun 2016 9:59

Tgt Ion: 122 Resp: 21733
 Ion Ratio Lower Upper
 122 100
 107 100.9 82.4 123.6
 121 45.6 46.3 69.5#

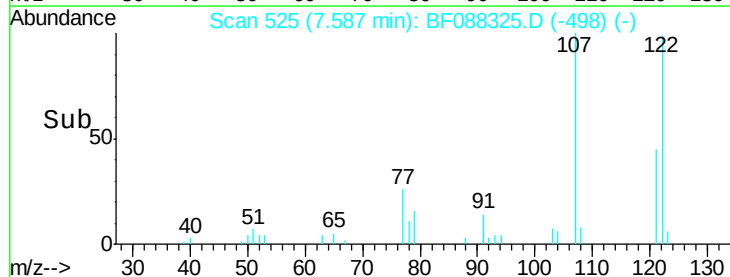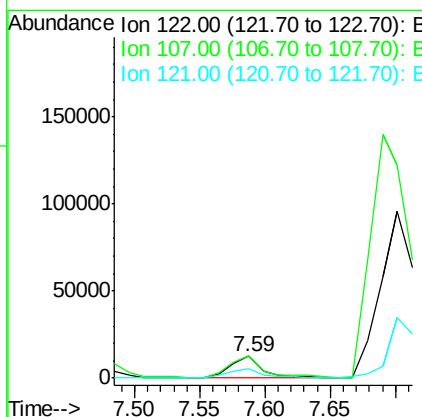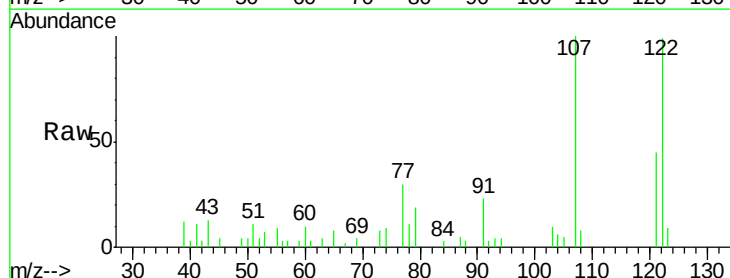







#31
Naphthalene
Concen: 10.38 ng
RT: 7.90 min Scan# 552
Delta R.T. -0.02 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59

Instrument :
BNA_F
ClientSampleId :
LF001MW001-160512DL

Tgt Ion:128 Resp: 168393
Ion Ratio Lower Upper
128 100
129 11.6 9.4 14.2
127 12.6 10.9 16.3

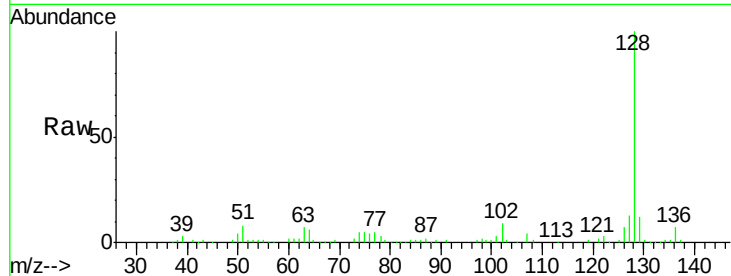


Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

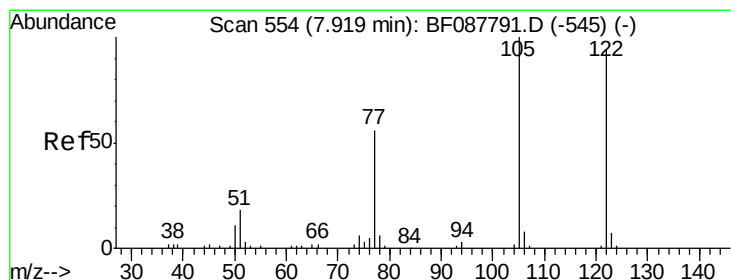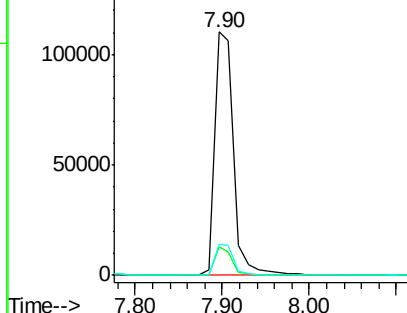




#32
Benzoic acid
Concen: 62.14 ng
RT: 7.70 min Scan# 535
Delta R.T. -0.02 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59

Tgt Ion:122 Resp: 183521
Ion Ratio Lower Upper
122 100
105 3.4 101.6 141.6#
77 36.4 70.6 110.6#



Abundance Ion 122.00 (121.70 to 122.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 77.00 (76.70 to 77.70): BF0

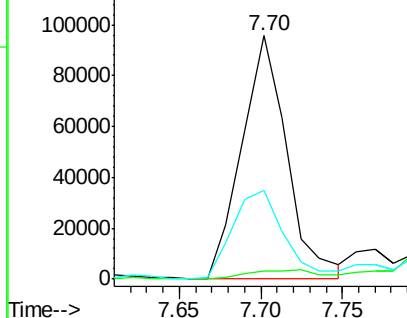







#33
4-Chloroaniline
Concen: 2.94 ng
RT: 7.90 min Scan# 552
Delta R.T. -0.08 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59

Instrument :
BNA_F
ClientSampleId :
LF001MW001-160512DL

Tgt Ion:127 Resp: 21304
Ion Ratio Lower Upper
127 100
129 91.8 26.3 39.5#
65 5.1 24.7 37.1#
92 0.0 15.4 23.0#




Abundance Ion 127.00 (126.70 to 127.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 65.00 (64.70 to 65.70): BF0
Ion 92.00 (91.70 to 92.70): BF0

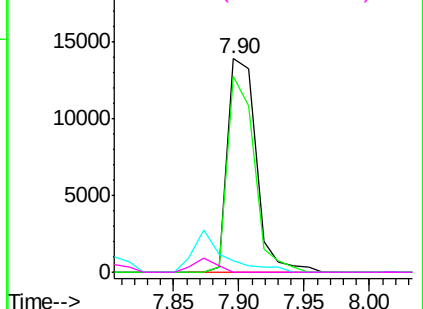




#38
Acenaphthene-d10
Concen: 5.00 ng
RT: 9.62 min Scan# 703
Delta R.T. -0.02 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59

Tgt Ion:164 Resp: 40584
Ion Ratio Lower Upper
164 100
162 105.1 85.4 128.2
160 45.4 39.5 59.3



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

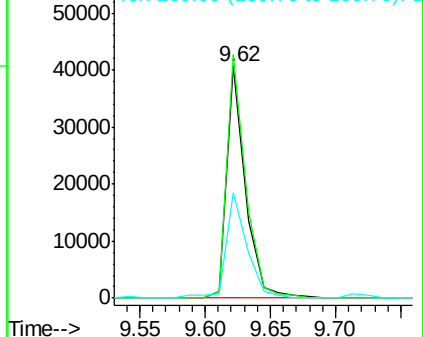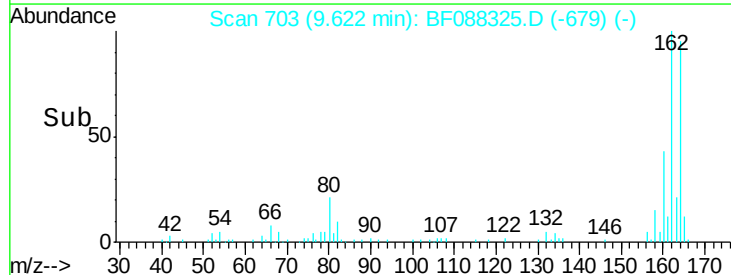







#41
 2,4,6-Tribromophenol
 Concen: 0.44 ng
 RT: 10.42 min Scan# 773
 Delta R.T. -0.01 min
 Lab File: BF088325.D
 Acq: 24 Jun 2016 9:59

Instrument :
 BNA_F
 ClientSampleId :
 LF001MW001-160512DL

Tgt Ion	Ratio	Lower	Upper
330	100		
332	133.4	0.0	0.0#
141	35.5	0.0	0.0#

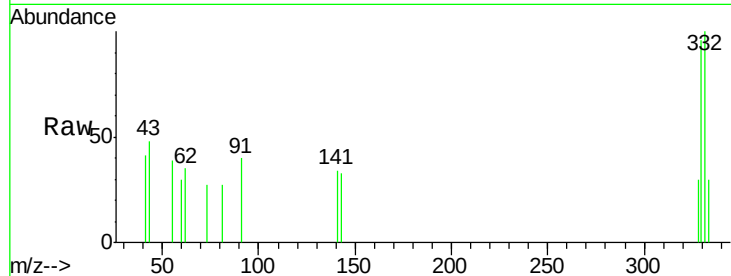


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

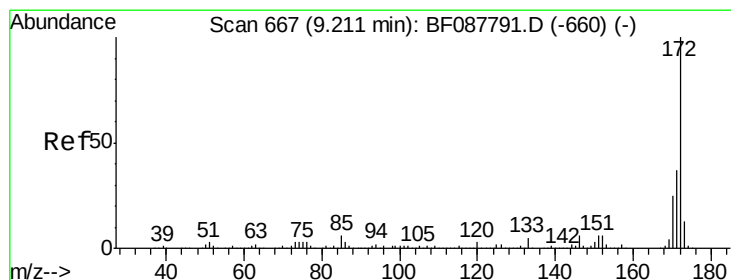
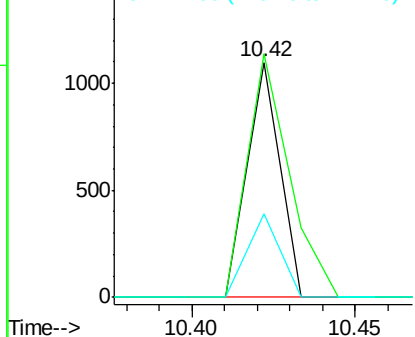



#44
 2-Fluorobiphenyl
 Concen: -0.84 ng
 RT: 8.96 min Scan# 645
 Delta R.T. -0.01 min
 Lab File: BF088325.D
 Acq: 24 Jun 2016 9:59

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.2	28.6	43.0
170	23.7	19.2	28.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

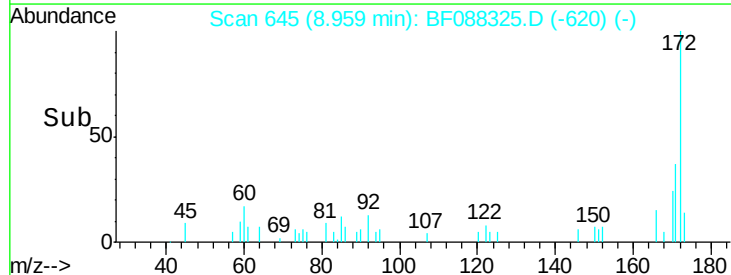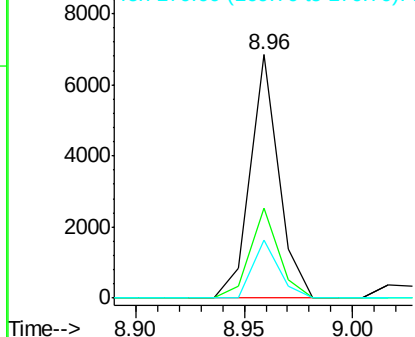







#63
Phenanthrene-d10
Concen: 5.00 ng
RT: 11.10 min Scan# 832
Delta R.T. -0.02 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59

Instrument :
BNA_F
ClientSampleId :
LF001MW001-160512DL

Tgt Ion:188 Resp: 61675
Ion Ratio Lower Upper
188 100
94 13.5 9.0 13.6
80 13.8 10.0 15.0

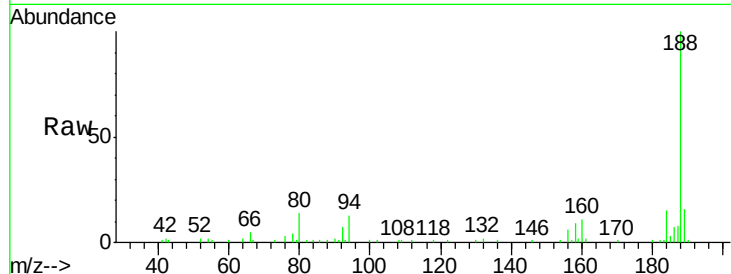


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


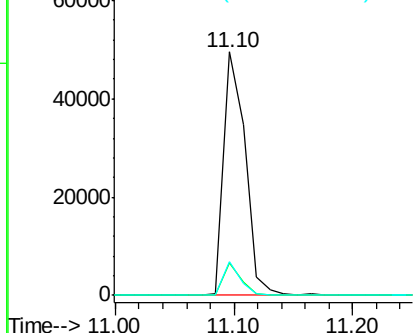



#75
Chrysene-d12
Concen: 5.00 ng
RT: 13.73 min Scan# 1062
Delta R.T. -0.02 min
Lab File: BF088325.D
Acq: 24 Jun 2016 9:59

Tgt Ion:240 Resp: 45947
Ion Ratio Lower Upper
240 100
120 11.2 6.8 10.2#
236 25.5 20.2 30.2



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

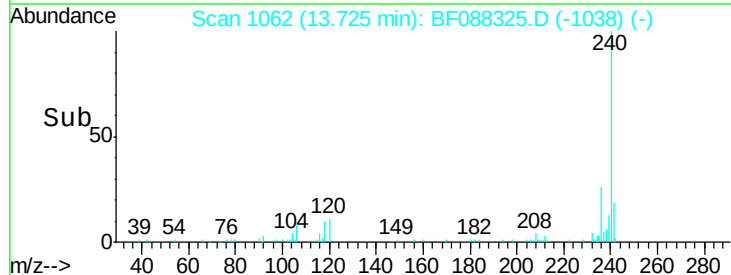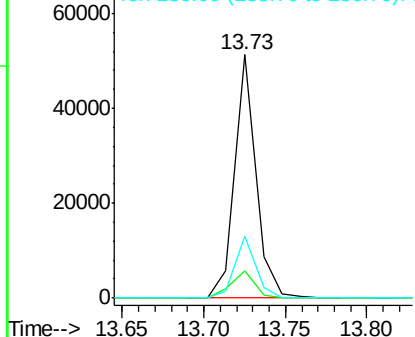







#78
 Terphenyl-d14
 Concen: 0.61 ng
 RT: 12.67 min Scan# 970
 Delta R.T. -0.02 min
 Lab File: BF088325.D
 Acq: 24 Jun 2016 9:59

Instrument :
 BNA_F
 ClientSampleId :
 LF001MW001-160512DL

Tgt Ion: 244 Resp: 4925
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.0 9.0
 122 19.2 11.2 16.8#




Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

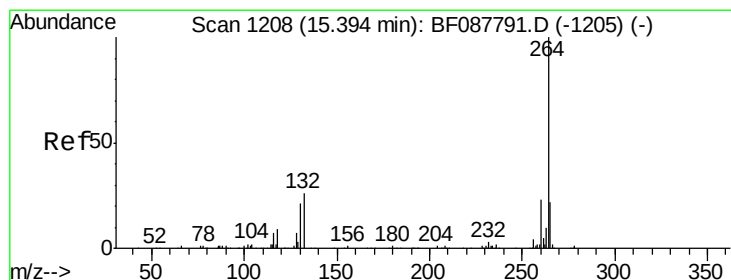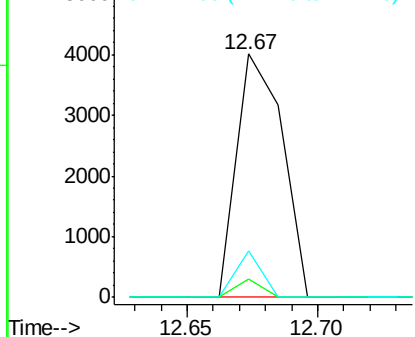

#86
 Perylene-d12
 Concen: 5.00 ng
 RT: 15.09 min Scan# 1181
 Delta R.T. -0.02 min
 Lab File: BF088325.D
 Acq: 24 Jun 2016 9:59

Tgt Ion: 264 Resp: 40536
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.2 28.8
 265 21.8 16.9 25.3

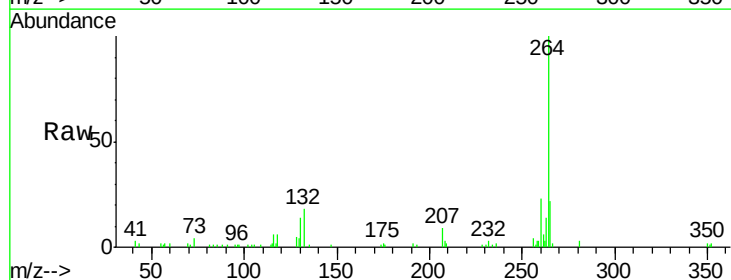

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

