
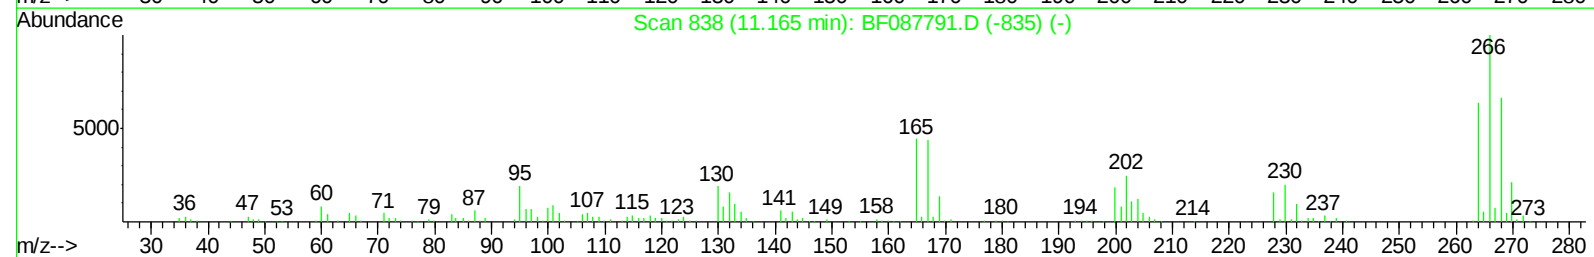
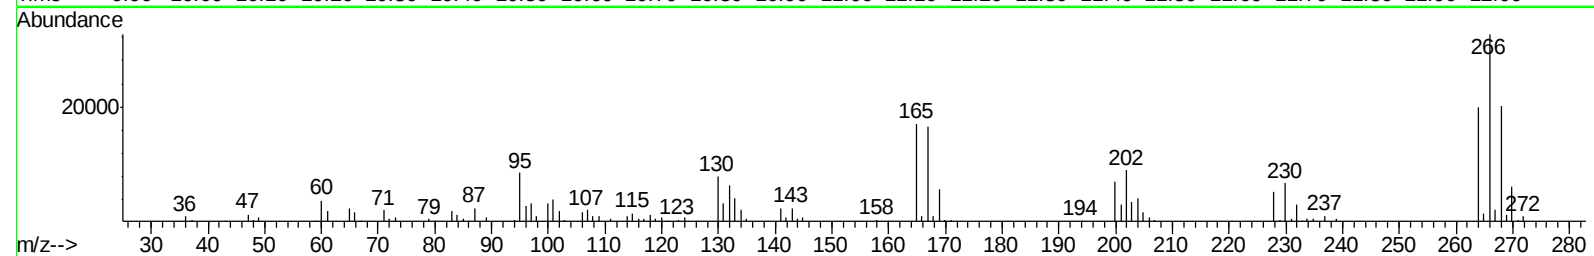


Data Path : Z:\HPCHEM1\BNA F\Data\BF062316\
Data File : BF088294.D
Acq On : 23 Jun 2016 16:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:15:33 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

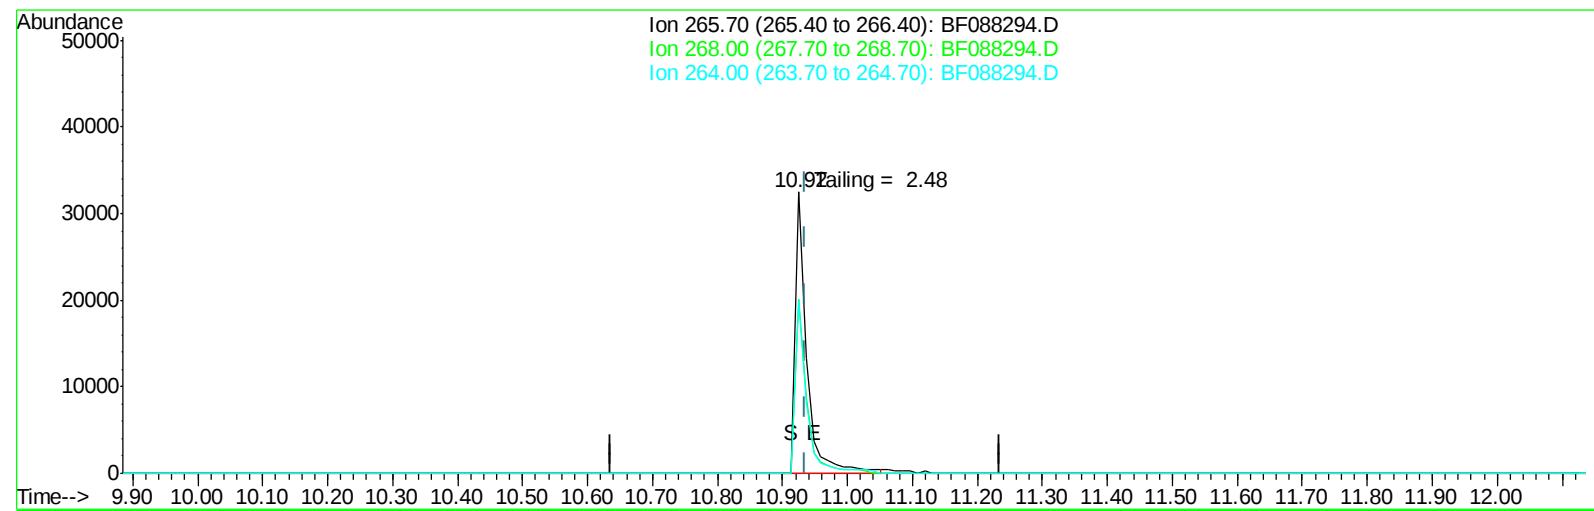

TIC: BF088294.D

(69) Pentachlorophenol (C)




10.925min (-0.011) 8030.28ng

response 40437

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	62.06
264.00	62.00	61.27
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF062316\
Data File : BF088294.D
Acq On : 23 Jun 2016 16:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:15:33 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

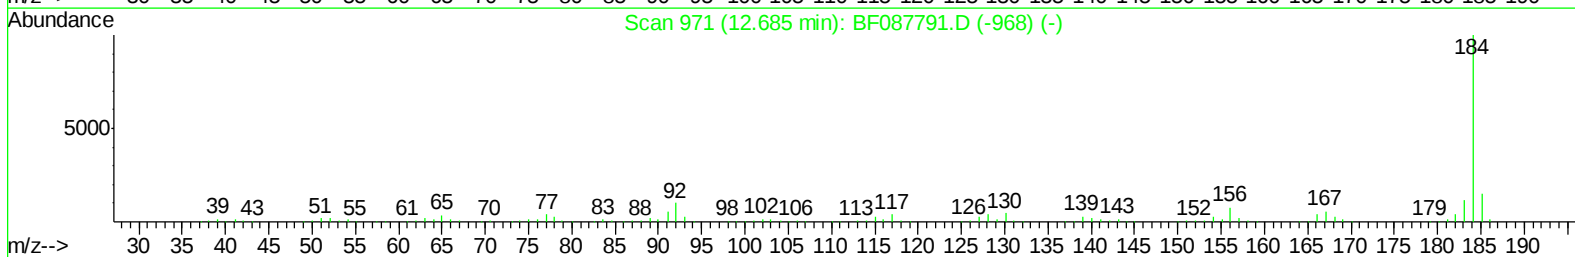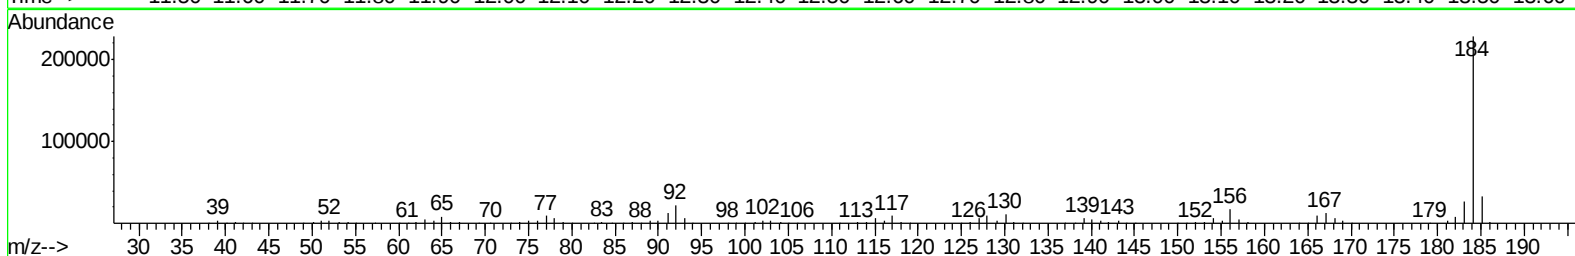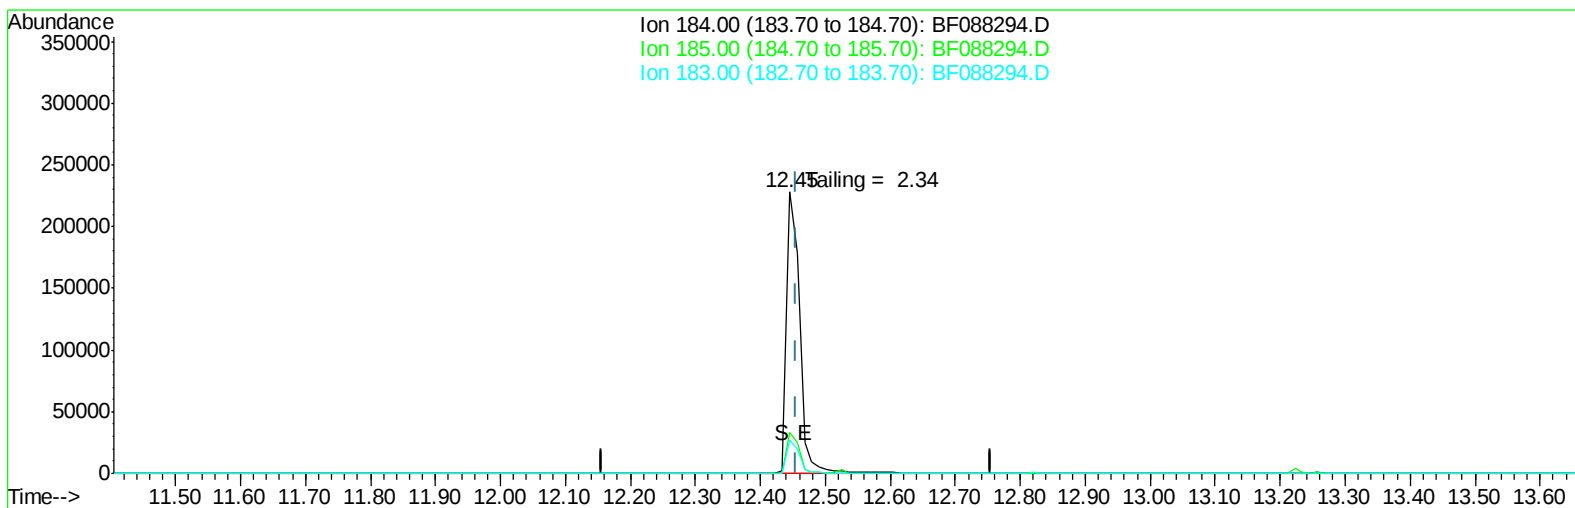

TIC: BF088294.D

(76) Benzidine

12.445min (-0.011) 2317.07ng

response 317900

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.47
183.00	11.60	11.68
0.00	0.00	0.00