
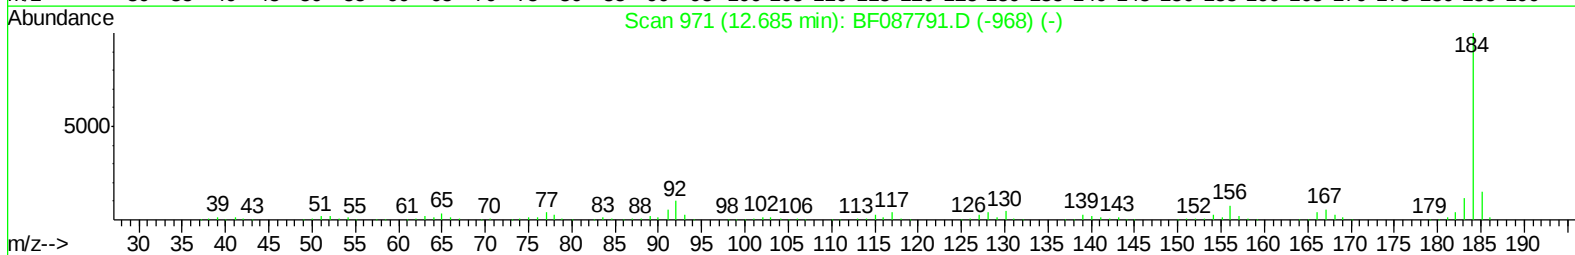
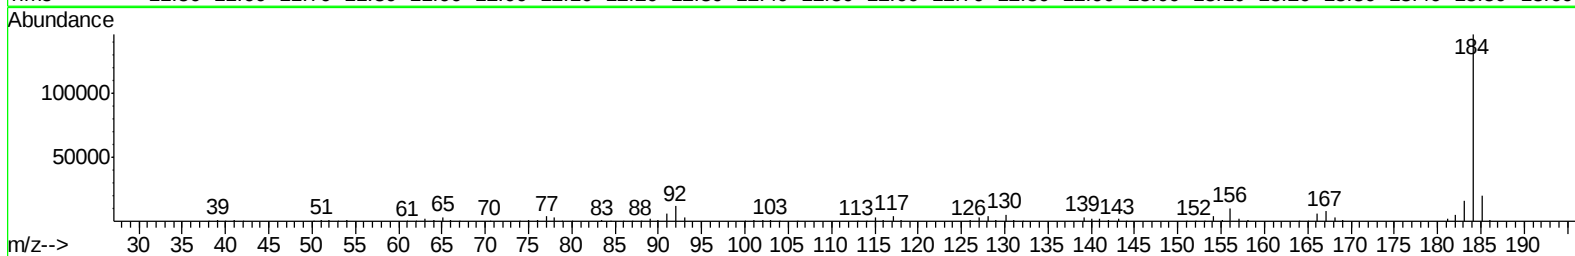


Data Path : Z:\HPCHEM1\BNA F\Data\BF062316\
Data File : BF088314.D
Acq On : 24 Jun 2016 4:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:16:54 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

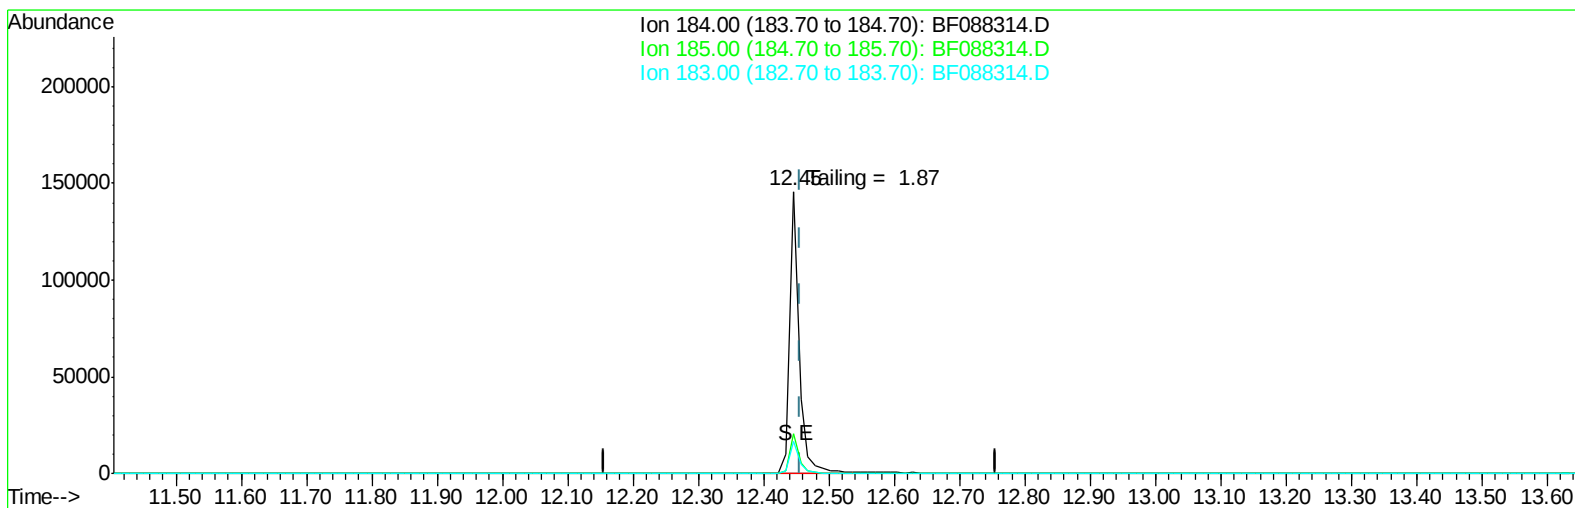

TIC: BF088314.D

(76) Benzidine




12.445min (-0.011) 5347.10ng

response 148500

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.20
183.00	11.60	11.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF062316\
Data File : BF088314.D
Acq On : 24 Jun 2016 4:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:16:54 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

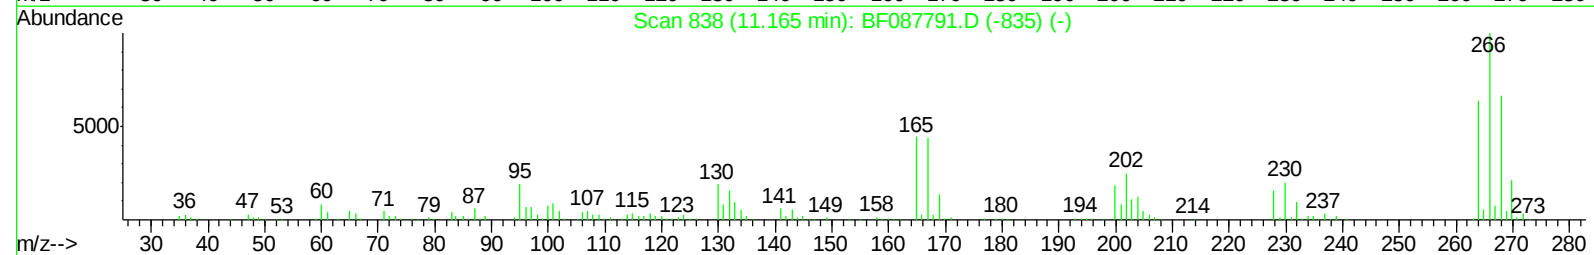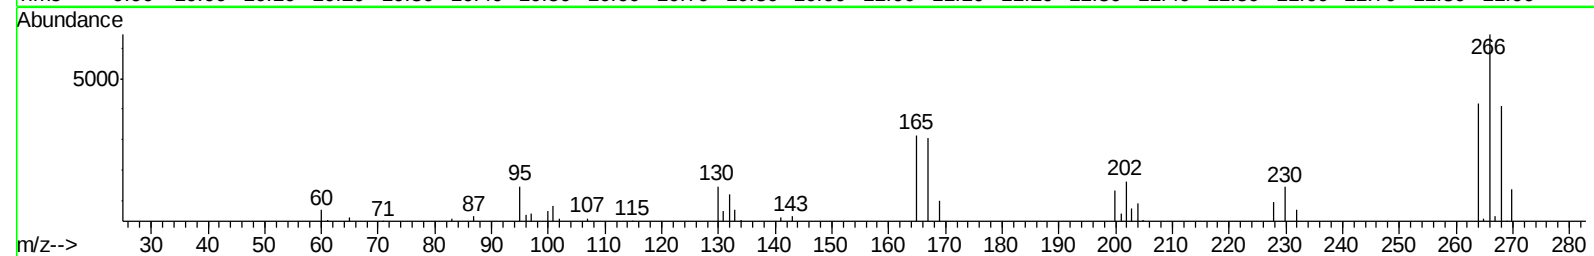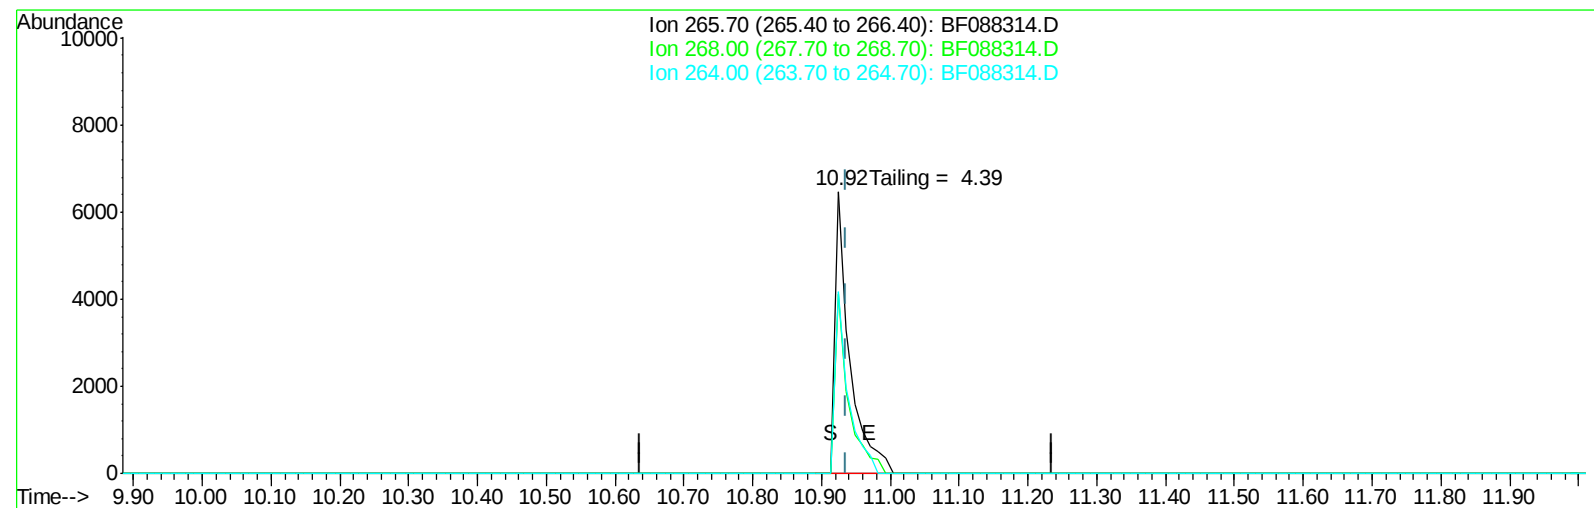

TIC: BF088314.D

(69) Pentachlorophenol (C)

10.925min (-0.011) 0.00ng

response 9453

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	63.80
264.00	62.00	64.76
0.00	0.00	0.00