

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062316\
 Data File : BF088303.D
 Acq On : 23 Jun 2016 22:12
 Operator : UM/SJ
 Sample : H3607-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TE-MW2-15

Quant Time: Jun 24 02:18:17 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 22 14:55:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.59	152	93865	20.00	ng	-0.01
21) Naphthalene-d8	7.88	136	360727	20.00	ng	-0.01
38) Acenaphthene-d10	9.62	164	160634	20.00	ng	-0.02
63) Phenanthrene-d10	11.11	188	286894	20.00	ng	-0.01
75) Chrysene-d12	13.73	240	185725	20.00	ng	-0.02
86) Perylene-d12	15.09	264	158729	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	346798	63.16	ng	0.01
7) Phenol-d6	6.26	99	290360	43.64	ng	0.00
23) Nitrobenzene-d5	7.18	82	539218	87.29	ng	0.00
41) 2,4,6-Tribromophenol	10.42	330	191634	112.98	ng	-0.01
44) 2-Fluorobiphenyl	8.96	172	912965	89.58	ng	-0.01
78) Terphenyl-d14	12.69	244	664493	81.42	ng	-0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062316\
Data File : BF088303.D
Acq On : 23 Jun 2016 22:12
Operator : UM/SJ
Sample : H3607-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TE-MW2-15

Quant Time: Jun 24 02:18:17 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration




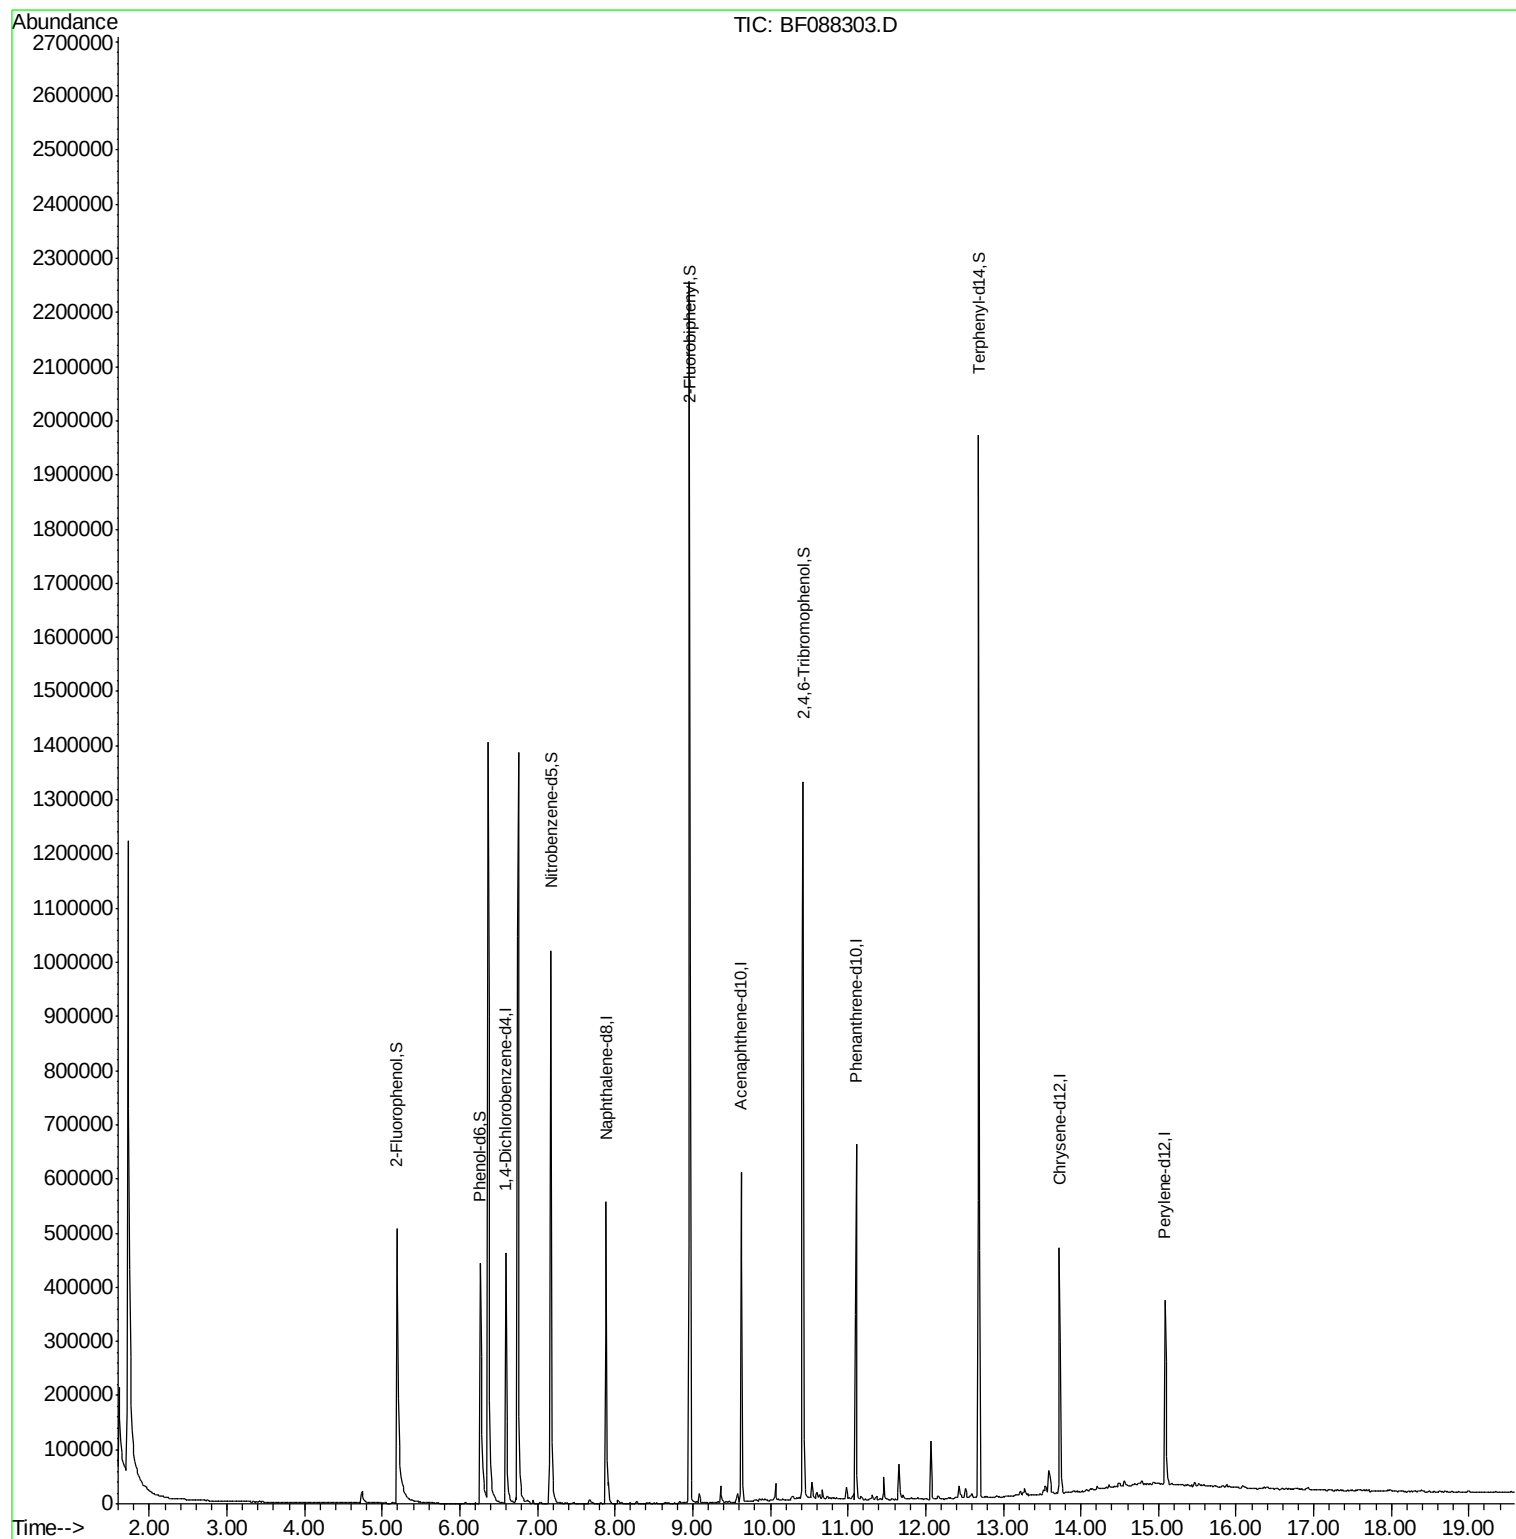


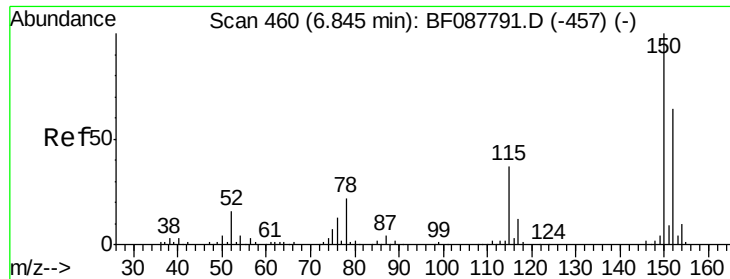

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.59 min Scan# 438
 Delta R.T. -0.01 min
 Lab File: BF088303.D
 Acq: 23 Jun 2016 22:12




Instrument :
 BNA_F
 ClientSampleId :
 TE-MW2-15


Tgt Ion:152 Resp: 93865
 Ion Ratio Lower Upper
 152 100
 150 151.6 123.8 185.6
 115 58.8 39.6 59.4

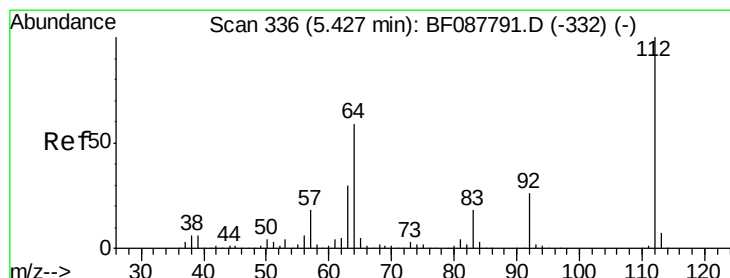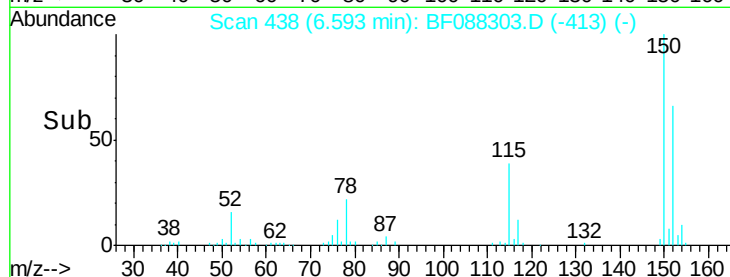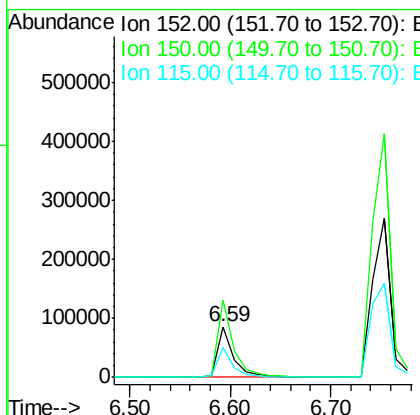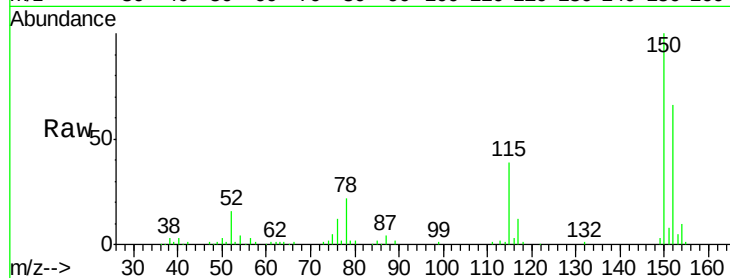

#5
 2-Fluorophenol
 Concen: 63.16 ng
 RT: 5.19 min Scan# 315
 Delta R.T. 0.01 min
 Lab File: BF088303.D
 Acq: 23 Jun 2016 22:12

Tgt Ion:112 Resp: 346798
 Ion Ratio Lower Upper
 112 100
 64 58.9 42.2 63.2
 63 29.5 21.8 32.8

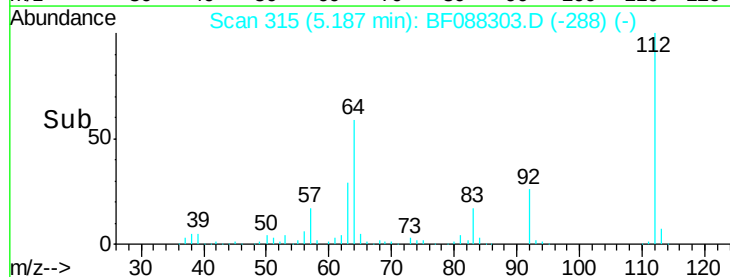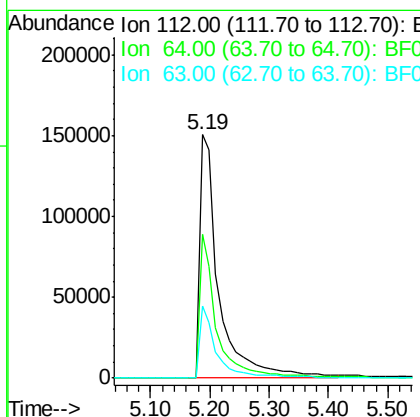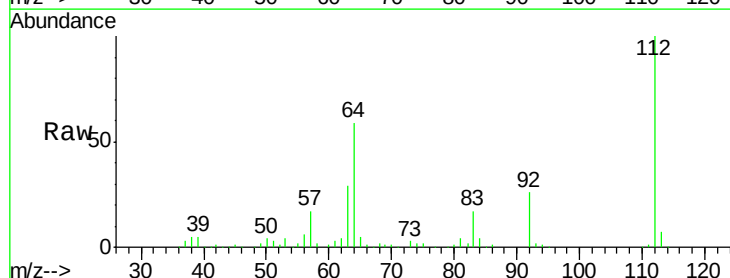

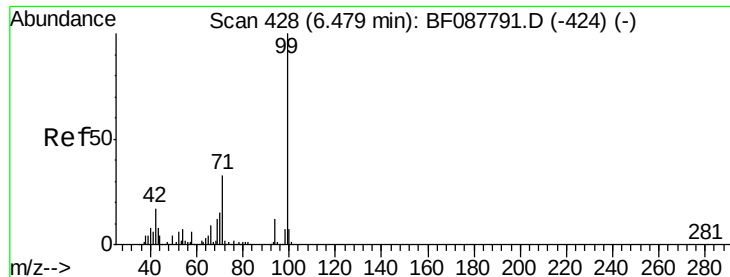

#7

Phenol-d6

Concen: 43.64 ng

RT: 6.26 min Scan# 409

Delta R.T. 0.00 min

Lab File: BF088303.D

Acq: 23 Jun 2016 22:12

Instrument :

BNA_F

ClientSampleId :

TE-MW2-15


Tgt Ion: 99 Resp: 290360

Ion Ratio Lower Upper

99 100

42 15.0 12.2 18.2




71 31.9 23.4 35.0

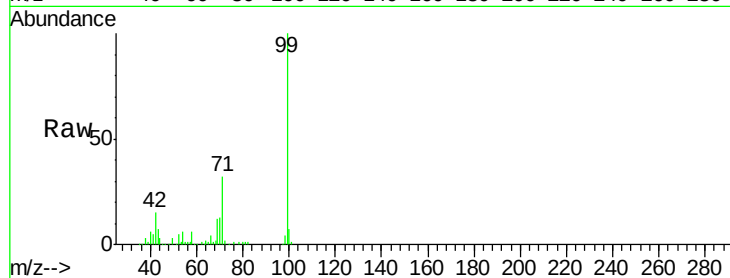

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

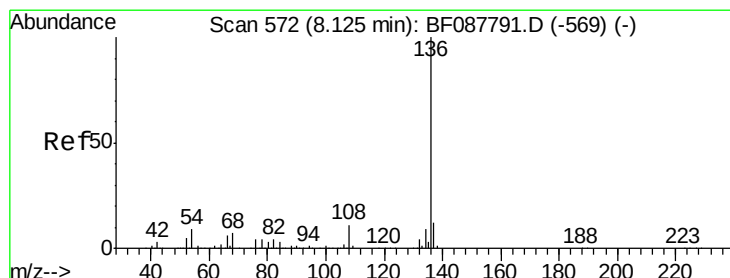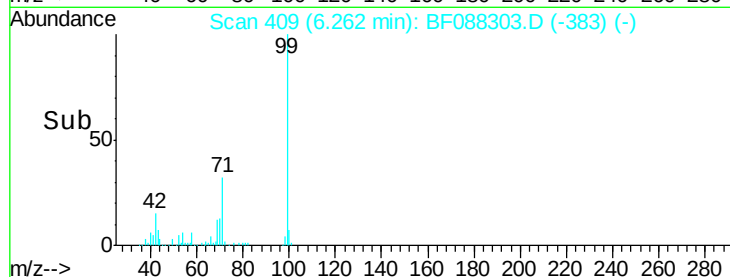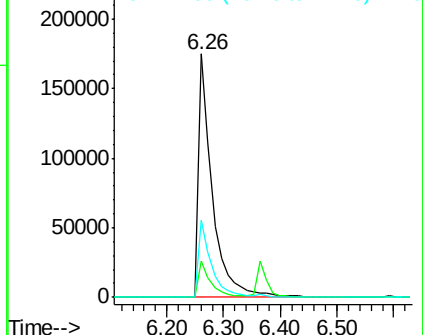

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.88 min Scan# 551

Delta R.T. -0.01 min

Lab File: BF088303.D

Acq: 23 Jun 2016 22:12

Tgt Ion: 136 Resp: 360727


Ion Ratio Lower Upper

136 100

137 10.7 9.1 13.7

54 5.2 6.6 10.0#

68 4.6 5.1 7.7#


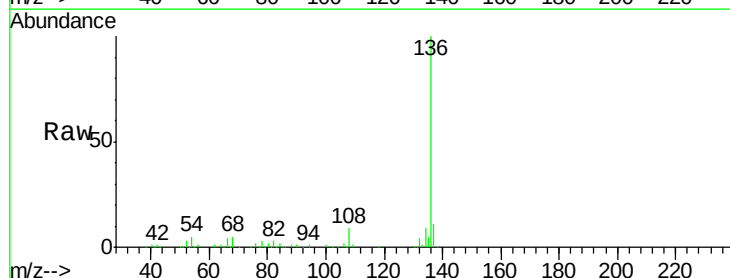



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



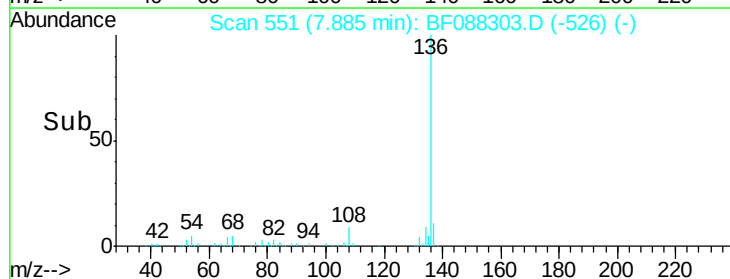
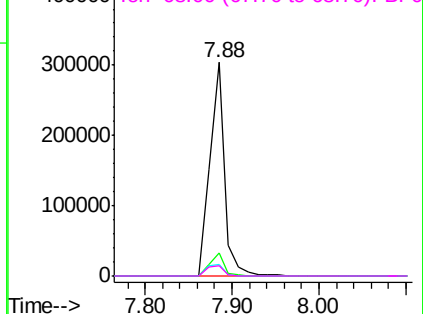


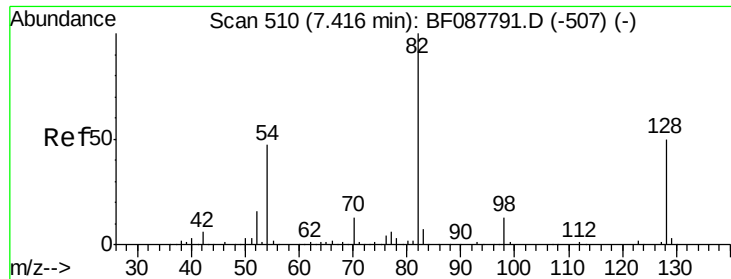

#23
 Nitrobenzene-d5
 Concen: 87.29 ng
 RT: 7.18 min Scan# 489
 Delta R.T. 0.00 min
 Lab File: BF088303.D
 Acq: 23 Jun 2016 22:12




Instrument :
 BNA_F
 ClientSampleId :
 TE-MW2-15


Tgt Ion: 82 Resp: 539218
 Ion Ratio Lower Upper
 82 100
 128 56.1 35.9 53.9#
 54 41.0 40.9 61.3

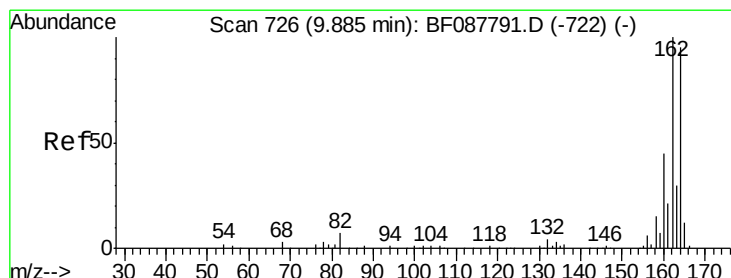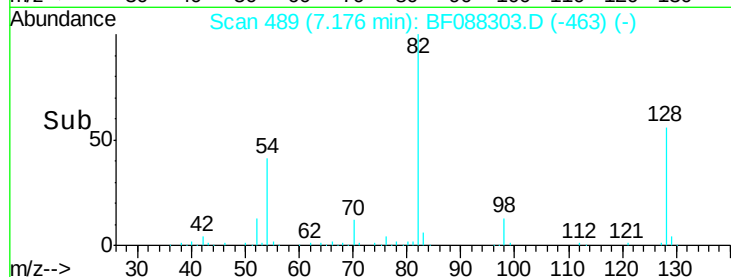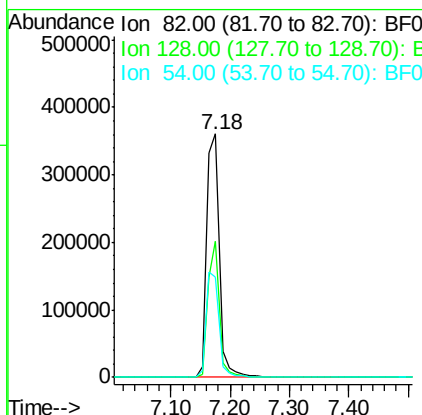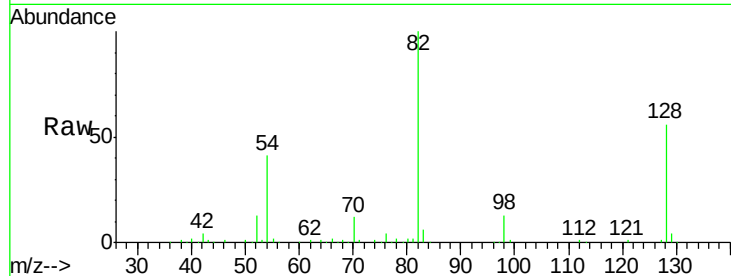

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.62 min Scan# 703
 Delta R.T. -0.02 min
 Lab File: BF088303.D
 Acq: 23 Jun 2016 22:12

Tgt Ion: 164 Resp: 160634
 Ion Ratio Lower Upper
 164 100
 162 104.9 85.4 128.2
 160 45.7 39.5 59.3


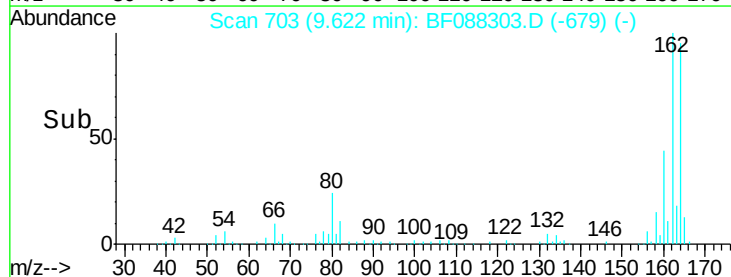
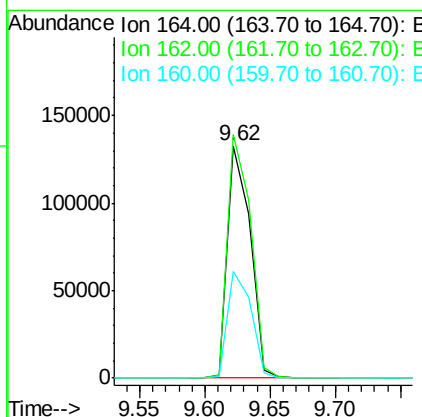
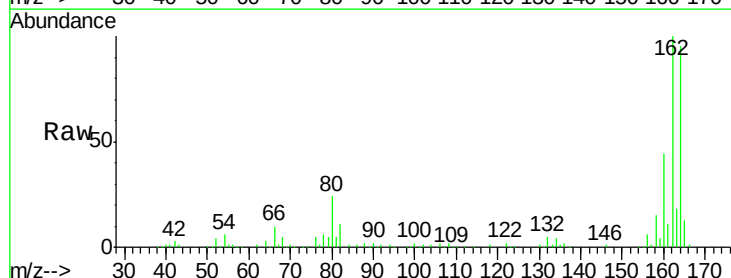


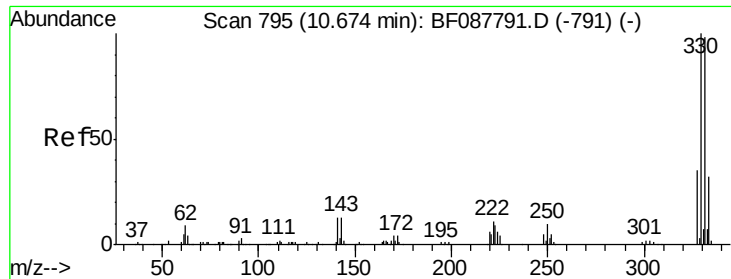

#41
 2,4,6-Tribromophenol
 Concen: 112.98 ng
 RT: 10.42 min Scan# 773
 Delta R.T. -0.01 min
 Lab File: BF088303.D
 Acq: 23 Jun 2016 22:12




Instrument :
 BNA_F
 ClientSampleId :
 TE-MW2-15


Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.2	0.0	0.0#
141	40.0	0.0	0.0#

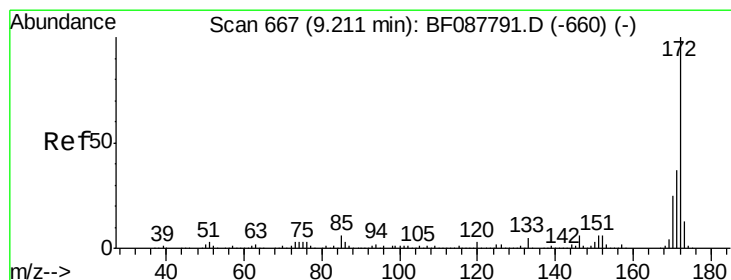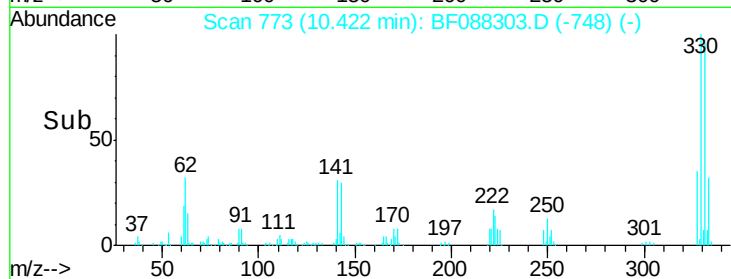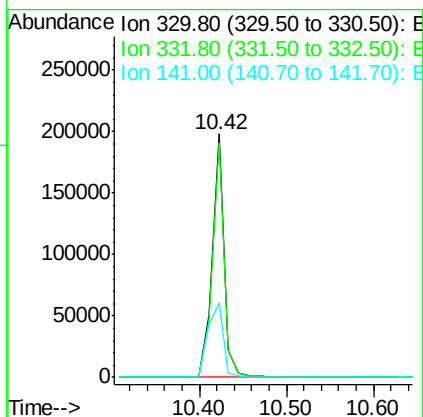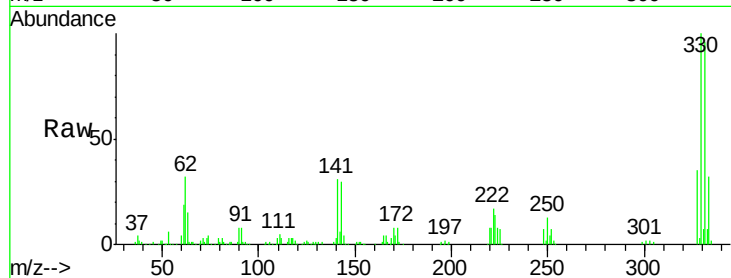

#44
 2-Fluorobiphenyl
 Concen: 89.58 ng
 RT: 8.96 min Scan# 645
 Delta R.T. -0.01 min
 Lab File: BF088303.D
 Acq: 23 Jun 2016 22:12

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.9	28.6	43.0
170	24.2	19.2	28.8

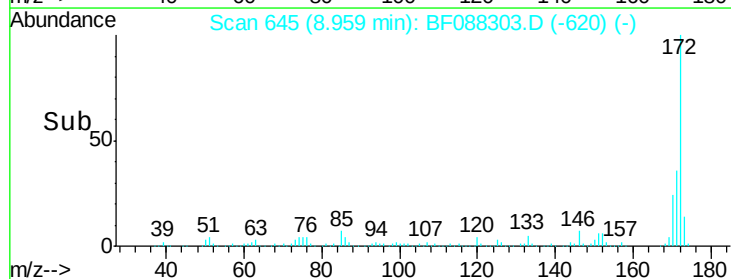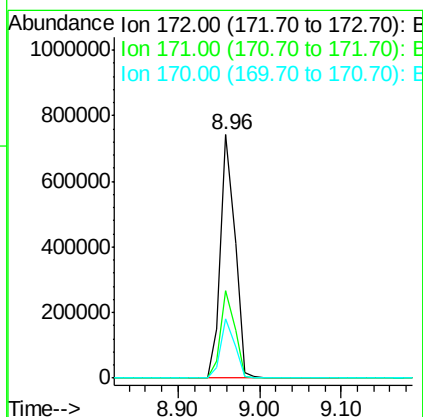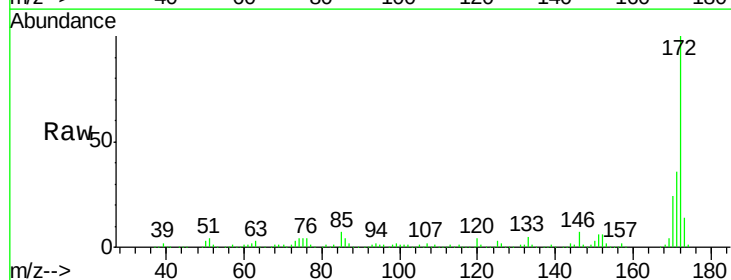


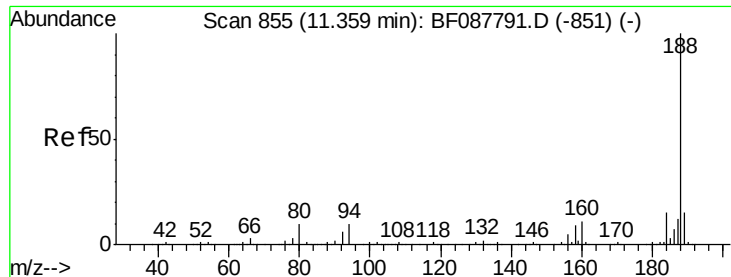




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.11 min Scan# 833
Delta R.T. -0.01 min
Lab File: BF088303.D
Acq: 23 Jun 2016 22:12

Instrument :
BNA_F
ClientSampleId :
TE-MW2-15

Tgt Ion:188 Resp: 286894
Ion Ratio Lower Upper
188 100
94 7.6 9.0 13.6#
80 7.4 10.0 15.0#

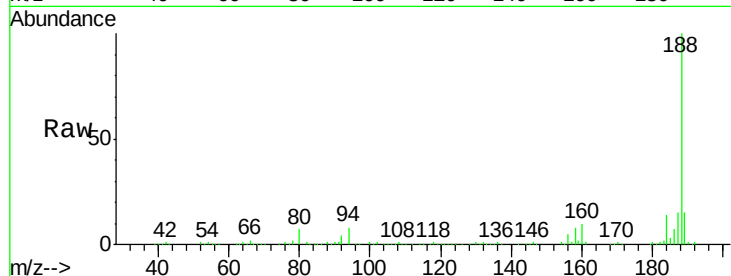


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

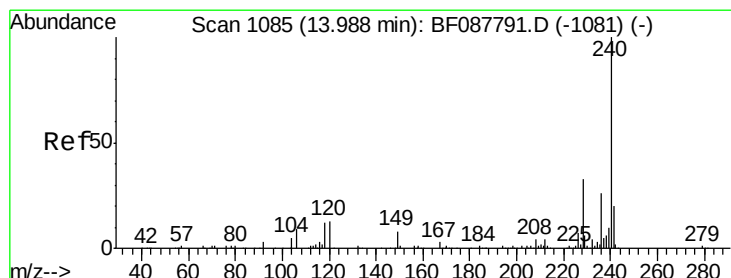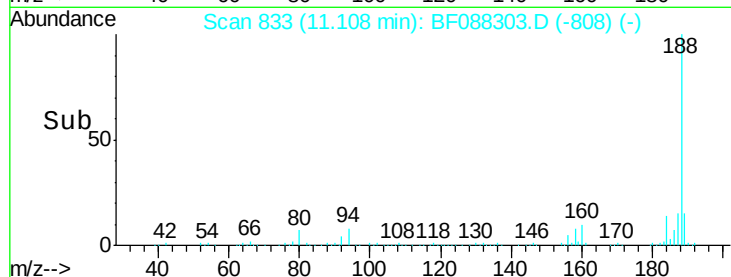
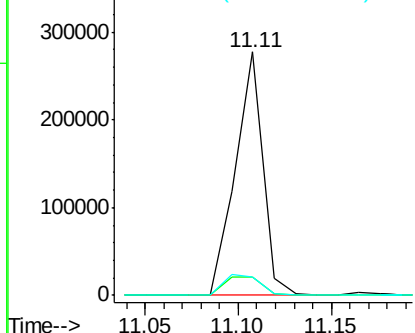



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.73 min Scan# 1062
Delta R.T. -0.02 min
Lab File: BF088303.D
Acq: 23 Jun 2016 22:12

Tgt Ion:240 Resp: 185725
Ion Ratio Lower Upper
240 100
120 17.7 6.8 10.2#
236 24.7 20.2 30.2

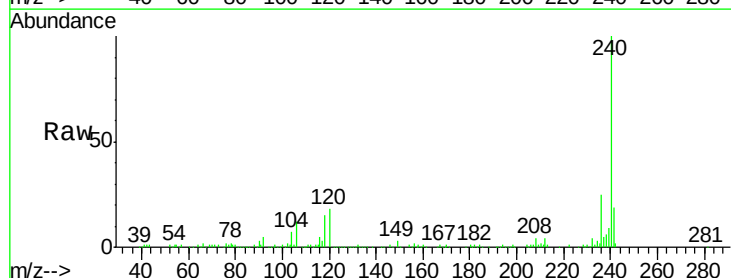

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

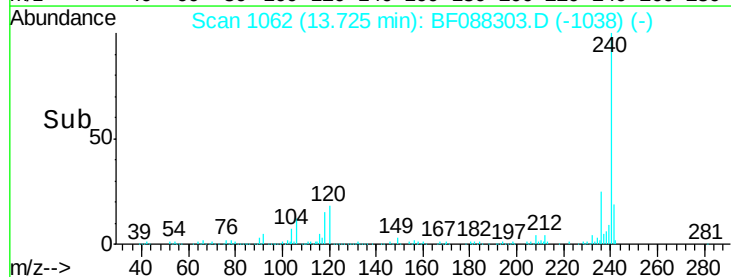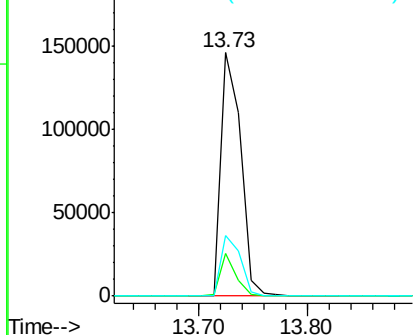


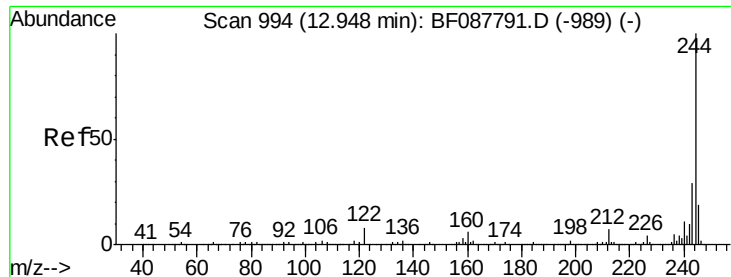




#78
 Terphenyl-d14
 Concen: 81.42 ng
 RT: 12.69 min Scan# 971
 Delta R.T. -0.01 min
 Lab File: BF088303.D
 Acq: 23 Jun 2016 22:12

Instrument :
 BNA_F
 ClientSampleId :
 TE-MW2-15

Tgt Ion:244 Resp: 664493
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.0 9.0
 122 14.2 11.2 16.8

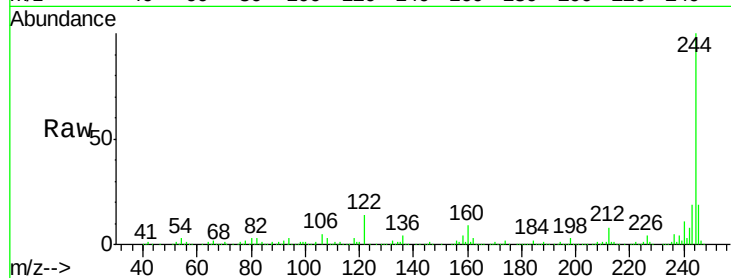


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

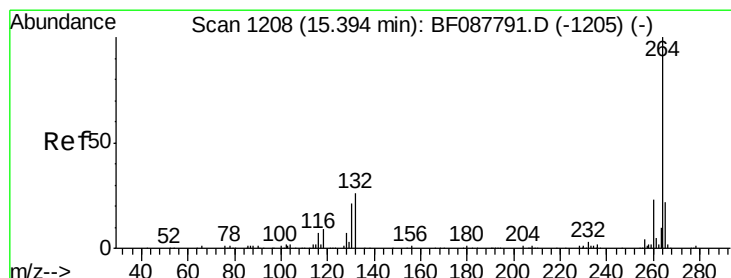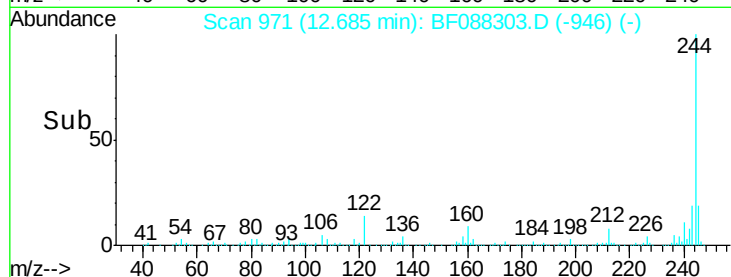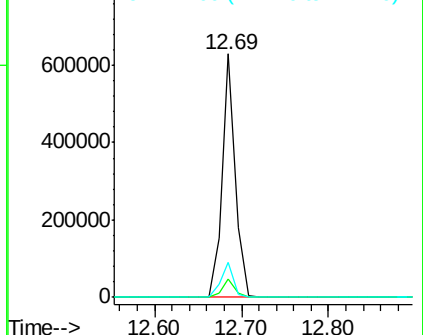

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.09 min Scan# 1181
 Delta R.T. -0.02 min
 Lab File: BF088303.D
 Acq: 23 Jun 2016 22:12

Tgt Ion:264 Resp: 158729
 Ion Ratio Lower Upper
 264 100
 260 23.1 19.2 28.8
 265 21.9 16.9 25.3

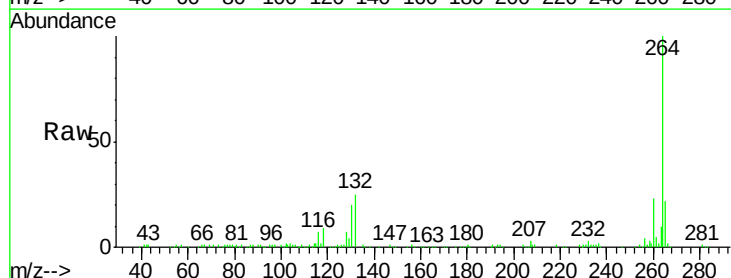

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

