

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062316\
 Data File : BF088304.D
 Acq On : 23 Jun 2016 22:40
 Operator : UM/SJ
 Sample : H3607-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TE-PMW-43

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.724	10	12	46	rVB	1284608	2720982	100.00%	14.263%
2	4.730	273	275	283	rBV	19785	35967	1.32%	0.189%
3	5.187	313	315	340	rBV	522614	942329	34.63%	4.940%
4	6.262	408	409	416	rBV	387688	606028	22.27%	3.177%
5	6.365	416	418	436	rVB	1374436	1720382	63.23%	9.018%
6	6.593	436	438	445	rBV	411699	449337	16.51%	2.355%
7	6.753	450	452	454	rBV	1228941	1633957	60.05%	8.565%
8	7.165	486	488	491	rBV	897794	1298580	47.72%	6.807%
9	7.885	548	551	561	rBV	511987	625631	22.99%	3.279%
10	8.959	642	645	648	rBV	2264131	2475669	90.98%	12.977%
11	9.279	671	673	678	rVB	27726	28215	1.04%	0.148%
12	9.622	701	703	706	rBV	603561	723655	26.60%	3.793%
13	10.068	737	742	744	rBV2	20322	27872	1.02%	0.146%
14	10.422	770	773	775	rBV	1281567	1514211	55.65%	7.937%
15	11.108	831	833	835	rBV	676335	723985	26.61%	3.795%
16	12.068	915	917	921	rBV2	49513	48152	1.77%	0.252%
17	12.685	968	971	974	rBV	2091136	2142069	78.72%	11.228%
18	13.542	1045	1046	1049	rVV	36904	39505	1.45%	0.207%
19	13.600	1049	1051	1054	rVB2	17937	31303	1.15%	0.164%
20	13.725	1060	1062	1065	rBV	609032	640024	23.52%	3.355%
21	15.085	1179	1181	1188	rBV	403596	504552	18.54%	2.645%
22	16.400	1293	1296	1301	rVB3	16302	37519	1.38%	0.197%
23	17.097	1352	1357	1362	rBV3	12880	39666	1.46%	0.208%
24	17.943	1427	1431	1439	rVB2	12164	39684	1.46%	0.208%
25	18.994	1519	1523	1528	rVB6	7805	28091	1.03%	0.147%


Sum of corrected areas: 19077365

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062316\
Data File : BF088304.D
Acq On : 23 Jun 2016 22:40
Operator : UM/SJ
Sample : H3607-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TE-PMW-43

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

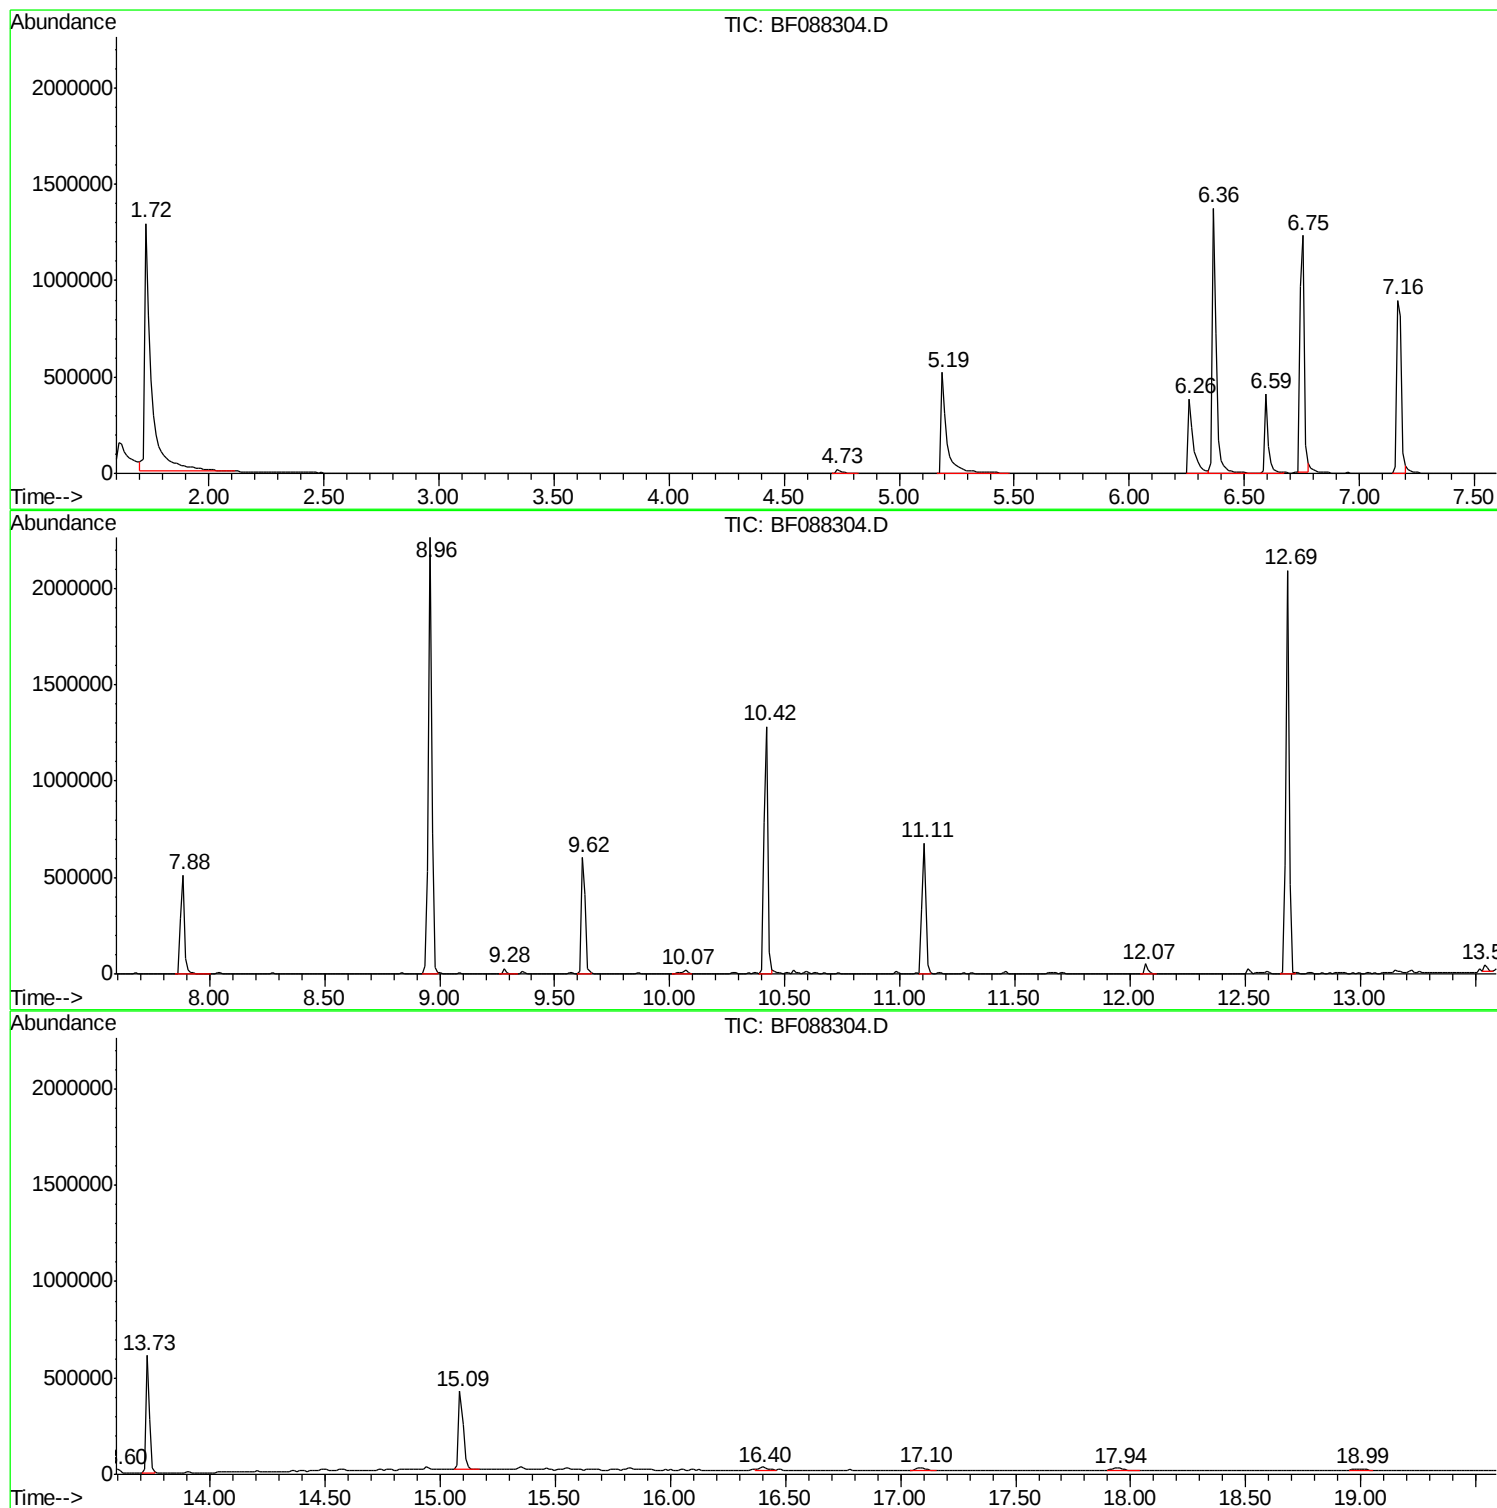

DbaaaPathh::ZZ\NRPBHHM1BBAFNDATA\BBO002366\
 DbaaaFile::BB0088004DD
 Aeqq00n ::23Jun2006 222400
 Oppaaaor ::UMMSJ
 Sample ::HB007009
 Misc ::
 ASSVaal ::122 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 TE-PMW-43

QqaantMebbdd::ZZ\NRPBHHM1BBAFMEH#00S82Z00BB000716MM
 QqaantTitle ::ASBPBNASSANDABBSF00R55P000NTC6AIBBATION

TICCLibbaay ::CC\DaababbaeN0\$SI11LL
 TICInteggaafionPaaameess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
