


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF062316\
 Data File : BF088294.D
 Acq On : 23 Jun 2016 16:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 01:47:17 2016

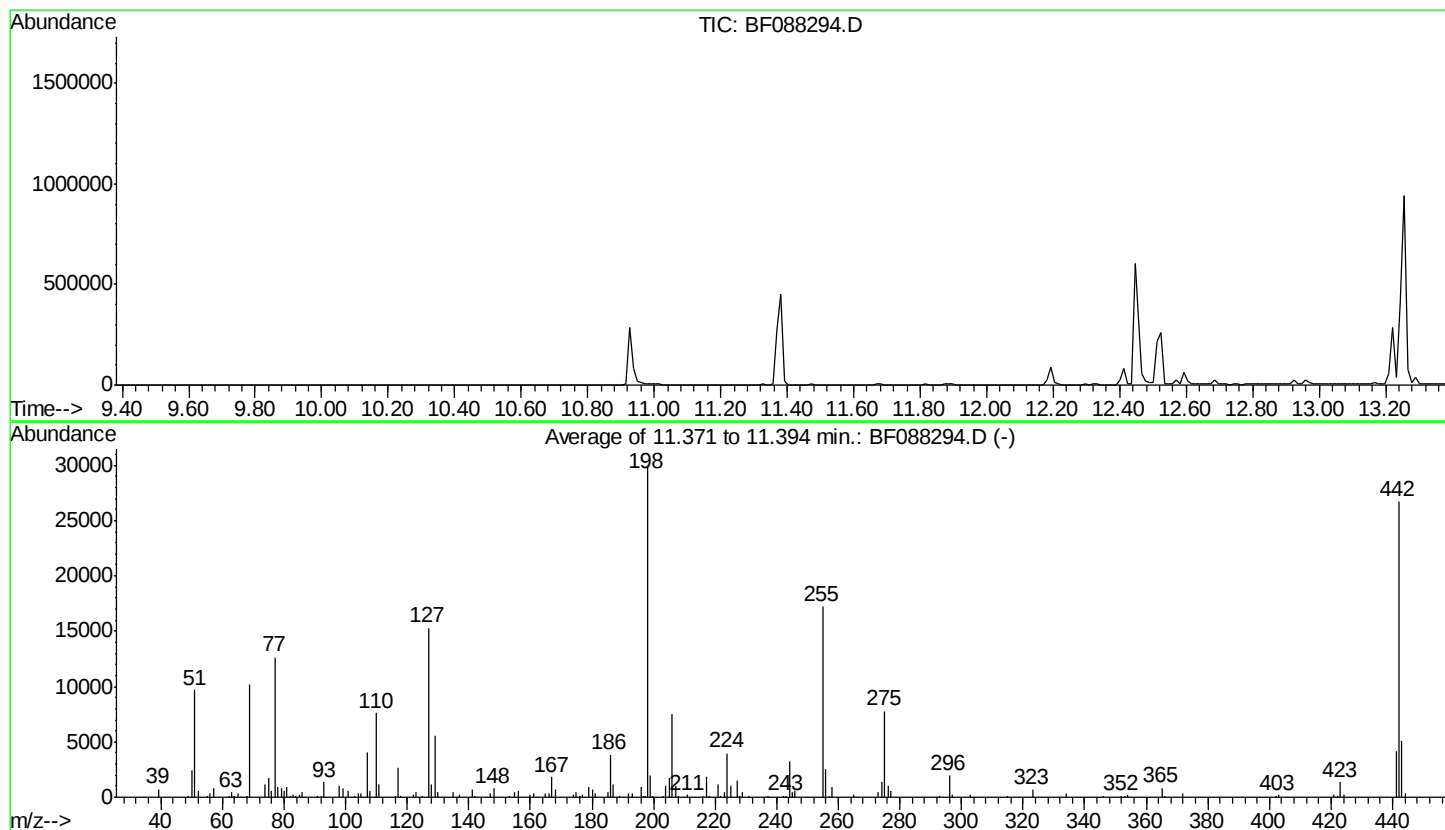

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	9712	PASS
68	69	0.00	2	1.4	147	PASS
69	198	0.00	100	34.1	10233	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.1	15307	PASS
197	198	0.00	2	0.4	122	PASS
198	198	100	100	100.0	29966	PASS
199	198	5	9	6.6	1974	PASS
275	198	10	60	26.0	7794	PASS
365	198	1	100	2.8	842	PASS
441	442	0.01	24	15.6	4177	PASS
442	198	50	100	89.1	26704	PASS
443	442	15	24	18.9	5050	PASS