


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF062316\  
 Data File : BF088294.D  
 Acq On : 23 Jun 2016 16:49  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF060716.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jun 22 14:55:14 2016

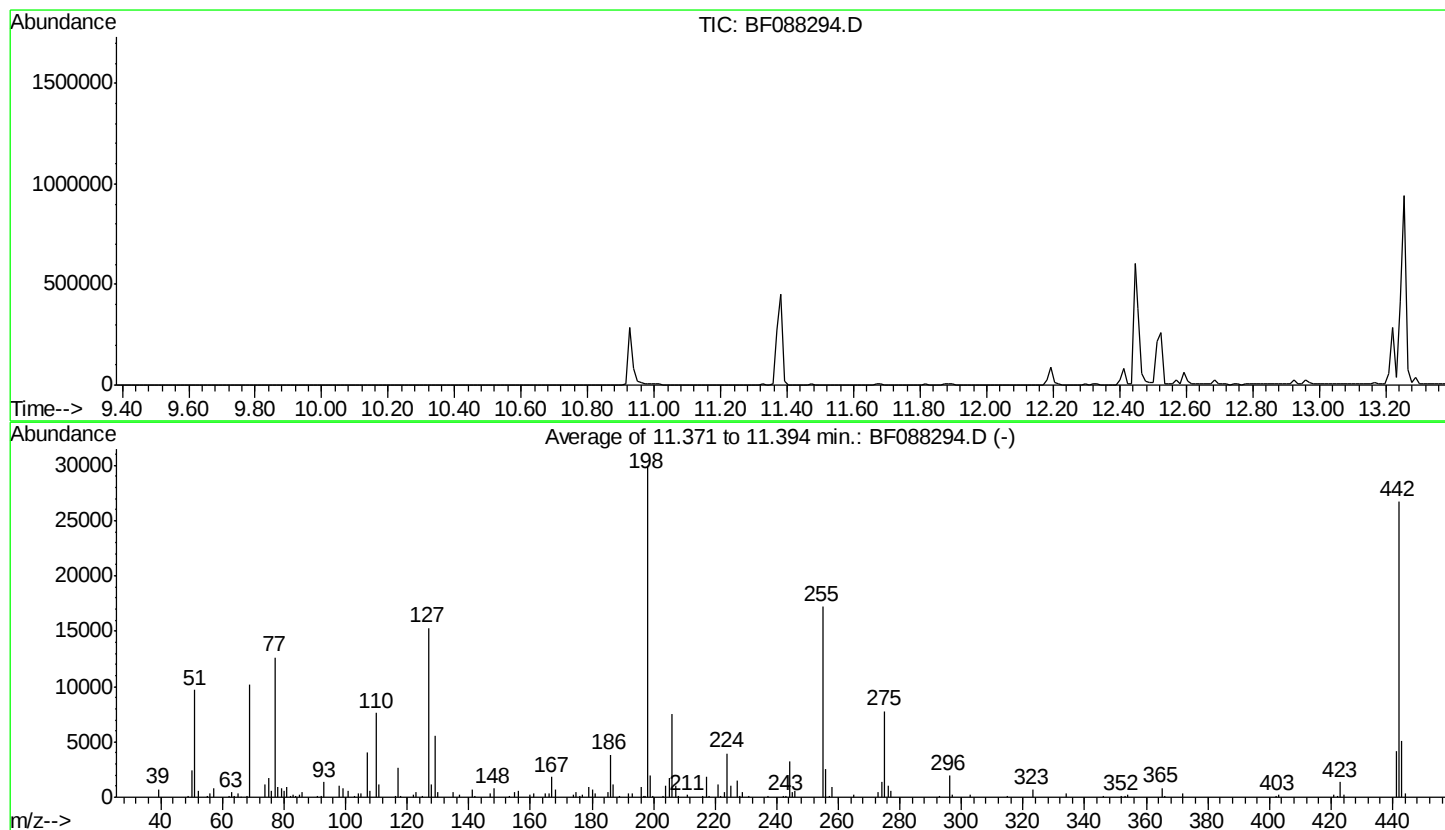

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 853

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 32.4      | 9712    | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 147     | PASS             |
| 69          | 198          | 0.00         | 100          | 34.1      | 10233   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 51.1      | 15307   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 122     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 29966   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 1974    | PASS             |
| 275         | 198          | 10           | 60           | 26.0      | 7794    | PASS             |
| 365         | 198          | 1            | 100          | 2.8       | 842     | PASS             |
| 441         | 442          | 0.01         | 24           | 15.6      | 4177    | PASS             |
| 442         | 198          | 50           | 100          | 89.1      | 26704   | PASS             |
| 443         | 442          | 15           | 24           | 18.9      | 5050    | PASS             |